

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014487.D
 Acq On : 03 Feb 2020 16:22
 Operator : SY/MD
 Sample : L1326-03 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBCS5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	66	72	85	rVB	203448	198467	10.21%	1.486%
2	1.582	147	153	166	rVB	118382	139405	7.17%	1.044%
3	2.010	282	286	289	rBV5	1453	1246	0.06%	0.009%
4	2.129	314	323	335	rBV	237727	342139	17.60%	2.561%
5	2.727	507	509	514	rVB2	829	445	0.02%	0.003%
6	2.746	514	515	519	rVB2	404	206	0.01%	0.002%
7	2.936	572	574	576	rBV2	587	319	0.02%	0.002%
8	2.949	576	578	584	rVB	718	627	0.03%	0.005%
9	3.036	600	605	609	rBV6	737	709	0.04%	0.005%
10	3.055	609	611	614	rVB2	535	238	0.01%	0.002%
11	3.100	622	625	628	rBV4	640	311	0.02%	0.002%
12	3.177	646	649	650	rBV2	418	201	0.01%	0.002%
13	3.203	655	657	662	rVB4	551	339	0.02%	0.003%
14	3.245	668	670	673	rVB2	642	287	0.01%	0.002%
15	3.293	683	685	688	rBV2	539	417	0.02%	0.003%
16	3.360	700	706	708	rBV4	573	492	0.03%	0.004%
17	3.457	733	736	737	rBV	414	239	0.01%	0.002%
18	3.479	741	743	748	rVV3	459	351	0.02%	0.003%
19	3.595	776	779	781	rVB	741	445	0.02%	0.003%
20	3.640	790	793	796	rBV2	588	379	0.02%	0.003%
21	3.679	804	805	809	rBV2	523	386	0.02%	0.003%
22	3.717	814	817	822	rVV4	465	515	0.03%	0.004%
23	3.753	826	828	830	rBV	506	213	0.01%	0.002%
24	3.830	848	852	853	rBV2	534	305	0.02%	0.002%
25	3.878	864	867	870	rBV3	660	541	0.03%	0.004%
26	3.926	870	882	888	rBV	113372	250991	12.91%	1.879%
27	4.399	1012	1029	1054	rBV	244007	609627	31.36%	4.563%
28	4.836	1163	1165	1167	rBV2	435	208	0.01%	0.002%
29	4.872	1171	1176	1177	rBV3	739	619	0.03%	0.005%
30	4.984	1209	1211	1214	rVB2	487	251	0.01%	0.002%
31	5.000	1214	1216	1221	rVB2	612	381	0.02%	0.003%
32	5.094	1224	1245	1285	rBV2	593562	1520780	78.23%	11.384%
33	5.405	1340	1342	1346	rVB4	684	385	0.02%	0.003%
34	5.537	1381	1383	1387	rBV2	568	511	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014487.D
 Acq On : 03 Feb 2020 16:22
 Operator : SY/MD
 Sample : L1326-03 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBCS5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis

35	5.659	1408	1421	1455	rBV	458541	914584	47.04%	6.846%
36	5.839	1474	1477	1480	rBV3	697	568	0.03%	0.004%
37	5.891	1490	1493	1494	rBV3	501	236	0.01%	0.002%
38	5.958	1502	1514	1533	rBV2	64076	128634	6.62%	0.963%
39	6.113	1547	1562	1590	rBV	334282	678400	34.90%	5.078%
40	6.405	1651	1653	1655	rBV3	666	364	0.02%	0.003%
41	6.466	1669	1672	1674	rBV	671	276	0.01%	0.002%
42	6.540	1691	1695	1698	rBV3	726	426	0.02%	0.003%
43	6.663	1731	1733	1736	rBV2	344	244	0.01%	0.002%
44	6.682	1736	1739	1740	rVV2	558	360	0.02%	0.003%
45	6.698	1742	1744	1749	rVB3	470	373	0.02%	0.003%
46	6.753	1758	1761	1764	rBV2	456	279	0.01%	0.002%
47	6.772	1764	1767	1770	rVB	425	256	0.01%	0.002%
48	6.849	1788	1791	1793	rBV	422	208	0.01%	0.002%
49	6.888	1798	1803	1805	rBV2	634	359	0.02%	0.003%
50	6.955	1822	1824	1828	rBV3	319	244	0.01%	0.002%
51	7.026	1832	1846	1868	rBV	205623	370061	19.04%	2.770%
52	7.235	1905	1911	1914	rBV5	832	748	0.04%	0.006%
53	7.357	1936	1949	1984	rBV	726059	1266839	65.16%	9.483%
54	7.659	2032	2043	2065	rBV	148488	253545	13.04%	1.898%
55	7.884	2104	2113	2123	rBV7	3746	6178	0.32%	0.046%
56	8.016	2140	2154	2170	rBV	1167681	1944069	100.00%	14.553%
57	8.129	2178	2189	2215	rBV	322870	681096	35.03%	5.098%
58	8.360	2259	2261	2262	rBV2	798	242	0.01%	0.002%
59	8.614	2338	2340	2345	rBV3	606	434	0.02%	0.003%
60	8.650	2347	2351	2353	rBV3	811	850	0.04%	0.006%
61	8.691	2360	2364	2366	rBV3	548	416	0.02%	0.003%
62	8.746	2378	2381	2386	rVB4	961	812	0.04%	0.006%
63	8.781	2386	2392	2394	rBV2	368	336	0.02%	0.003%
64	8.891	2414	2426	2455	rBV	672247	1095550	56.35%	8.201%
65	9.097	2487	2490	2491	rBV2	471	245	0.01%	0.002%
66	9.180	2508	2516	2523	rBV7	1880	3454	0.18%	0.026%
67	9.225	2527	2530	2534	rVV2	453	408	0.02%	0.003%
68	9.244	2534	2536	2539	rVB2	620	281	0.01%	0.002%
69	9.273	2539	2545	2547	rBV3	706	530	0.03%	0.004%
70	9.341	2563	2566	2569	rBV3	580	357	0.02%	0.003%
71	9.486	2608	2611	2613	rBV	353	236	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014487.D
 Acq On : 03 Feb 2020 16:22
 Operator : SY/MD
 Sample : L1326-03 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBCS5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis

72	9.498	2613	2615	2616	rVV2	643	264	0.01%	0.002%
73	9.569	2632	2637	2638	rBV	755	401	0.02%	0.003%
74	9.707	2678	2680	2682	rBV	704	252	0.01%	0.002%
75	9.759	2694	2696	2698	rBV2	530	216	0.01%	0.002%
76	9.810	2710	2712	2714	rBV	532	265	0.01%	0.002%
77	9.826	2714	2717	2719	rVV3	640	506	0.03%	0.004%
78	9.933	2747	2750	2752	rBV3	470	278	0.01%	0.002%
79	10.052	2785	2787	2789	rBV2	541	263	0.01%	0.002%
80	10.109	2801	2805	2808	rBV3	629	346	0.02%	0.003%
81	10.148	2812	2817	2819	rBV3	415	374	0.02%	0.003%
82	10.254	2837	2850	2874	rBV	434582	693484	35.67%	5.191%
83	10.460	2911	2914	2915	rBV	450	246	0.01%	0.002%
84	10.498	2923	2926	2928	rBV2	498	289	0.01%	0.002%
85	10.576	2946	2950	2952	rBV2	1069	855	0.04%	0.006%
86	10.588	2952	2954	2957	rVB	1018	487	0.03%	0.004%
87	10.679	2980	2982	2984	rBV3	463	229	0.01%	0.002%
88	10.810	3020	3023	3027	rBV3	478	412	0.02%	0.003%
89	10.836	3029	3031	3034	rBV2	611	320	0.02%	0.002%
90	10.910	3044	3054	3063	rBV5	18337	29143	1.50%	0.218%
91	11.051	3096	3098	3103	rBV2	528	423	0.02%	0.003%
92	11.119	3117	3119	3121	rVB2	849	312	0.02%	0.002%
93	11.170	3130	3135	3138	rVB2	588	485	0.02%	0.004%
94	11.193	3140	3142	3146	rBV3	369	275	0.01%	0.002%
95	11.289	3160	3172	3191	rBV	701171	1087562	55.94%	8.141%
96	11.547	3248	3252	3256	rBV2	710	778	0.04%	0.006%
97	11.666	3275	3289	3312	rBV	693343	1091648	56.15%	8.172%
98	12.061	3410	3412	3416	rBV2	481	361	0.02%	0.003%
99	12.373	3506	3509	3511	rBV4	556	388	0.02%	0.003%
100	13.550	3868	3875	3889	rBV	13689	22512	1.16%	0.169%


Sum of corrected areas: 13358847

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020320\
Data File : VV014487.D
Acq On : 03 Feb 2020 16:22
Operator : SY/MD
Sample : L1326-03 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBCS5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

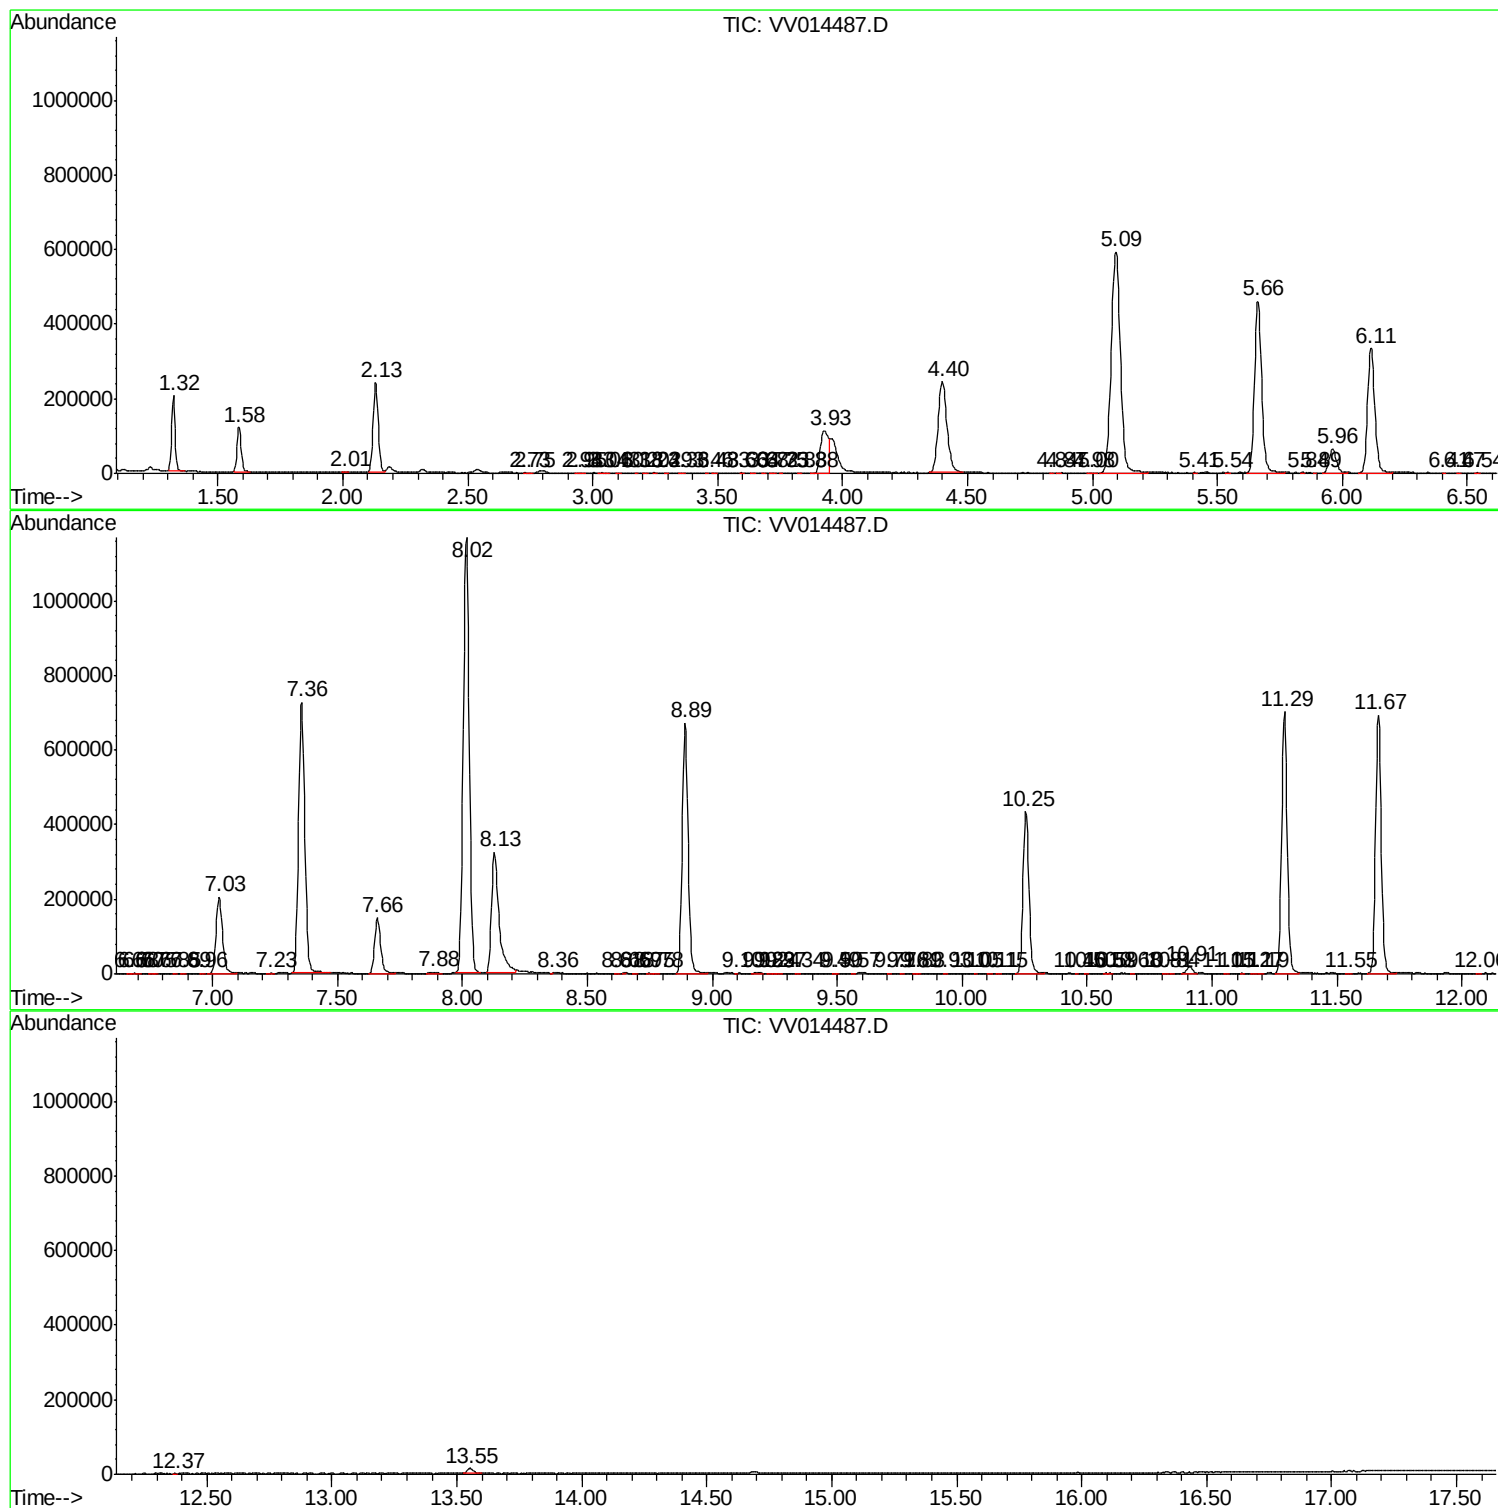

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV020320\
Data File : VV014487.D
Acq On : 03 Feb 2020 16:22
Operator : SY/MD
Sample : L1326-03 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBCS5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV020320\
Data File : VV014487.D
Acq On : 03 Feb 2020 16:22
Operator : SY/MD
Sample : L1326-03 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBCS5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
