


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020320\
 Data File : VV014479.D
 Acq On : 03 Feb 2020 09:33
 Operator : SY/MD
 Sample : BFB85
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB85

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 05 00:35:12 2020

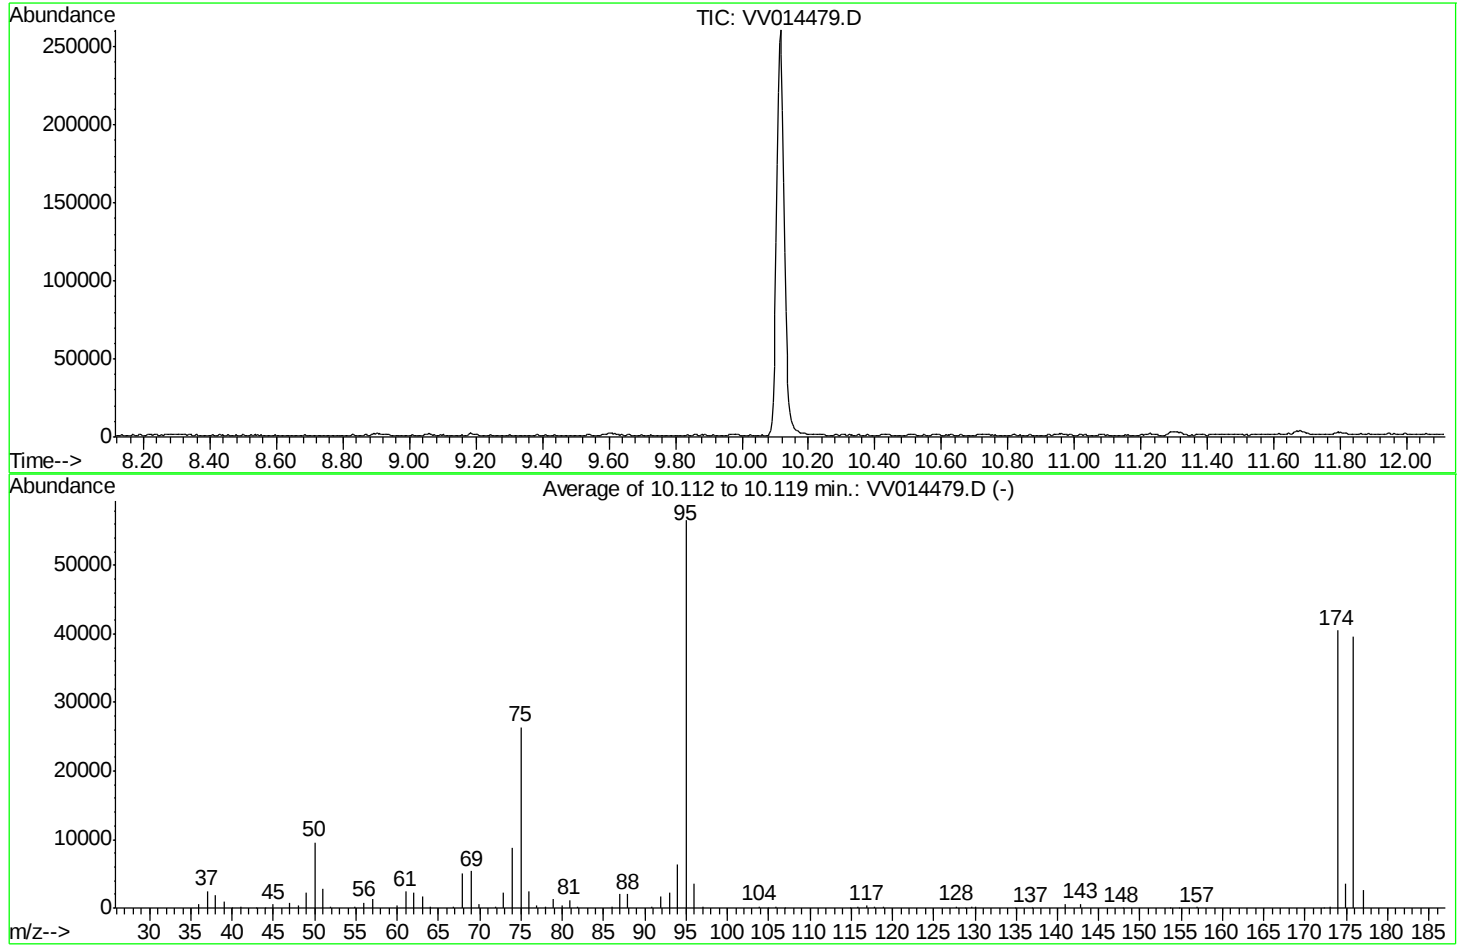

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	9606	PASS
75	95	30	80	46.6	26400	PASS
95	95	100	100	100.0	56592	PASS
96	95	5	9	6.3	3575	PASS
173	174	0.00	2	0.5	189	PASS
174	95	50	120	71.6	40498	PASS
175	174	5	9	8.7	3534	PASS
176	174	95	101	98.0	39680	PASS
177	176	5	9	6.4	2545	PASS

Scan 2794 (10.074 min): VV014479.D
BFB85

m/z	Abundance
39.90	367.0
43.10	112.0
43.90	545.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	643.0
37.00	2674.0
38.00	2025.0
39.00	886.0
39.90	403.0
40.90	107.0
42.90	175.0
44.00	637.0
45.00	544.0
47.00	673.0
48.00	388.0
49.00	2154.0
50.00	9472.0
51.00	2980.0
51.90	175.0
54.90	259.0
56.00	710.0
56.90	1203.0
60.00	404.0
61.00	2457.0
61.90	2290.0
63.00	1721.0
64.00	215.0
66.80	161.0
68.00	5101.0
69.00	5537.0
69.90	497.0
71.90	276.0
72.90	2296.0
74.00	8887.0
75.00	26688.0
76.00	2514.0
76.90	343.0
77.90	280.0
78.90	1321.0
79.90	456.0
80.90	1291.0
81.90	290.0
86.00	146.0
87.00	2091.0
87.90	2181.0
90.90	190.0
91.90	1717.0
93.00	2215.0
94.00	6060.0
95.00	56792.0
96.00	3656.0
97.10	152.0
103.90	272.0
104.90	115.0
105.90	212.0
107.00	115.0
114.90	109.0
115.80	209.0
116.90	279.0
117.80	189.0
118.80	233.0
127.80	269.0
128.90	115.0
129.60	155.0
130.00	159.0
134.90	108.0
136.80	115.0
140.90	457.0
142.80	520.0
147.90	122.0
154.80	106.0
157.00	149.0
172.20	137.0
173.90	39536.0
175.00	3588.0
175.90	38640.0
177.00	2443.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	619.0
37.00	2590.0
38.00	1945.0
39.00	979.0
39.90	413.0
41.00	125.0
42.90	159.0
44.00	636.0
45.00	534.0
47.00	715.0
48.00	372.0
49.00	2282.0
50.00	9919.0
51.00	2885.0
52.00	157.0
54.90	275.0
55.90	774.0
57.00	1295.0
60.00	441.0
61.00	2502.0
61.90	2222.0
63.00	1723.0
64.00	190.0
66.80	187.0
68.00	5098.0
69.00	5596.0
70.00	511.0
72.00	304.0
72.90	2301.0
74.00	8994.0
75.00	27352.0
76.00	2549.0
76.90	375.0
77.90	257.0
78.90	1357.0
79.90	455.0
80.90	1225.0
81.90	288.0
86.00	159.0
87.00	2040.0
87.90	2127.0
90.90	225.0
91.90	1696.0
93.00	2357.0
94.00	6516.0
95.00	58656.0
96.00	3635.0
97.10	144.0
103.90	243.0
104.90	130.0
105.90	227.0
115.80	242.0
116.90	322.0
117.90	223.0
118.90	261.0
127.80	273.0
129.60	165.0
130.00	164.0
141.00	494.0
142.80	597.0
153.60	103.0
156.90	136.0
173.90	41896.0
175.00	3649.0
175.90	40928.0
177.00	2637.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
35.90	497.0
37.00	2318.0
38.00	1739.0
39.00	878.0
39.90	478.0
41.10	149.0
42.90	128.0
44.00	628.0
44.90	485.0
47.00	715.0
48.00	364.0
49.00	2111.0
50.00	9429.0
51.00	2674.0
52.00	141.0
54.90	233.0
55.90	794.0
57.00	1297.0
60.00	428.0
61.00	2247.0
62.00	1983.0
63.00	1616.0
64.00	200.0
66.90	206.0
67.90	4736.0
69.00	4981.0
70.00	501.0
72.00	275.0
72.90	2114.0
74.00	8421.0
75.00	25160.0
76.00	2412.0
76.90	351.0
77.90	184.0
78.90	1169.0
79.90	386.0
80.90	1084.0
81.90	281.0
86.10	110.0
86.90	1855.0
87.90	1840.0
90.90	232.0
91.90	1515.0
93.00	2220.0
94.00	6243.0
95.00	54328.0
96.00	3435.0
97.10	102.0
103.90	210.0
105.90	227.0
115.80	256.0
116.90	301.0
117.90	252.0
118.90	265.0
127.80	227.0
130.00	193.0
136.90	103.0
140.90	490.0
142.80	639.0
156.90	118.0
173.00	569.0
173.90	40064.0
174.90	3365.0
175.90	39472.0
177.00	2555.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85