
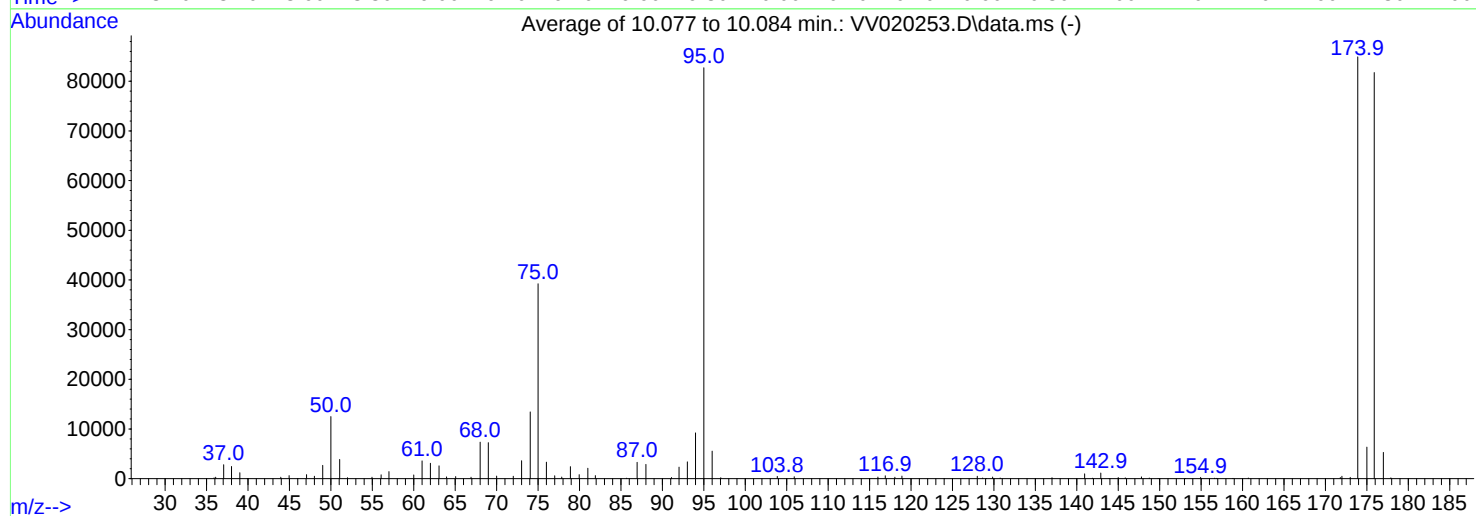


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020321\
 Data File : VV020253.D
 Acq On : 03 Feb 2021 11:11
 Operator : SY/MD
 Sample : BFB85
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB85

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020321WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 03 17:26:57 2021

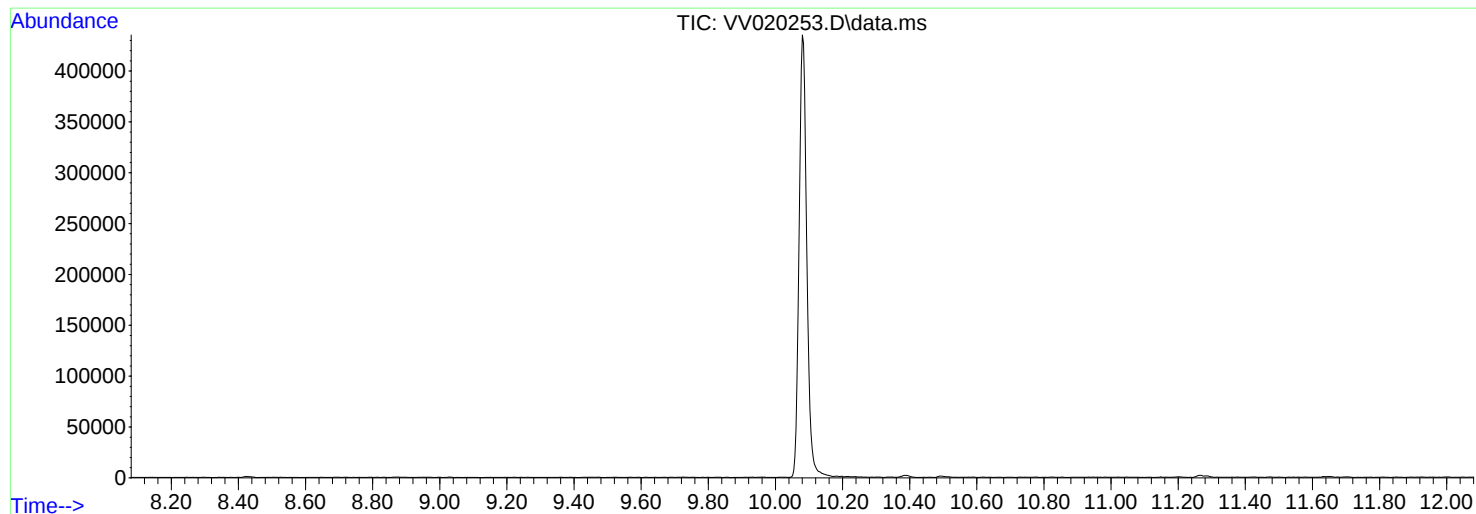

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	12504	PASS
75	95	30	80	47.4	39232	PASS
95	95	100	100	100.0	82709	PASS
96	95	5	9	6.7	5546	PASS
173	174	0.00	2	0.3	267	PASS
174	95	50	120	102.7	84915	PASS
175	174	5	9	7.5	6353	PASS
176	174	95	101	96.3	81768	PASS
177	176	5	9	6.5	5283	PASS

m/z	Abundance
35.90	466.0
37.10	2792.0
38.00	2314.0
39.00	1087.0
39.90	255.0
44.00	559.0
44.90	601.0
46.00	116.0
47.00	826.0
48.00	448.0
49.00	2495.0
50.00	12488.0
51.10	3584.0
52.00	219.0
54.90	240.0
56.00	628.0
57.00	1419.0
60.00	744.0
61.00	3544.0
62.00	2921.0
63.10	2621.0
64.00	318.0
65.00	353.0
66.90	233.0
68.00	7124.0
69.00	7139.0
70.00	475.0
72.00	470.0
73.00	3507.0
74.10	13336.0
75.00	38344.0
76.00	3215.0
77.10	584.0
77.80	313.0
78.90	2343.0
79.90	739.0
81.00	2062.0
81.90	590.0
87.00	3124.0
88.00	2700.0
91.10	227.0
92.00	2307.0
93.00	3377.0
94.00	8816.0
95.00	79120.0
96.00	5082.0
97.00	185.0
103.80	400.0
106.00	322.0
116.00	310.0
116.80	590.0
118.00	271.0
118.90	569.0
124.00	113.0
128.00	443.0
128.60	128.0
129.80	322.0
130.80	143.0
137.00	222.0
140.90	890.0
142.90	912.0
145.00	167.0
145.80	163.0
147.80	288.0
148.70	122.0
149.80	107.0
154.90	260.0
156.60	141.0
160.60	128.0
171.80	683.0
173.00	800.0
173.90	79680.0
175.00	6547.0
175.90	75544.0
177.00	5046.0
177.90	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.10	464.0
37.00	2848.0
38.00	2475.0
39.00	1248.0
39.90	260.0
44.00	618.0
45.00	631.0
47.10	800.0
48.00	524.0
49.00	2800.0
50.00	13056.0
51.00	3961.0
52.00	222.0
55.00	307.0
56.00	782.0
57.00	1465.0
60.00	756.0
61.00	3714.0
62.00	3157.0
63.10	2682.0
63.90	365.0
65.00	428.0
66.90	315.0
68.00	7597.0
69.00	7494.0
70.00	518.0
72.00	529.0
73.00	3761.0
74.10	13941.0
75.00	40592.0
76.00	3470.0
77.00	599.0
77.80	338.0
78.90	2502.0
79.90	837.0
81.00	2163.0
81.90	673.0
85.70	105.0
86.90	3445.0
88.00	2925.0
91.10	222.0
92.00	2367.0
93.00	3516.0
94.00	9401.0
95.00	85568.0
96.00	5832.0
97.00	200.0
103.80	459.0
105.90	396.0
116.00	355.0
116.90	597.0
118.10	285.0
118.90	512.0
128.00	499.0
128.60	142.0
129.90	307.0
130.80	139.0
137.00	219.0
141.00	988.0
141.90	151.0
142.90	1211.0
145.00	241.0
145.90	175.0
147.80	376.0
148.80	137.0
154.90	266.0
156.70	145.0
158.90	102.0
160.70	144.0
172.00	725.0
173.90	87800.0
175.00	6491.0
175.90	84408.0
177.00	5489.0
177.90	176.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.10	449.0
37.00	2795.0
38.00	2587.0
39.00	1243.0
39.90	214.0
44.00	712.0
45.00	579.0
47.10	780.0
48.00	520.0
49.00	2686.0
50.00	11968.0
51.00	4080.0
52.00	174.0
55.00	289.0
56.10	888.0
57.00	1368.0
60.00	713.0
61.00	3495.0
62.00	3169.0
63.00	2433.0
63.90	337.0
65.10	485.0
66.90	308.0
68.00	7313.0
69.00	7149.0
70.00	529.0
72.00	475.0
73.00	3551.0
74.00	13035.0
75.00	38760.0
76.00	3282.0
76.90	579.0
77.90	333.0
78.90	2366.0
80.00	826.0
81.00	2037.0
81.90	612.0
85.70	148.0
86.90	3329.0
88.00	2966.0
91.10	221.0
92.00	2261.0
93.00	3299.0
94.00	9406.0
95.00	83440.0
96.00	5725.0
97.10	204.0
103.90	477.0
105.80	419.0
116.00	306.0
117.00	567.0
118.10	285.0
118.90	484.0
128.00	473.0
128.70	127.0
129.10	127.0
129.90	298.0
130.70	129.0
137.00	187.0
140.90	1033.0
141.90	155.0
142.90	1305.0
143.90	106.0
145.00	263.0
145.90	163.0
147.80	403.0
148.80	105.0
153.10	107.0
155.00	237.0
156.90	173.0
158.80	135.0
160.80	160.0
172.00	783.0
173.90	87264.0
175.00	6021.0
175.90	85352.0
177.00	5313.0
177.90	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
39.90	228.0
43.90	332.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85