




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
 Data File : VV030037.D
 Acq On : 03 Feb 2023 15:30
 Operator : SY/MD
 Sample : 01393-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Manual IntegrationsAPPROVED

Quant Time: Feb 04 01:04:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 04 01:01:21 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

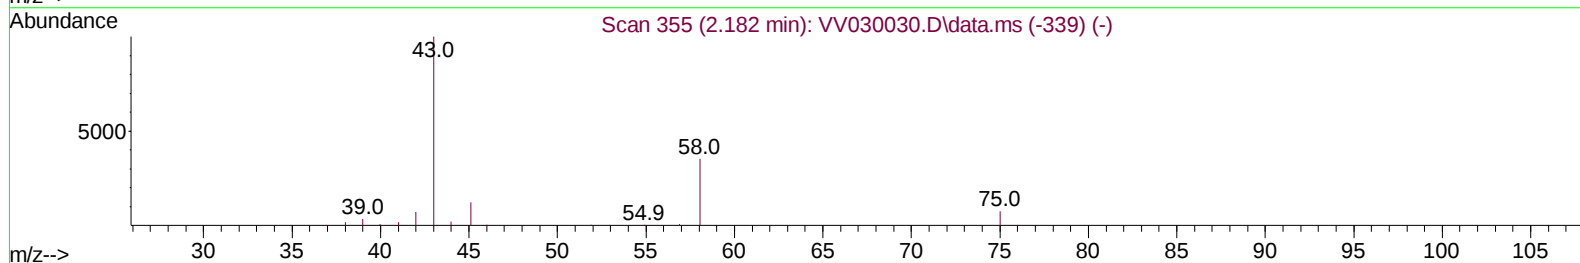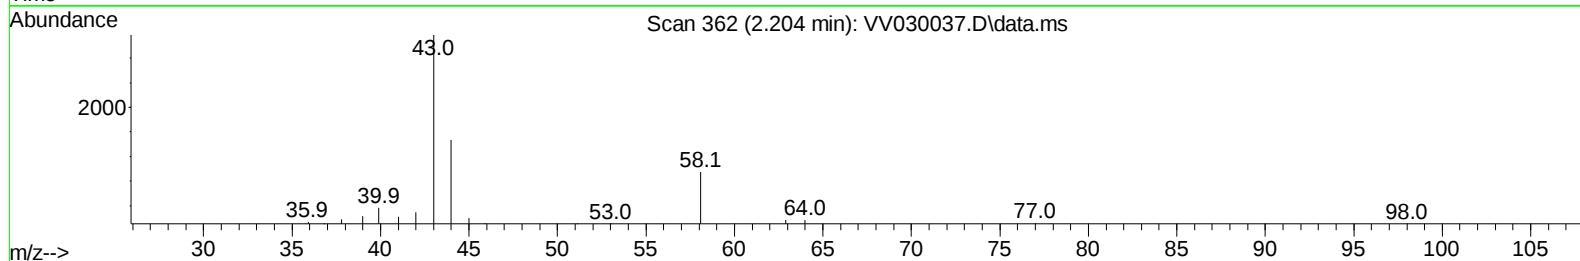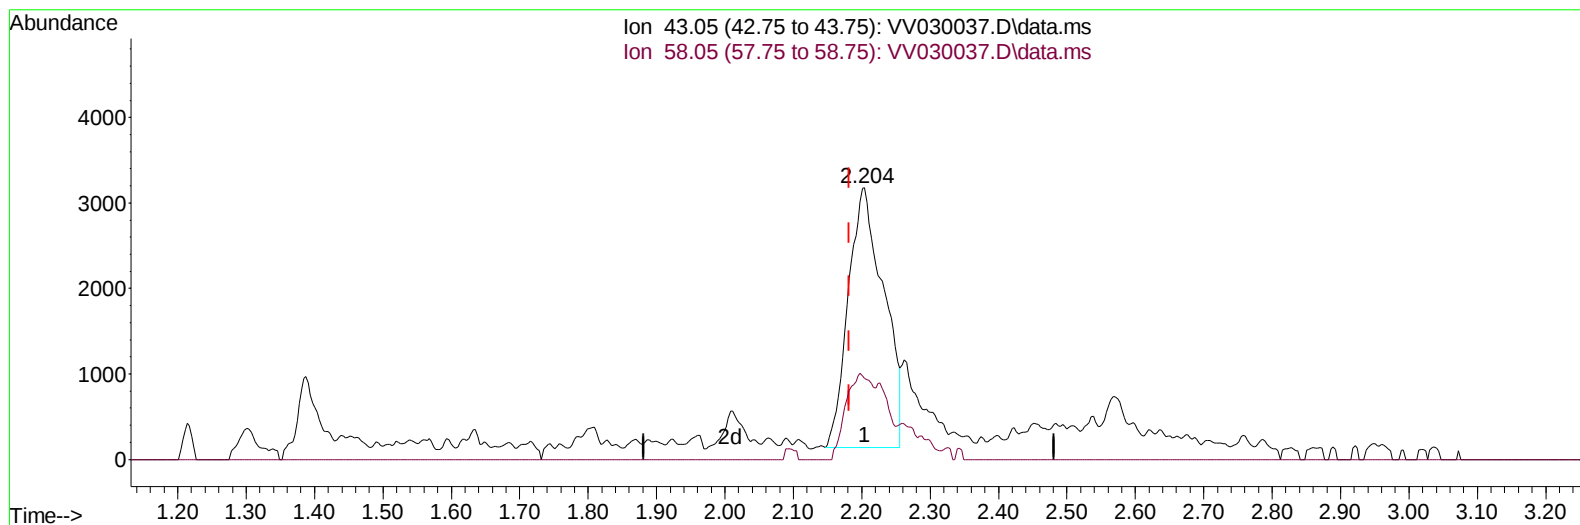

TIC: VV030037.D\data.ms

(13) Acetone (T)

2.204min (+ 0.023) 5.14 ug/L

response 10935

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	25.41
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
 Data File : VV030037.D
 Acq On : 03 Feb 2023 15:30
 Operator : SY/MD
 Sample : 01393-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

Quant Time: Feb 04 01:04:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 04 01:01:21 2023
 Response via : Initial Calibration

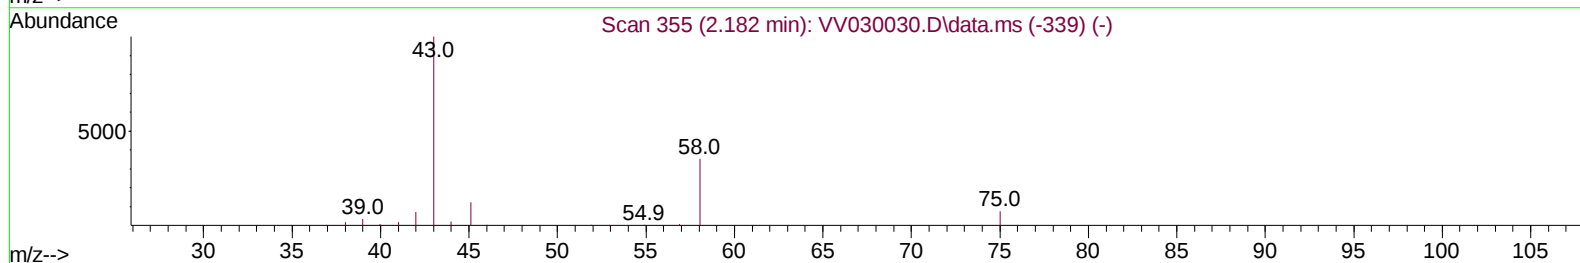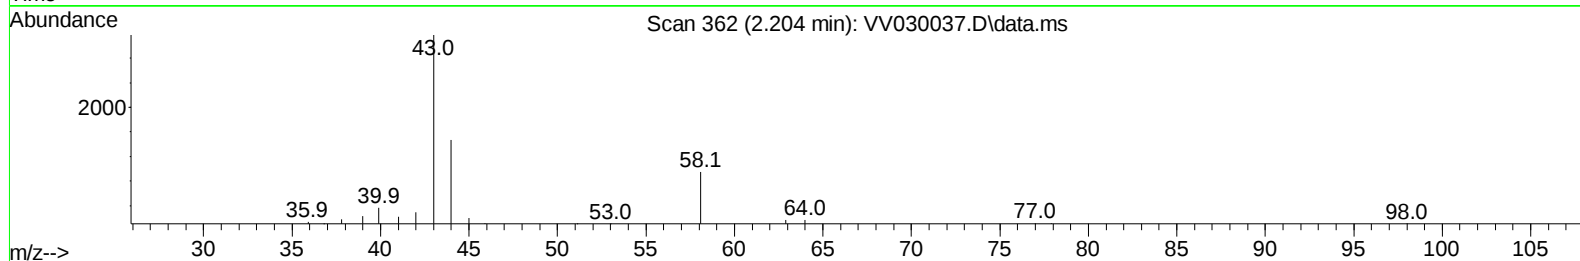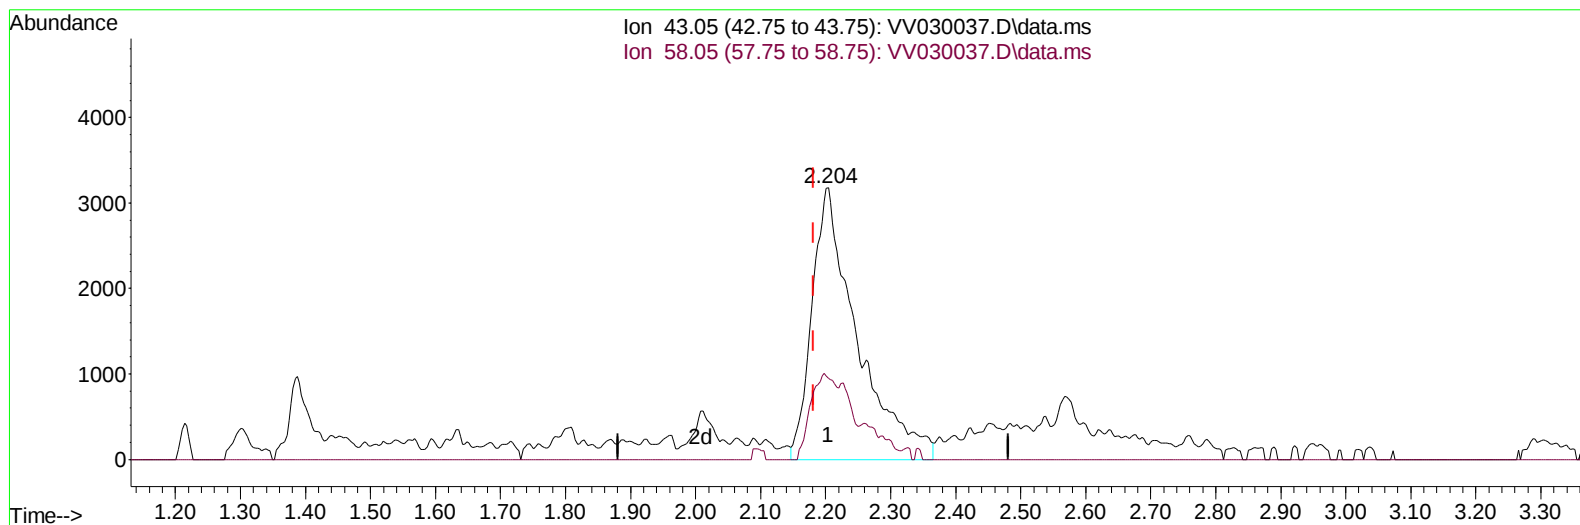

TIC: VV030037.D\data.ms

(13) Acetone (T)

2.204min (+ 0.023) 7.17 ug/L m

response 15263

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.40	18.21
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
 Data File : VV030037.D
 Acq On : 03 Feb 2023 15:30
 Operator : SY/MD
 Sample : 01393-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Manual IntegrationsAPPROVED

Quant Time: Feb 04 01:04:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 04 01:01:21 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.606	114		221925	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117		214184	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152		103323	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		76549	4.548	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.000%	
7) Chloroethane-d5	1.564	69		75775	5.431	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.600%	
11) 1,1-Dichloroethene-d2	2.101	63		108453	3.534	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.600%	
20) 2-Butanone-d5	3.905	46		163763	54.890	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.780%	
24) Chloroform-d	4.336	84		148545	4.811	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%	
26) 1,2-Dichloroethane-d4	5.024	65		65000	4.971	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%	
32) Benzene-d6	5.040	84		301622	4.747	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%	
36) 1,2-Dichloropropane-d6	6.059	67		101022	5.433	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.600%	
41) Toluene-d8	7.307	98		250597	4.260	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%	
43) trans-1,3-Dichloroprop...	7.612	79		31927	4.701	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.000%	
46) 2-Hexanone-d5	8.085	63		154094	55.737	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.480%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84		71613	5.256	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.200%	
66) 1,2-Dichlorobenzene-d4	11.612	152		95755	5.097	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%	
Target Compounds							
13) Acetone	2.204	43		15263m	7.168	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
Data File : VV030037.D
Acq On : 03 Feb 2023 15:30
Operator : SY/MD
Sample : 01393-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0B67

Manual IntegrationsAPPROVED

Quant Time: Feb 04 01:04:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 04 01:01:21 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 02/06/2023
Supervised By :Mahesh Dadoda 02/06/2023

