

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020323\
 Data File : VW030037.D
 Acq On : 03 Feb 2023 15:30
 Operator : SY/MD
 Sample : 01393-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

Quant Time: Feb 04 01:04:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Feb 04 01:01:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	221925	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.841	117	214184	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	103323	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	76549	4.548	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.000%
7) Chloroethane-d5	1.564	69	75775	5.431	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.600%
11) 1,1-Dichloroethene-d2	2.101	63	108453	3.534	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.600%
20) 2-Butanone-d5	3.905	46	163763	54.890	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.780%
24) Chloroform-d	4.336	84	148545	4.811	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.200%
26) 1,2-Dichloroethane-d4	5.024	65	65000	4.971	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.040	84	301622	4.747	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.000%
36) 1,2-Dichloropropane-d6	6.059	67	101022	5.433	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.600%
41) Toluene-d8	7.307	98	250597	4.260	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.200%
43) trans-1,3-Dichloroprop...	7.612	79	31927	4.701	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.000%
46) 2-Hexanone-d5	8.085	63	154094	55.737	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	111.480%
56) 1,1,2,2-Tetrachloroeth...	10.204	84	71613	5.256	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.200%
66) 1,2-Dichlorobenzene-d4	11.612	152	95755	5.097	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%
Target Compounds					Qvalue	
13) Acetone	2.204	43	15263m	7.168	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
Data File : VV030037.D
Acq On : 03 Feb 2023 15:30
Operator : SY/MD
Sample : 01393-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
C0B67

Quant Time: Feb 04 01:04:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Feb 04 01:01:21 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 02/06/2023
Supervised By :Mahesh Dadoda 02/06/2023

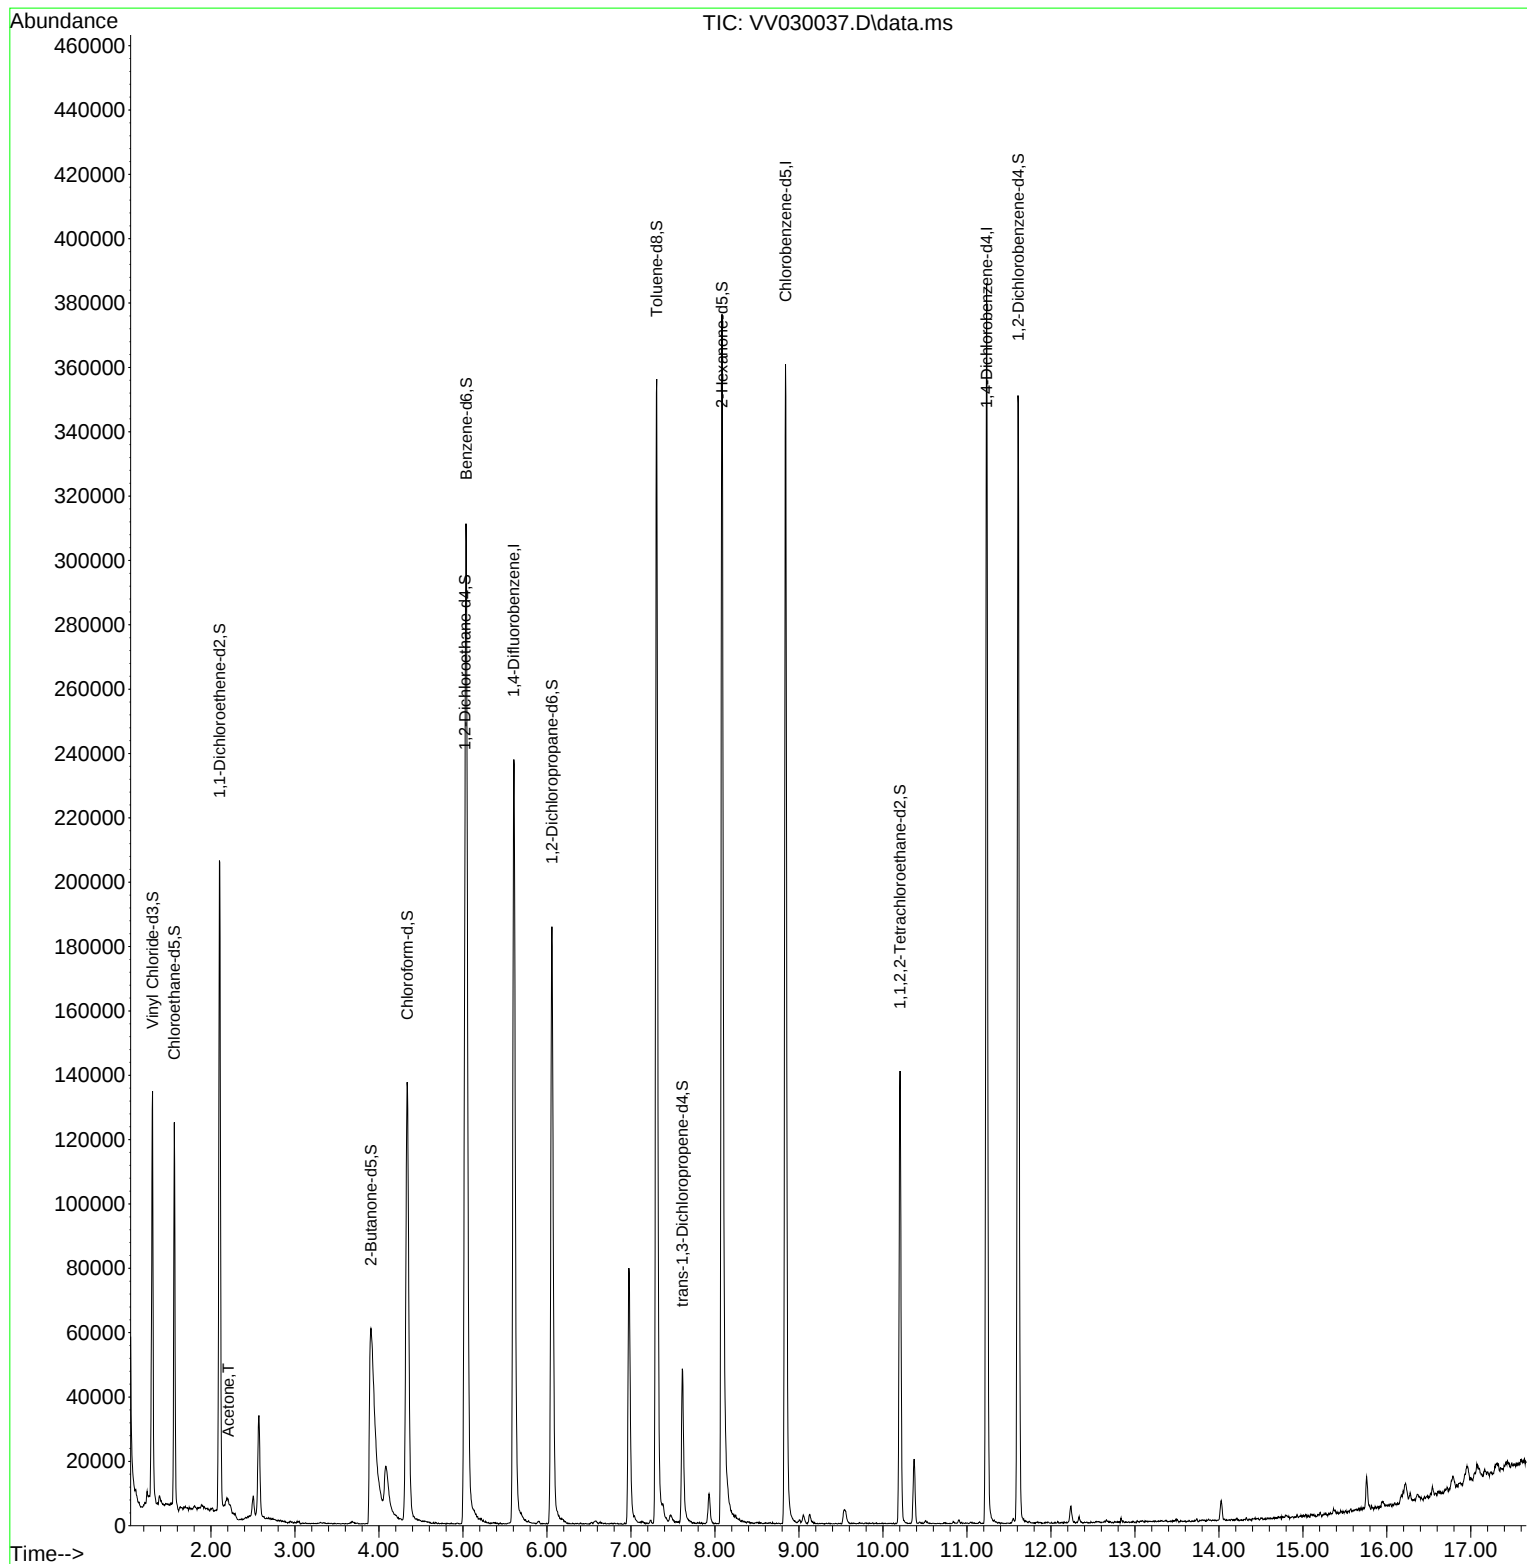

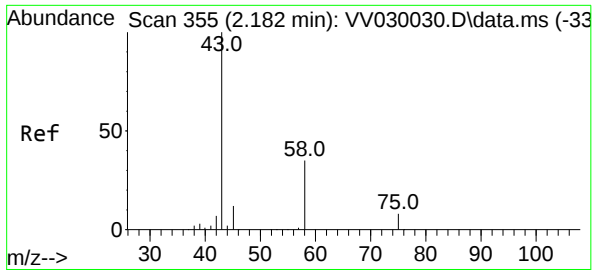

#13
 Acetone
 Concen: 7.168 ug/L m
 RT: 2.204 min Scan# 30
 Delta R.T. 0.023 min
 Lab File: VV030037.D
 Acq: 03 Feb 2023 15:30

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B67

Tgt Ion: 43 Resp: 1526
 Ion Ratio Lower Upper
 43 100
 58 18.2 0.0 68.8

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 02/06/2023
 Supervised By :Mahesh Dadoda 02/06/2023

