

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
 Data File : VV030031.D
 Acq On : 03 Feb 2023 10:28
 Operator : SY/MD
 Sample : VV0203WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK302

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	99	rVB	126127	138107	17.62%	2.174%
2	1.561	155	162	173	rVB	121577	136160	17.37%	2.144%
3	2.101	319	330	348	rBV	209285	295913	37.75%	4.658%
4	2.500	442	454	465	rBV3	8638	13674	1.74%	0.215%
5	3.889	874	886	925	rBV	74684	264878	33.79%	4.170%
6	4.336	1007	1025	1050	rBV	136175	341093	43.51%	5.370%
7	5.037	1220	1243	1277	rBV2	308446	783870	100.00%	12.340%
8	5.606	1406	1420	1443	rBV	239483	488629	62.34%	7.692%
9	6.059	1547	1561	1580	rBV	184677	381397	48.66%	6.004%
10	6.976	1834	1846	1877	rBV	80581	156479	19.96%	2.463%
11	7.304	1936	1948	1985	rBV	355933	647142	82.56%	10.188%
12	7.612	2033	2044	2069	rBV	48550	90248	11.51%	1.421%
13	8.082	2179	2190	2231	rBV	368713	685160	87.41%	10.786%
14	8.841	2414	2426	2455	rBV	363239	597322	76.20%	9.403%
15	10.204	2838	2850	2866	rBV	134543	208457	26.59%	3.282%
16	11.236	3159	3171	3189	rBV	374621	568687	72.55%	8.953%
17	11.609	3275	3287	3309	rBV	334678	531194	67.77%	8.362%
18	14.027	4025	4039	4051	rBV2	6134	10767	1.37%	0.170%
19	15.757	4570	4577	4584	rBV6	8386	12951	1.65%	0.204%




Sum of corrected areas: 6352128

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
Data File : VV030031.D
Acq On : 03 Feb 2023 10:28
Operator : SY/MD
Sample : VV0203WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

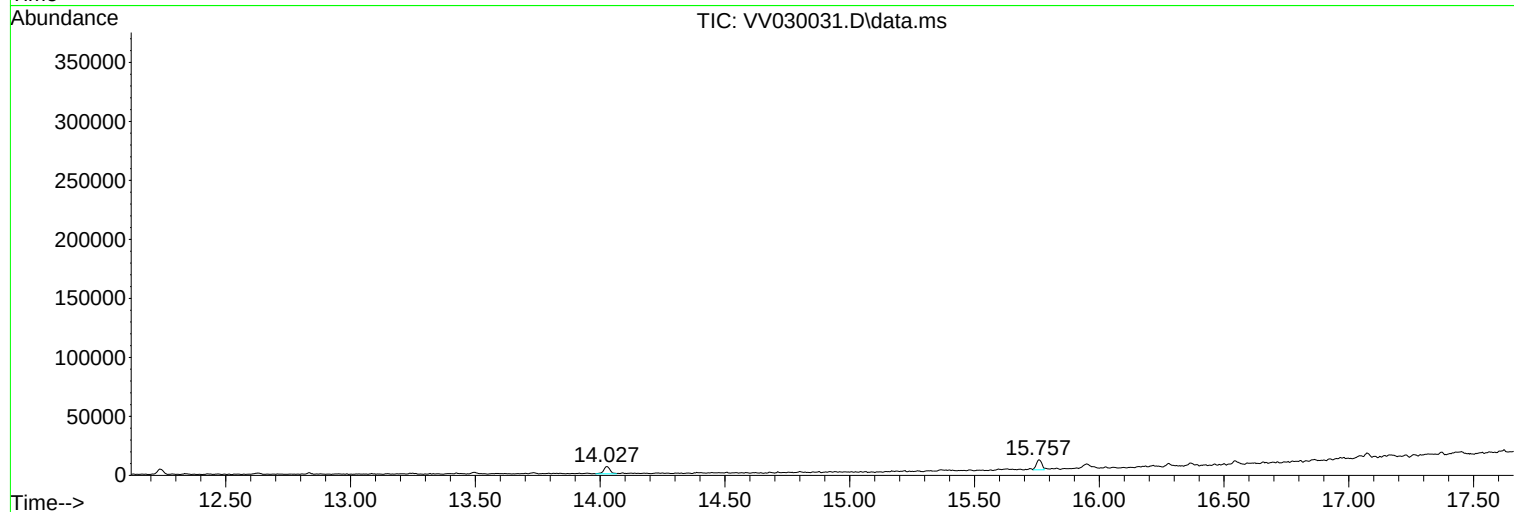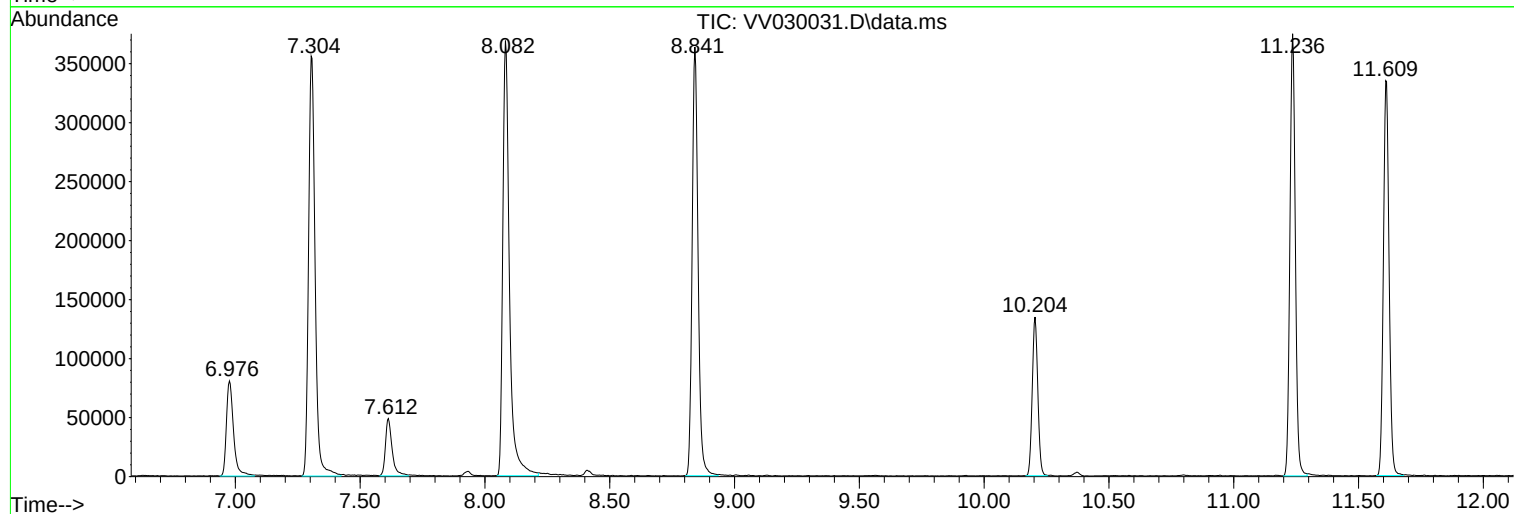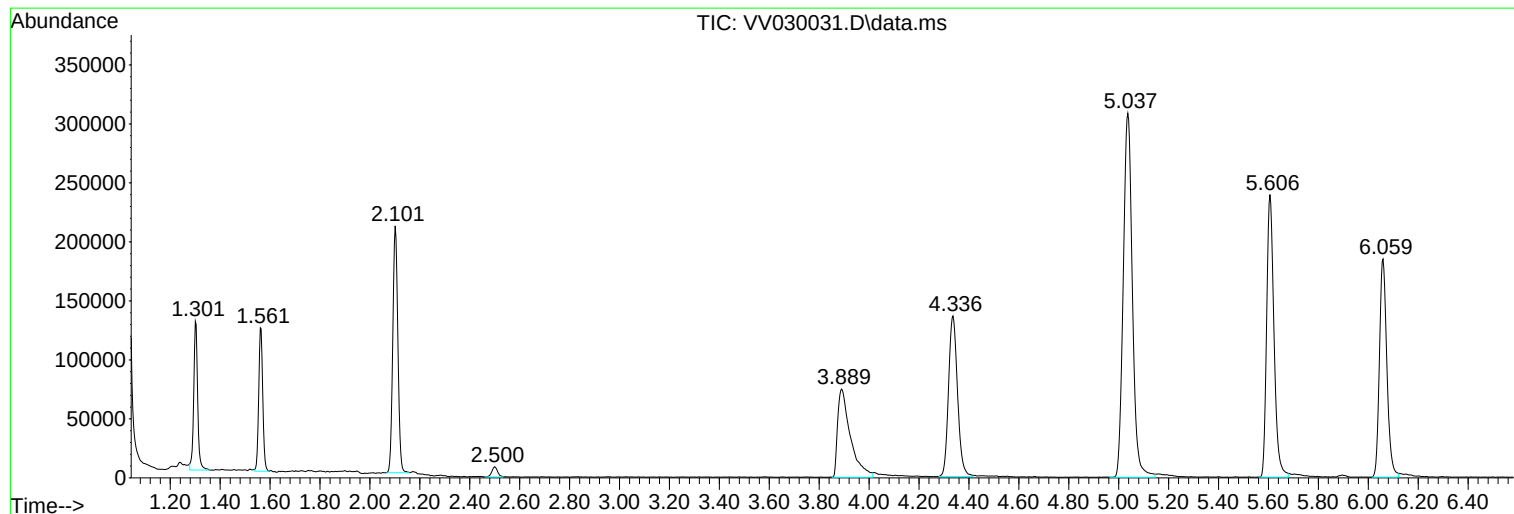

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
Data File : VV030031.D
Acq On : 03 Feb 2023 10:28
Operator : SY/MD
Sample : VV0203WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
Data File : VV030031.D
Acq On : 03 Feb 2023 10:28
Operator : SY/MD
Sample : VV0203WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK302

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------