
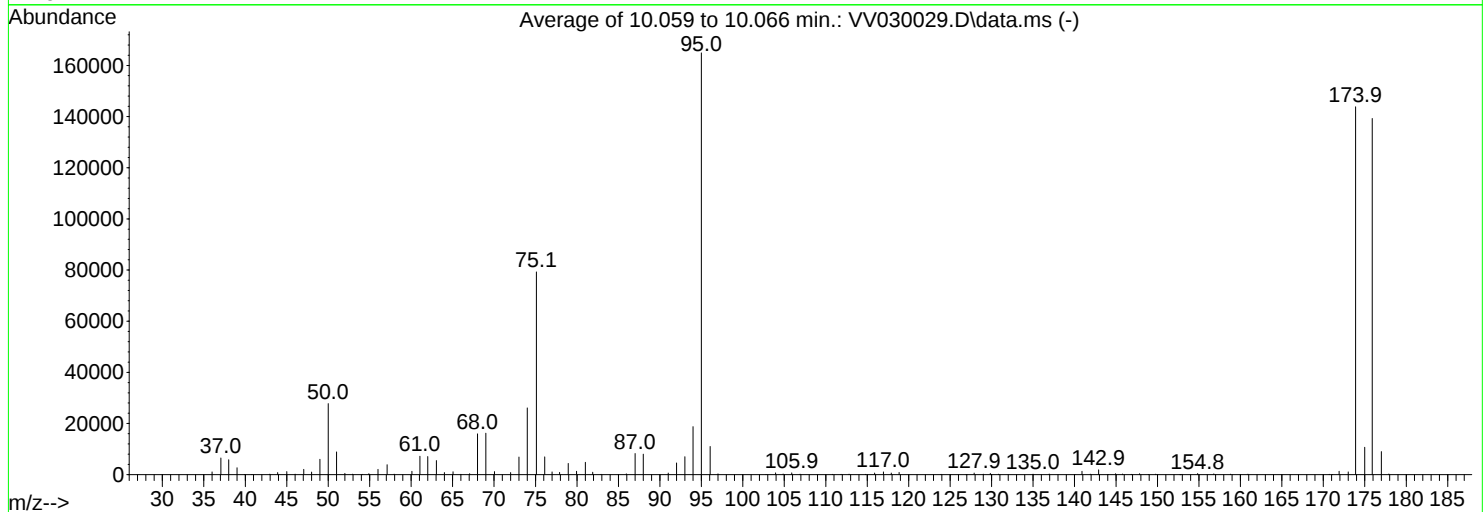


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020323\
Data File : VV030029.D
Acq On : 03 Feb 2023 09:07
Operator : SY/MD
Sample : BFB221
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB221

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR011223WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Feb 06 00:35:05 2023

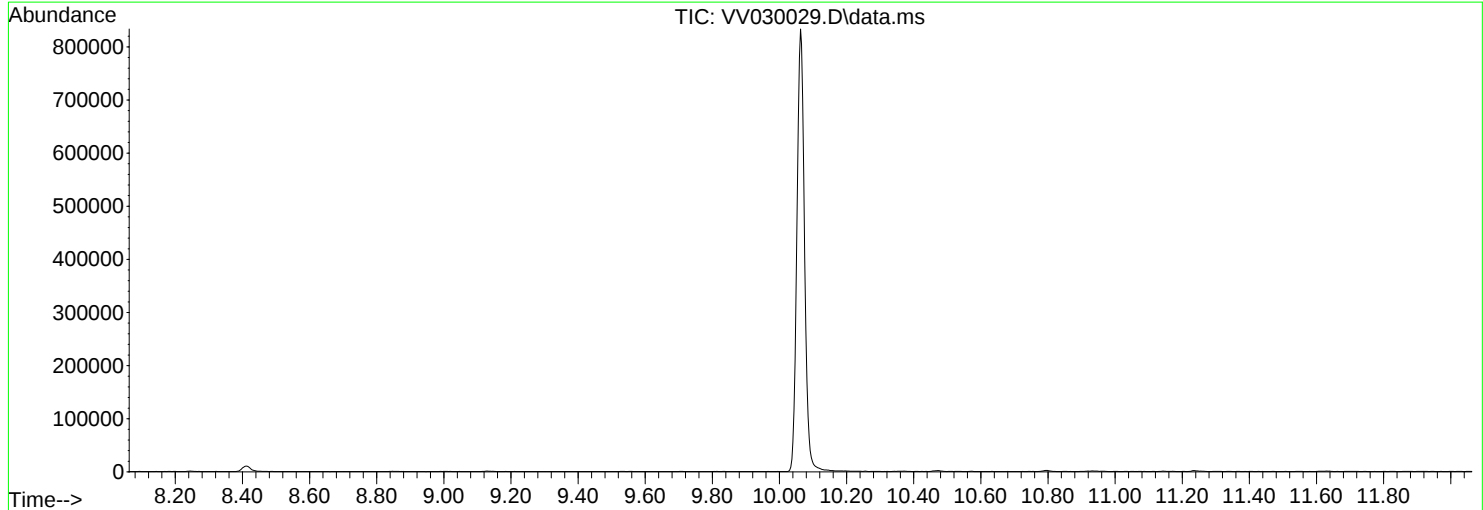

AutoFind: Scans 2805, 2806, 2807; Background Corrected with Scan 2792

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	27768	PASS
75	95	30	80	48.1	79256	PASS
95	95	100	100	100.0	164928	PASS
96	95	5	9	6.7	11010	PASS
173	174	0.00	2	0.7	1058	PASS
174	95	50	120	87.2	143808	PASS
175	174	5	9	7.4	10675	PASS
176	174	95	105	96.8	139243	PASS
177	176	5	10	6.5	9035	PASS

m/z	Abundance
39.90	179.0
43.90	475.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	1086.0
37.00	6334.0
38.00	5953.0
39.00	2590.0
39.90	222.0
42.90	129.0
43.90	1201.0
45.00	1175.0
45.90	234.0
47.00	2098.0
48.00	991.0
49.00	5827.0
50.00	27168.0
51.00	8790.0
52.00	422.0
52.90	199.0
54.10	107.0
54.90	364.0
56.00	2130.0
57.10	3807.0
57.90	207.0
60.10	1392.0
61.10	7033.0
62.00	7209.0
63.00	5446.0
64.00	751.0
65.10	1162.0
66.00	170.0
67.00	411.0
68.00	15446.0
69.00	15504.0
70.10	1235.0
72.00	739.0
73.00	6593.0
74.00	25576.0
75.10	77144.0
76.10	7050.0
77.00	1046.0
77.90	851.0
78.90	4283.0
80.00	1261.0
81.00	4725.0
81.90	881.0
82.90	126.0
85.90	336.0
87.00	8088.0
88.00	8090.0
91.00	695.0
92.00	4476.0
93.00	6928.0
94.00	18280.0
95.00	159808.0
96.10	11029.0
97.00	344.0
102.80	119.0
104.00	667.0
104.80	245.0
105.90	614.0
106.90	182.0
110.80	105.0
112.80	159.0
114.80	160.0
115.90	586.0
116.90	1007.0
117.90	516.0
118.90	881.0
123.90	130.0
127.90	607.0
129.00	245.0
129.80	565.0
130.80	248.0
135.00	225.0
137.00	261.0
140.10	102.0
140.90	1250.0
141.90	156.0
142.90	1821.0
145.00	384.0
145.80	235.0
146.80	114.0
147.90	392.0
149.80	153.0
153.00	161.0
154.80	400.0
156.80	261.0
158.80	186.0
160.90	176.0
170.70	159.0
171.10	189.0
171.90	1175.0
173.90	137728.0
175.00	10446.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

175.90132480.0

177.008770.0

177.90233.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	1133.0
37.00	6705.0
38.00	5990.0
39.00	2774.0
39.90	234.0
40.80	111.0
42.90	174.0
44.00	1350.0
45.00	1233.0
46.00	208.0
47.00	2142.0
48.00	1048.0
49.00	6239.0
50.00	28568.0
51.00	9238.0
52.00	498.0
52.90	194.0
54.10	123.0
54.90	382.0
56.00	2147.0
57.10	3985.0
58.00	183.0
60.10	1352.0
61.10	7411.0
62.00	7261.0
63.10	5595.0
64.00	843.0
65.10	1131.0
66.00	167.0
67.00	392.0
68.00	16584.0
69.00	16672.0
70.10	1217.0
72.00	805.0
73.00	7058.0
74.00	27000.0
75.10	82136.0
76.10	7253.0
77.00	1107.0
77.90	919.0
78.90	4479.0
80.00	1320.0
81.00	5007.0
81.90	992.0
82.90	165.0
85.90	316.0
87.00	8446.0
88.00	8379.0
91.00	688.0
92.00	4705.0
93.00	7333.0
94.00	19424.0
95.00	170560.0
96.10	11265.0
97.00	346.0
102.80	110.0
103.90	696.0
104.80	220.0
105.90	714.0
106.90	189.0
110.80	148.0
111.80	141.0
112.80	177.0
114.80	159.0
115.90	696.0
116.90	1101.0
117.90	636.0
118.90	881.0
123.90	146.0
127.90	697.0
129.00	231.0
129.80	532.0
130.80	217.0
135.00	216.0
137.00	233.0
140.00	105.0
140.90	1335.0
141.90	201.0
142.90	1921.0
144.00	117.0
145.00	375.0
145.80	242.0
146.90	108.0
147.80	403.0
148.90	109.0
149.80	176.0
152.90	142.0
154.80	452.0
156.80	307.0
158.80	232.0
160.90	185.0
170.70	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

171.90	1324.0
173.00	1537.0
173.90	148544.0
175.00	11053.0
175.90	143872.0
177.00	9288.0
177.90	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

m/z	Abundance
36.00	1076.0
37.10	6442.0
38.00	5442.0
39.00	2695.0
39.90	250.0
40.80	131.0
43.00	189.0
44.00	1367.0
45.00	1109.0
46.10	197.0
47.10	2005.0
48.00	948.0
49.00	5935.0
50.00	27568.0
51.00	8690.0
52.00	537.0
53.00	165.0
54.10	121.0
54.90	348.0
56.00	1965.0
57.10	3851.0
57.90	171.0
60.10	1208.0
61.00	7067.0
62.00	6735.0
63.10	5433.0
64.00	844.0
65.00	1113.0
66.00	130.0
67.10	342.0
68.00	15757.0
69.00	16432.0
70.00	1042.0
72.00	885.0
73.00	6990.0
74.00	25776.0
75.10	78488.0
76.10	6605.0
77.00	1091.0
77.90	911.0
79.00	4389.0
79.90	1290.0
81.00	4736.0
81.90	976.0
82.90	171.0
86.00	273.0
87.00	8245.0
88.00	7673.0
91.00	606.0
92.00	4530.0
93.00	6800.0
94.00	18632.0
95.00	164416.0
96.00	10735.0
97.00	297.0
103.90	655.0
104.90	225.0
105.90	744.0
106.90	158.0
110.80	180.0
111.90	149.0
112.80	153.0
114.80	156.0
115.90	667.0
117.00	1067.0
117.90	650.0
118.80	823.0
123.90	126.0
126.90	108.0
127.90	668.0
129.00	193.0
129.90	505.0
130.90	170.0
135.00	199.0
136.90	222.0
140.90	1321.0
141.90	242.0
142.90	1819.0
144.10	122.0
144.90	342.0
145.80	240.0
146.90	113.0
147.80	366.0
148.90	104.0
149.80	167.0
152.70	115.0
154.90	427.0
156.80	315.0
158.80	221.0
160.90	193.0
171.90	1388.0
173.00	1638.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221

173.90	145152.0
175.00	10526.0
175.90	141376.0
177.00	9047.0
177.90	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB221