
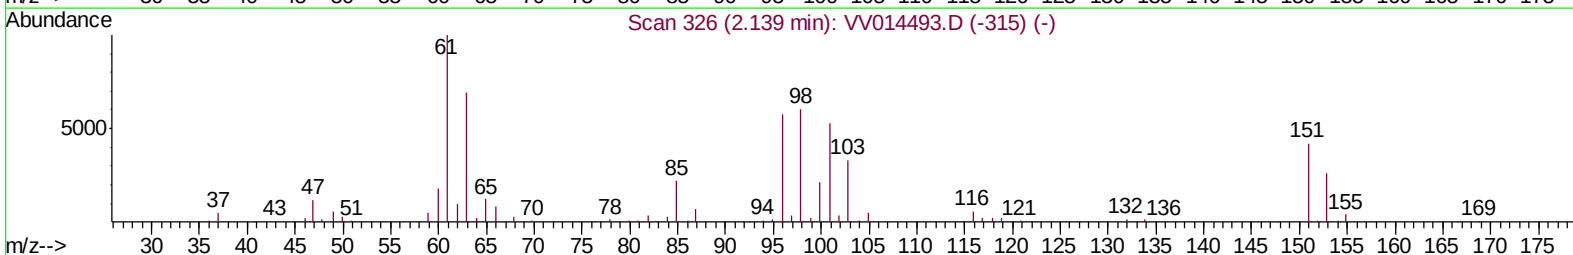
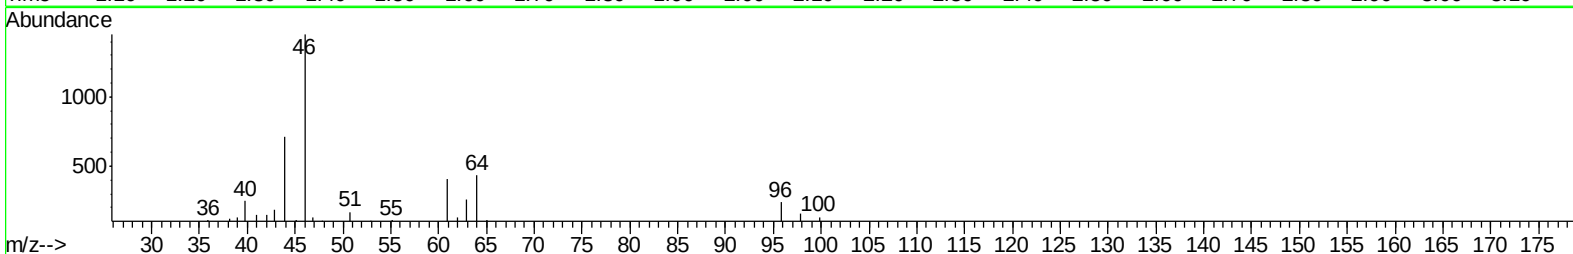


Data File : VV014502.D
Acq On : 04 Feb 2020 19:05
Operator : SY/MD
Sample : L1324-11MSD
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 05 01:09:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 05 01:06:41 2020
Response via : Initial Calibration

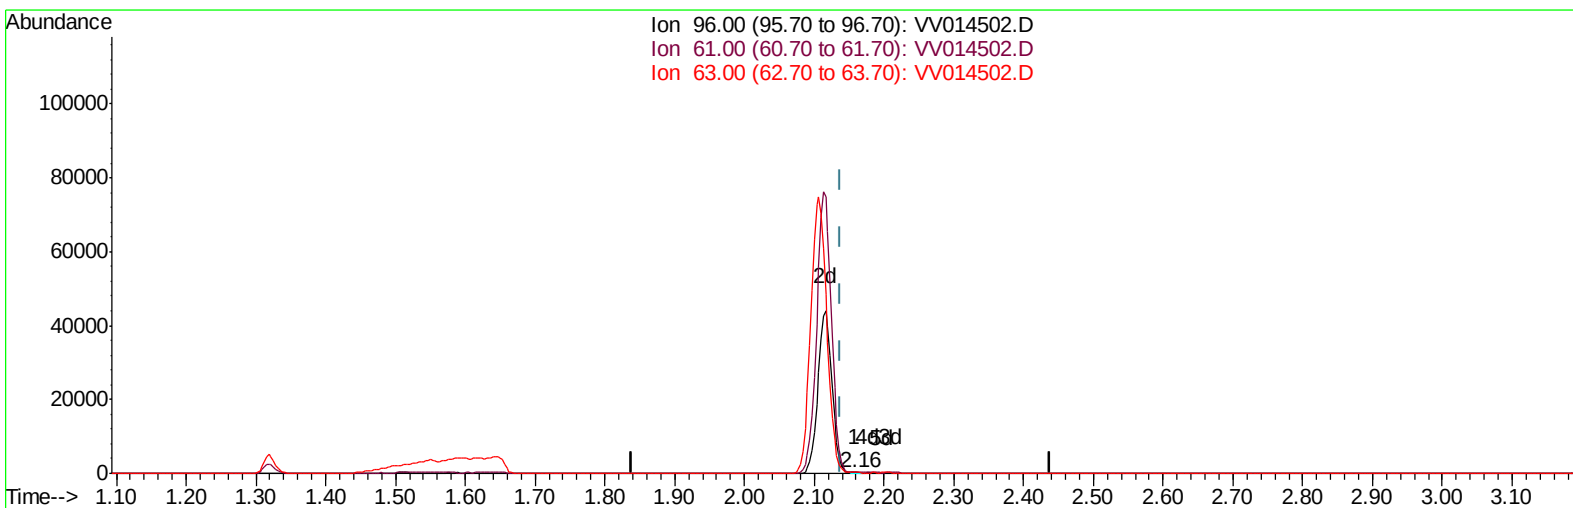

TIC: VV014502.D

(12) 1,1-Dichloroethene (T)

2.158min (+0.019) 0.13ug/L

response 189

Ion	Exp%	Act%
96.00	100	100
61.00	172.10	172.03
63.00	124.40	109.32
0.00	0.00	0.00