


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020420\
Data File : VV014502.D
Acq On : 04 Feb 2020 19:05
Operator : SY/MD
Sample : L1324-11MSD
Misc : 5.08µ/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 15 05:38:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 05 01:06:41 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
Client Sampled :
GAT66MSD

Manual Integrations
APPROVED

MMDadoda
2/5/2020 12:25:24 PM

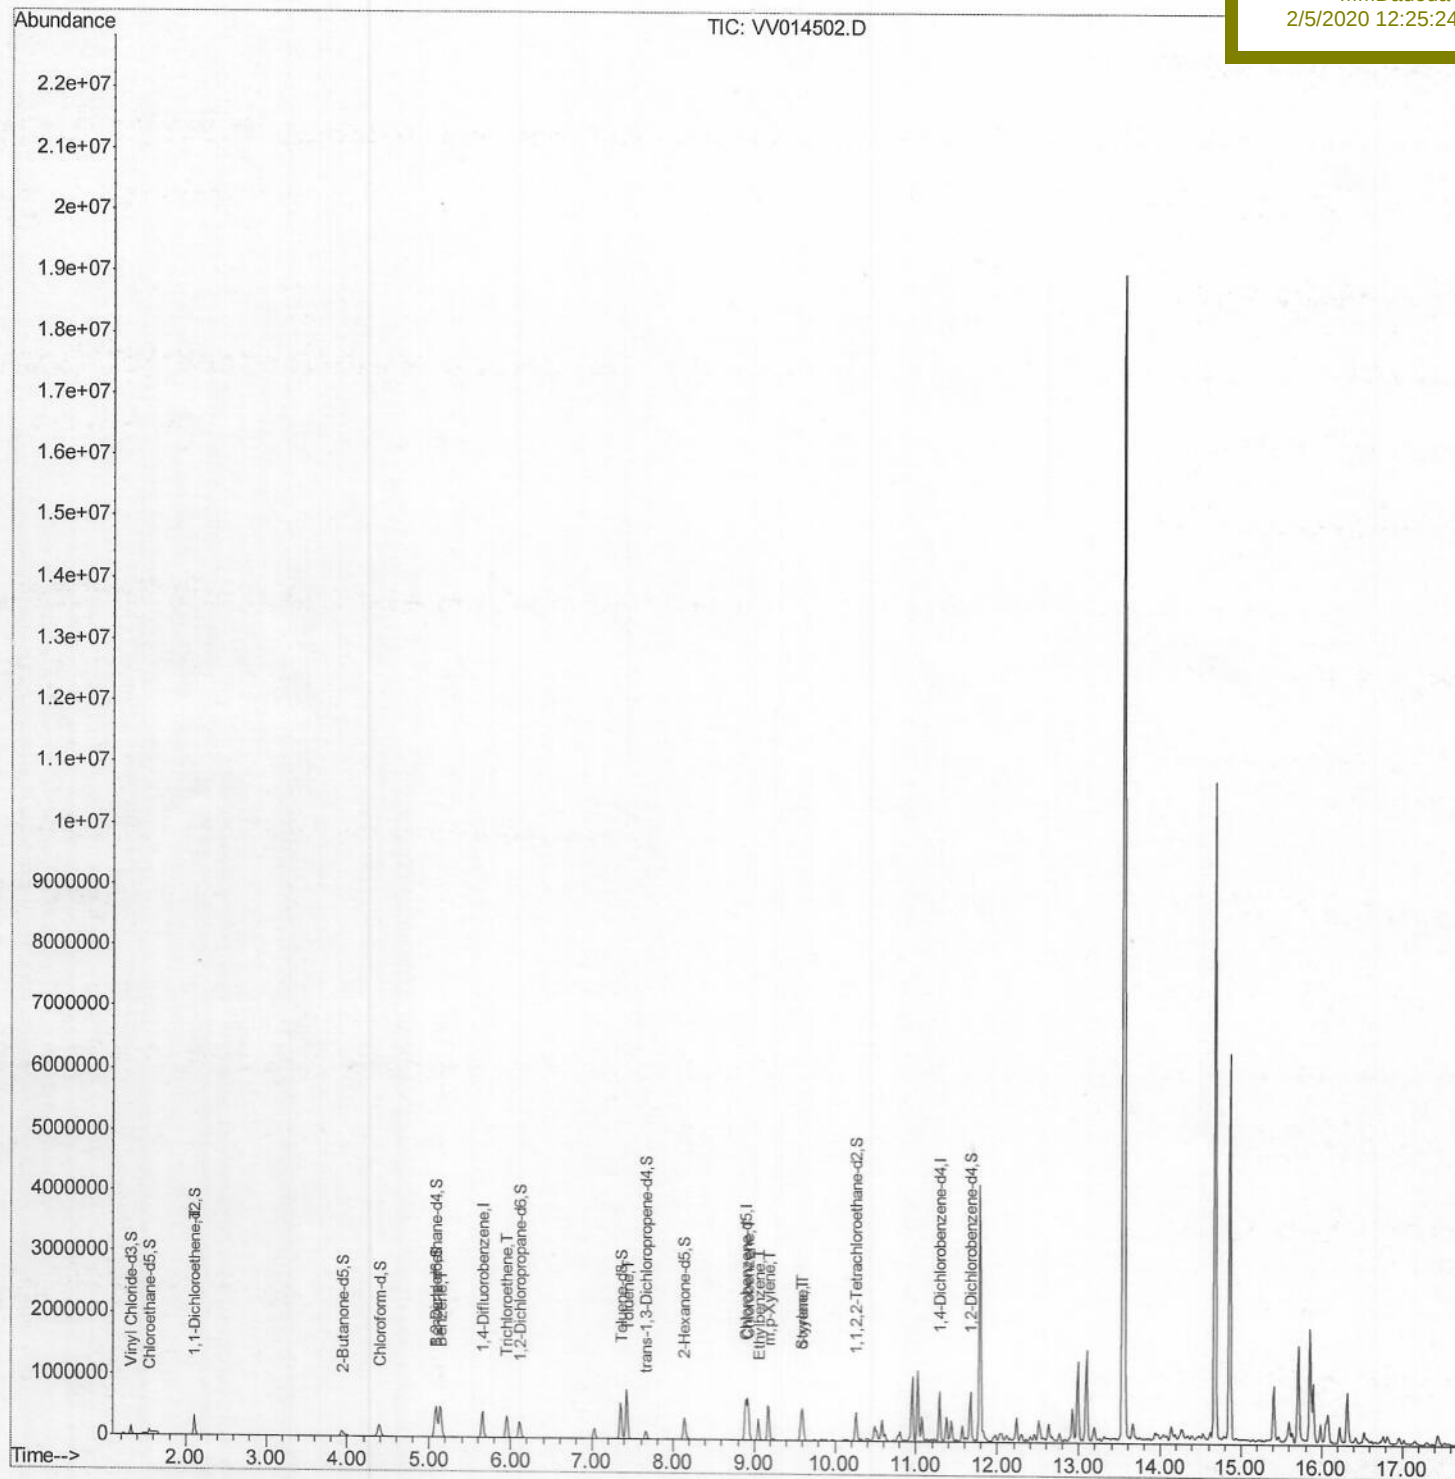

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV020420\
Quantitation Report (Qedit)




Data File : VV014502.D
Acq On : 04 Feb 2020 19:05
Operator : SY/MD
Sample : L1324-11MSD
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 05 01:09:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 05 01:06:41 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
Client Sampled :
GAT66MSD

Manual Integrations
APPROVED

MMDadoda
2/5/2020 12:25:24 PM

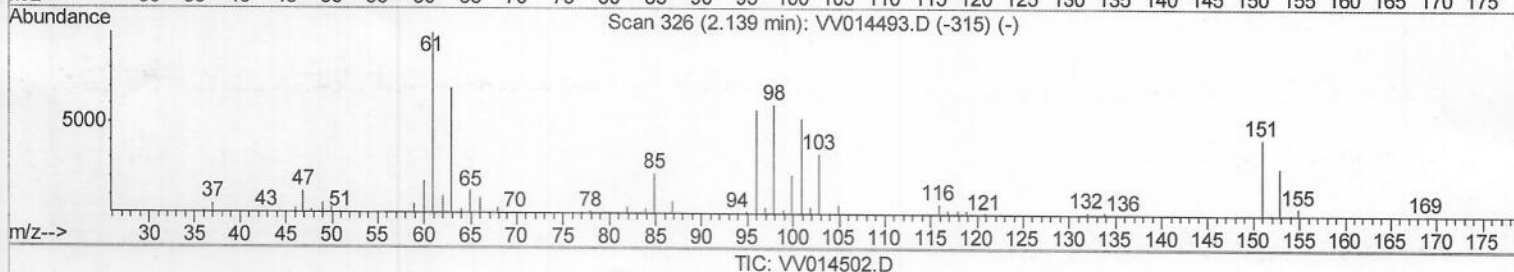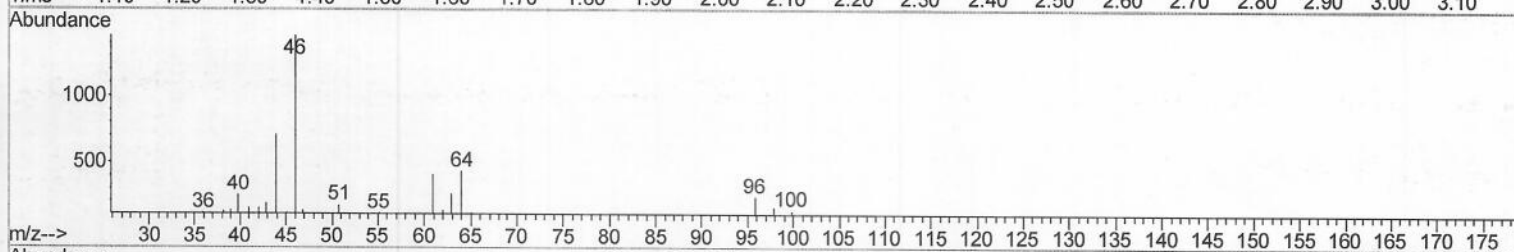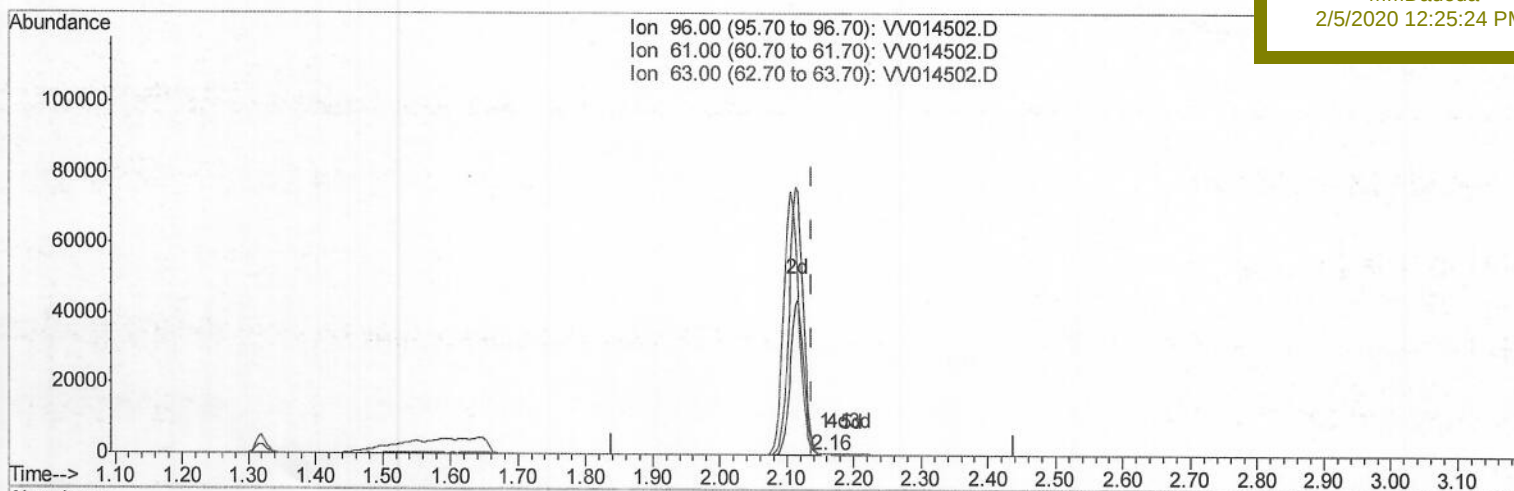

(12) 1,1-Dichloroethene (T)

2.158min (+0.019) 0.13ug/L

response 189

Ion	Exp%	Act%
96.00	100	100
61.00	172.10	172.03
63.00	124.40	109.32
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV020420\
Quantitation Report (Qedit)




Data File : VV014502.D
Acq On : 04 Feb 2020 19:05
Operator : SY/MD
Sample : L1324-11MSD
Misc : 5.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 05 01:09:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 05 01:06:41 2020
Response via : Initial Calibration

Instrument :
MSVOA_V
ClientSampleId :
GAT66MSD

Manual Integrations
APPROVED

MMDadoda
2/5/2020 12:25:24 PM

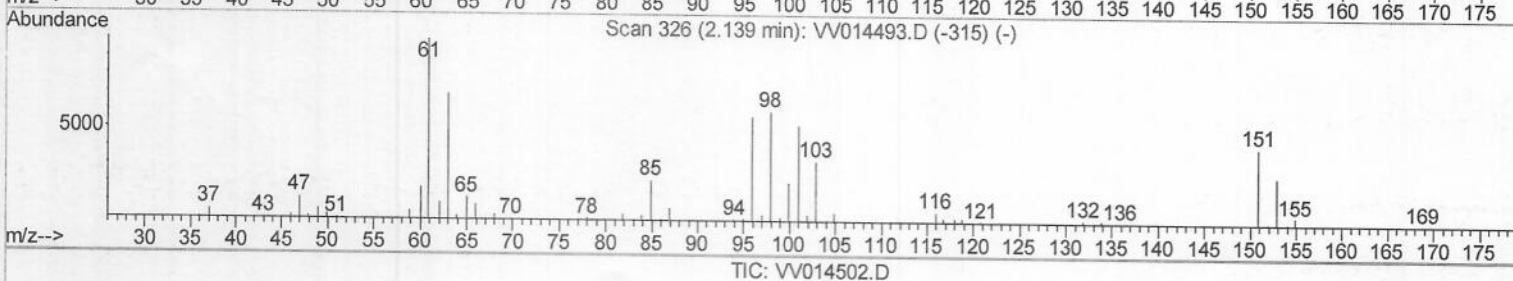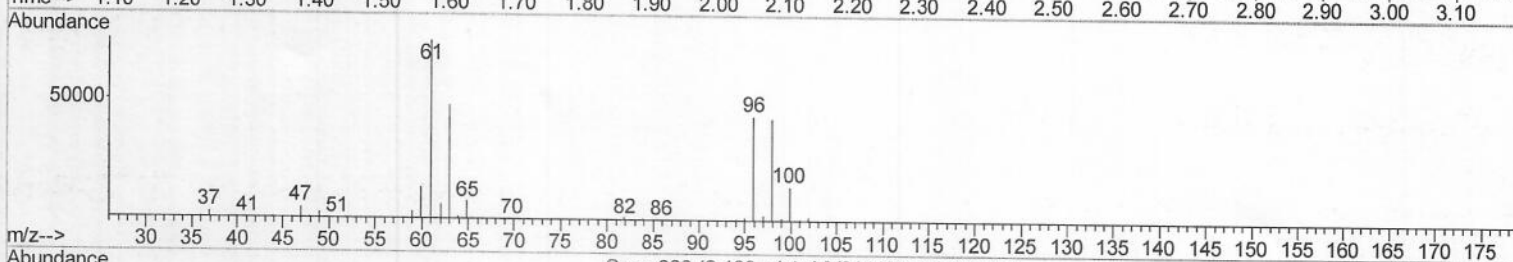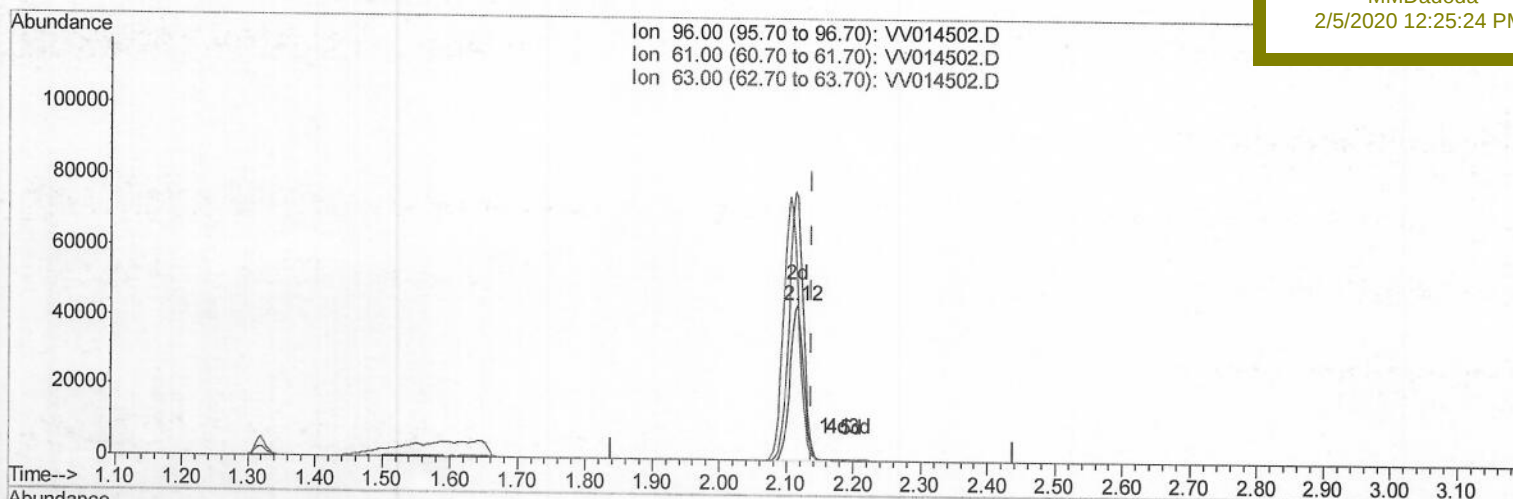

(12) 1,1-Dichloroethene (T)
2.116min (-0.023) 43.69ug/L m
response 61562

> 02/06/20 SJ

Ion	Exp%	Act%
96.00	100	100
61.00	172.10	169.56
63.00	124.40	109.84
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020420\
 Data File : VV014502.D
 Acq On : 04 Feb 2020 19:05
 Operator : SY/MD
 Sample : L1324-11MSD
 Misc : 5.08µ/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 15 05:38:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 05 01:06:41 2020
 Response via : Initial Calibration

Instrument :
 MSVOA_V
 Client Sampled :
 GAT66MSD

Manual Integrations
 APPROVED

MMDadoda
 2/5/2020 12:25:24 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.66	114	370444	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	365259	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	204942	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	86228	41.91	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.82%		
7) Chloroethane-d5	1.55	69	33190	25.95	ug/L	-0.04
Spiked Amount 50.000	Range 70 - 130		Recovery =	51.90%#		
11) 1,1-Dichloroethene-d2	2.11	63	118301	43.07	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.14%		
21) 2-Butanone-d5	3.94	46	142852	103.19	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.19%		
24) Chloroform-d	4.39	84	191749	44.04	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.08%		
26) 1,2-Dichloroethane-d4	5.07	65	126898	48.38	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.76%		
32) Benzene-d6	5.09	84	413291	42.97	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.94%		
36) 1,2-Dichloropropane-d6	6.11	67	132244	43.46	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	86.92%		
41) Toluene-d8	7.35	98	400373	45.10	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.20%		
43) trans-1,3-Dichloropropene-	7.66	79	69847	45.16	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.32%		
47) 2-Hexanone-d5	8.14	63	139975	117.58	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	117.58%		
57) 1,1,2,2-Tetrachloroethane-	10.26	84	214046	54.60	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	109.20%		
64) 1,2-Dichlorobenzene-d4	11.67	152	186427	49.39	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.78%		

Target Compounds

					Ovalue
12) 1,1-Dichloroethene	2.12	96	61562m	43.686	ug/L
33) Benzene	5.14	78	502606	46.635	ug/L
34) Trichloroethene	5.95	95	122637	45.053	ug/L
42) Toluene	7.43	91	582910	51.667	ug/L
51) Chlorobenzene	8.92	112	373180	51.706	ug/L
52) Ethylbenzene	9.05	91	245301	19.372	ug/L
53) m,p-Xylene	9.18	106	163878	34.659	ug/L
54) o-xylene	9.59	106	97391	20.787	ug/L
55) Styrene	9.60	104	198634	25.262	ug/L

202106/2021

(#) = qualifier out of range (m) = manual integration (+) = signals summed