

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020420\
 Data File : VV014494.D
 Acq On : 04 Feb 2020 11:21
 Operator : SY/MD
 Sample : VV0204WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK66

Quant Time: Feb 05 01:19:16 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Feb 05 01:06:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	426254	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	394527	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	190977	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	96935	40.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.90%
7) Chloroethane-d5	1.59	69	69765	47.40	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.80%
11) 1,1-Dichloroethene-d2	2.13	63	112562	35.62	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.24%
21) 2-Butanone-d5	3.92	46	168881	106.02	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	106.02%
24) Chloroform-d	4.40	84	236418	47.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.38%
26) 1,2-Dichloroethane-d4	5.07	65	149693	49.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.20%
32) Benzene-d6	5.09	84	504008	48.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.04%
36) 1,2-Dichloropropane-d6	6.11	67	160089	48.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.42%
41) Toluene-d8	7.35	98	465157	48.51	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.02%
43) trans-1,3-Dichloropropene-	7.66	79	81698	48.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.82%
47) 2-Hexanone-d5	8.13	63	132092	102.72	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.72%
57) 1,1,2,2-Tetrachloroethane-	10.25	84	203404	48.03	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.06%
64) 1,2-Dichlorobenzene-d4	11.67	152	174326	49.56	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.12%


Target Compounds					Ovalue
13) Acetone	2.18	43	2018	1.485 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020420\
Data File : VV014494.D
Acq On : 04 Feb 2020 11:21
Operator : SY/MD
Sample : VV0204WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Quant Time: Feb 05 01:19:16 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Feb 05 01:06:41 2020
Response via : Initial Calibration

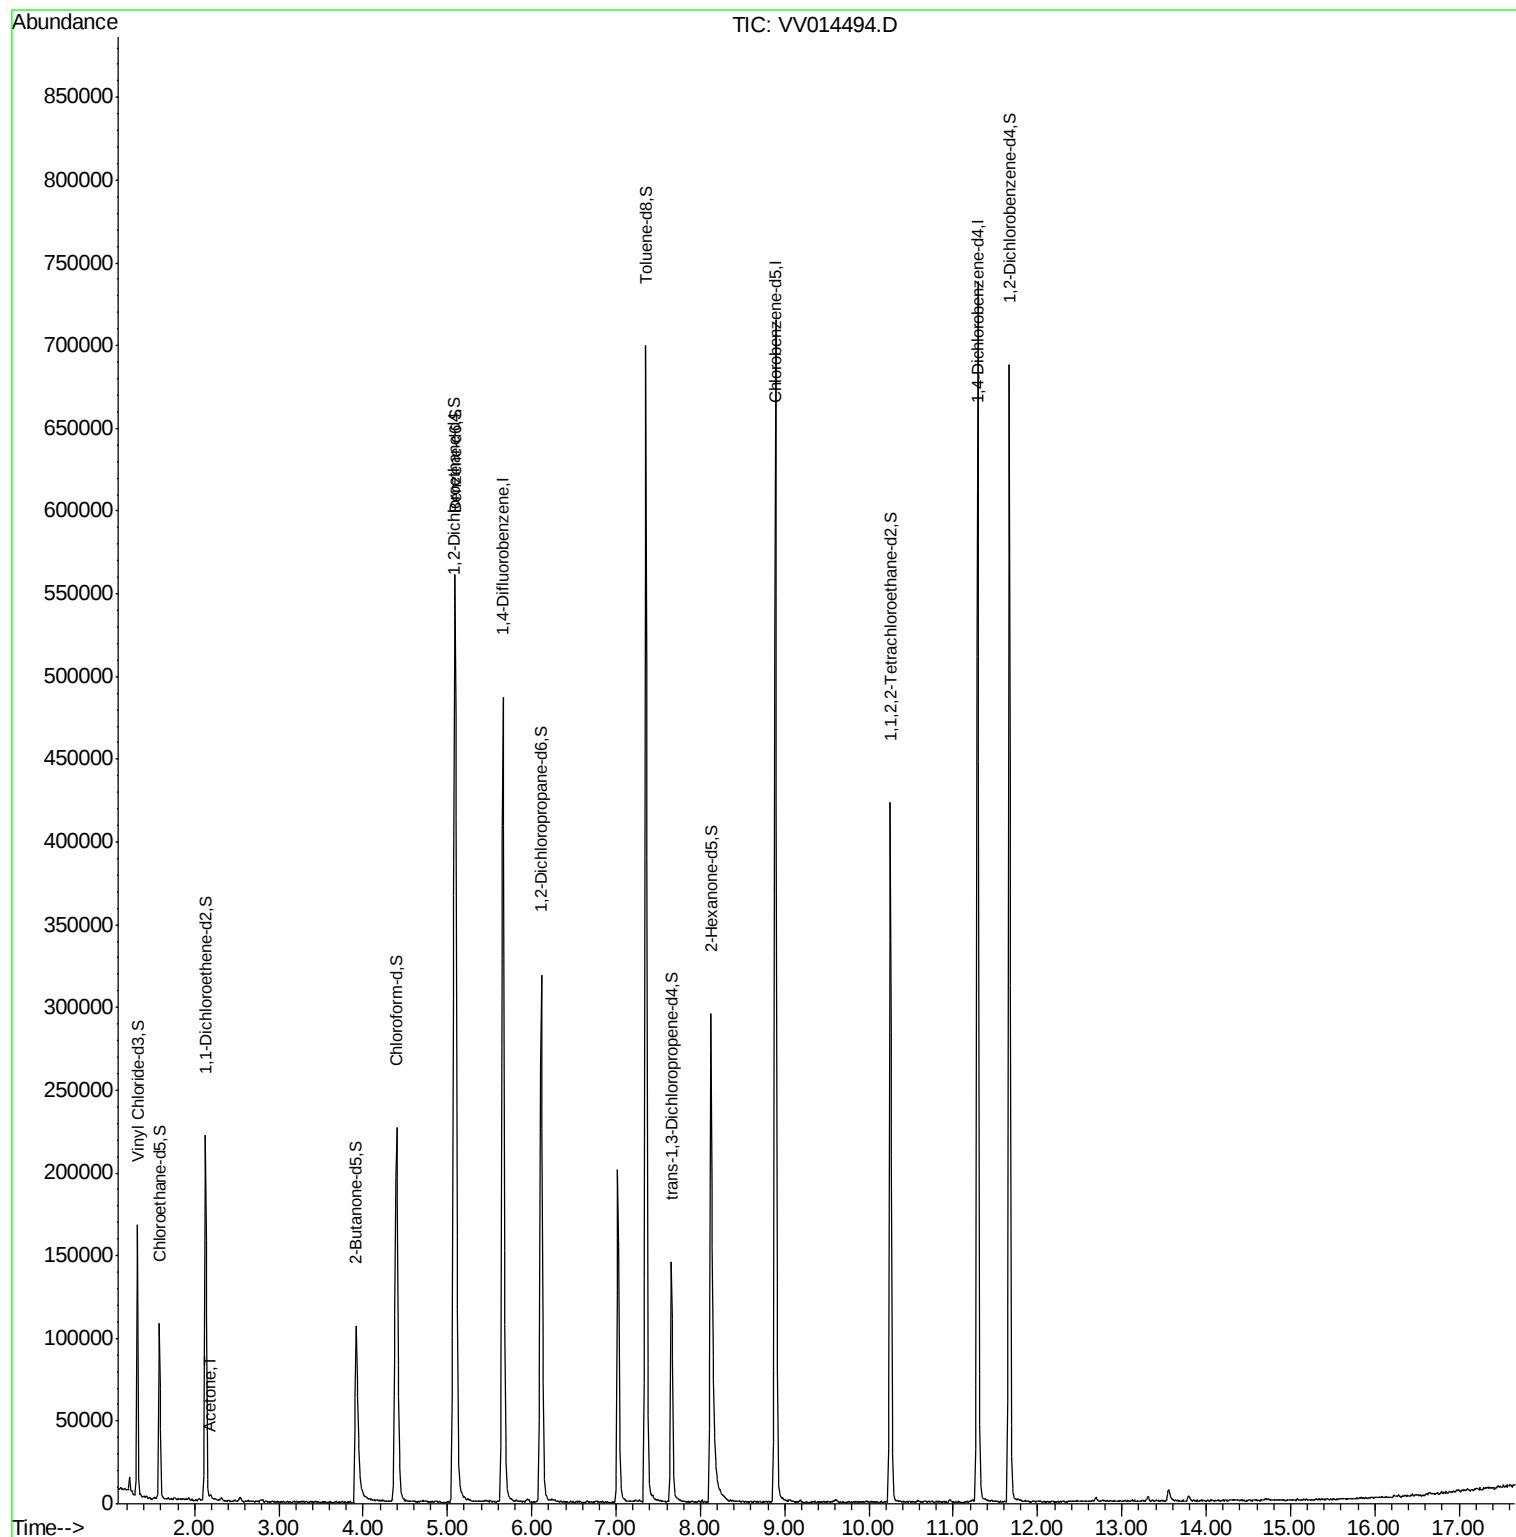

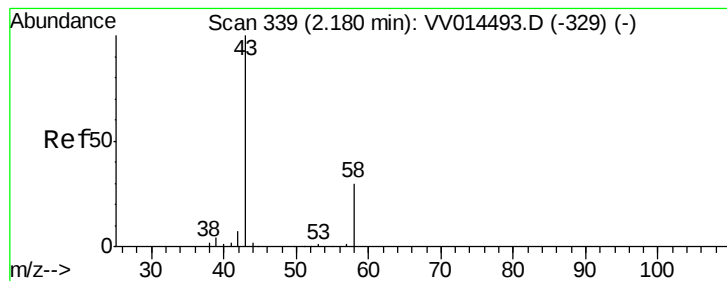

#13
Acetone
Concen: 1.485 ug/L
RT: 2.18 min Scan# 340
Delta R.T. 0.00 min
Lab File: VV014494.D
Acq: 04 Feb 2020 11:21

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Tot Ion: 43 Resp: 2018
Ion Ratio Lower Upper
43 100
58 28.9 0.0 61.2

