


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV020420\
 Data File : VV014492.D
 Acq On : 04 Feb 2020 09:06
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM020120WMA.M
 Title : VOC Analysis
 Last Update : Wed Feb 05 05:59:31 2020

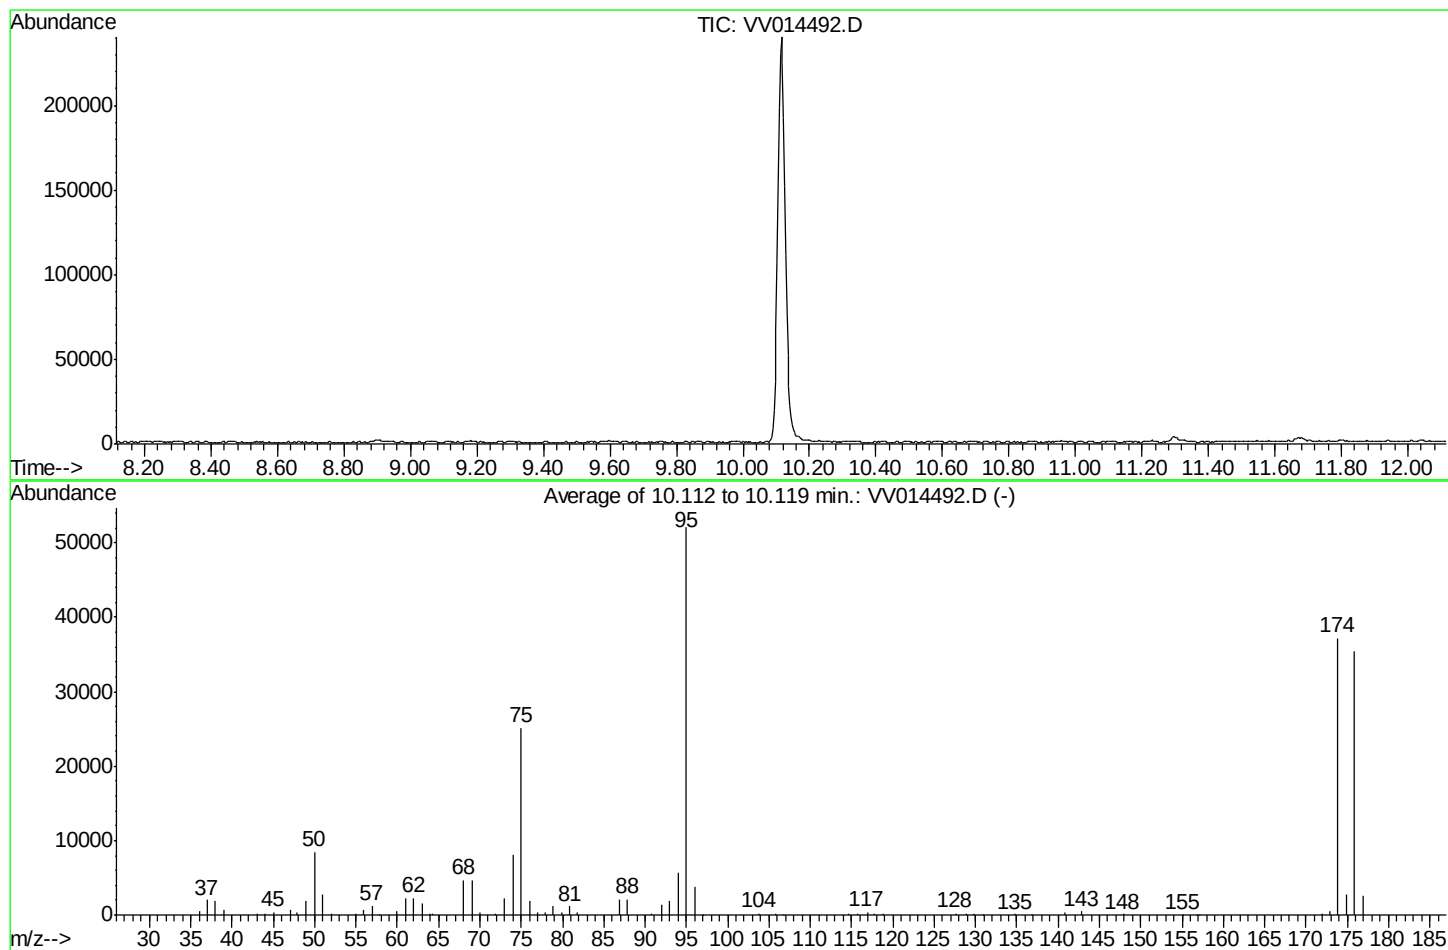

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	8438	PASS
75	95	30	80	48.3	25154	PASS
95	95	100	100	100.0	52077	PASS
96	95	5	9	7.2	3748	PASS
173	174	0.00	2	1.4	504	PASS
174	95	50	120	71.4	37189	PASS
175	174	5	9	7.4	2739	PASS
176	174	95	101	95.4	35474	PASS
177	176	5	9	7.4	2613	PASS

m/z	Abundance
36.00	429.0
37.00	2062.0
37.90	1970.0
39.00	741.0
39.90	348.0
43.10	141.0
43.90	779.0
45.00	357.0
47.00	775.0
47.90	262.0
49.00	1895.0
50.00	8182.0
51.00	2762.0
52.00	143.0
54.90	125.0
55.90	657.0
57.00	1266.0
59.90	451.0
60.90	2096.0
61.90	2286.0
63.00	1671.0
64.00	180.0
68.00	4789.0
69.00	4671.0
70.10	353.0
71.90	261.0
73.00	2242.0
74.00	8245.0
75.00	25136.0
76.00	1989.0
77.00	388.0
77.90	270.0
78.80	1167.0
79.90	452.0
80.90	1195.0
81.80	234.0
86.90	1911.0
87.90	2086.0
90.80	153.0
92.00	1387.0
93.00	2008.0
94.00	5724.0
95.00	52152.0
96.00	3662.0
96.90	141.0
103.80	193.0
105.90	161.0
106.80	104.0
114.70	137.0
115.80	216.0
116.90	374.0
117.90	155.0
118.80	240.0
127.70	177.0
129.00	115.0
129.80	217.0
134.90	141.0
136.80	142.0
140.80	406.0
142.90	490.0
147.90	139.0
155.10	124.0
156.80	105.0
171.90	181.0
172.90	542.0
173.90	36304.0
174.90	2738.0
175.90	34672.0
177.00	2576.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	455.0
36.90	2057.0
37.90	1897.0
39.00	729.0
39.90	394.0
43.10	139.0
43.90	757.0
45.00	356.0
47.00	707.0
47.90	273.0
49.00	1904.0
50.00	8738.0
51.00	2802.0
52.00	148.0
55.00	135.0
55.90	636.0
57.00	1268.0
57.70	118.0
59.90	477.0
61.00	2276.0
61.90	2334.0
63.00	1595.0
63.90	152.0
64.20	159.0
68.00	4876.0
69.00	4815.0
70.10	320.0
71.90	203.0
72.90	2396.0
74.00	8456.0
75.00	26200.0
76.00	2032.0
77.10	403.0
77.80	296.0
78.90	1261.0
79.90	443.0
80.90	1243.0
81.80	264.0
86.90	2129.0
87.90	2233.0
90.70	154.0
92.00	1468.0
93.00	1989.0
94.00	5879.0
95.00	53888.0
96.00	3940.0
96.90	103.0
103.80	205.0
105.80	153.0
114.70	159.0
115.70	181.0
117.00	408.0
117.70	179.0
118.80	266.0
127.60	209.0
129.00	118.0
129.90	192.0
134.80	127.0
136.80	112.0
140.80	414.0
142.90	460.0
147.90	171.0
155.10	111.0
172.00	198.0
172.90	516.0
173.90	38712.0
174.90	2794.0
175.90	36624.0
177.00	2704.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	430.0
37.00	1835.0
37.90	1711.0
39.00	698.0
39.90	370.0
43.10	130.0
43.90	707.0
45.00	325.0
47.00	560.0
47.90	272.0
48.90	1784.0
50.00	8396.0
51.00	2572.0
52.00	133.0
55.00	142.0
55.90	558.0
56.90	1161.0
57.80	109.0
59.90	386.0
61.00	2257.0
62.00	2114.0
63.00	1363.0
63.90	154.0
64.20	145.0
68.00	4525.0
69.00	4492.0
70.00	294.0
71.80	171.0
72.90	2317.0
74.00	7801.0
75.00	24128.0
76.00	1841.0
77.10	345.0
77.80	307.0
78.90	1221.0
79.90	403.0
80.90	1134.0
81.90	297.0
86.90	2160.0
87.90	2063.0
90.80	160.0
92.00	1418.0
93.00	1768.0
94.00	5468.0
95.00	50192.0
96.00	3642.0
103.90	189.0
105.80	158.0
114.70	159.0
115.70	138.0
117.00	340.0
117.70	183.0
118.80	267.0
127.60	195.0
128.80	111.0
129.90	152.0
130.90	107.0
134.80	117.0
140.80	415.0
142.90	441.0
147.90	166.0
157.10	112.0
172.00	186.0
173.00	456.0
173.90	36552.0
174.90	2686.0
175.90	35128.0
177.00	2559.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

Scan 2795 (10.077 min): VV014492.D
BFB86

m/z	Abundance
39.90	464.0
41.10	125.0
44.00	557.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86