

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020521\
 Data File : VW020274.D
 Acq On : 05 Feb 2021 13:53
 Operator : SY/MD
 Sample : M1330-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG504

Quant Time: Feb 06 04:27:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 05 11:56:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	649929	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.855	117	626316	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.254	152	314027	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.306	65	197016	41.58	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.16%		
7) Chloroethane-d5	1.570	69	165929	42.68	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	85.36%		
11) 1,1-Dichloroethene-d2	2.110	63	299650	33.45	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.90%		
21) 2-Butanone-d5	3.888	46	221836	83.80	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.80%		
24) Chloroform-d	4.354	84	367549	43.59	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.18%		
26) 1,2-Dichloroethane-d4	5.036	65	244389	45.72	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.44%		
32) Benzene-d6	5.052	84	747647	46.07	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.14%		
36) 1,2-Dichloropropane-d6	6.074	67	227786	47.02	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.04%		
41) Toluene-d8	7.318	98	699579	45.88	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.76%		
43) trans-1,3-Dichloroprop...	7.624	79	105172	42.59	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.18%		
47) 2-Hexanone-d5	8.090	63	158447	78.62	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.62%		
57) 1,1,2,2-Tetrachloroeth...	10.222	84	289316	41.59	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	83.18%		
64) 1,2-Dichlorobenzene-d4	11.630	152	286046	48.14	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.28%		
Target Compounds						
13) Acetone	2.180	43	8915	4.77	ug/L	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
Data File : VV020274.D
Acq On : 05 Feb 2021 13:53
Operator : SY/MD
Sample : M1330-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG504

Quant Time: Feb 06 04:27:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 05 11:56:25 2021
Response via : Initial Calibration

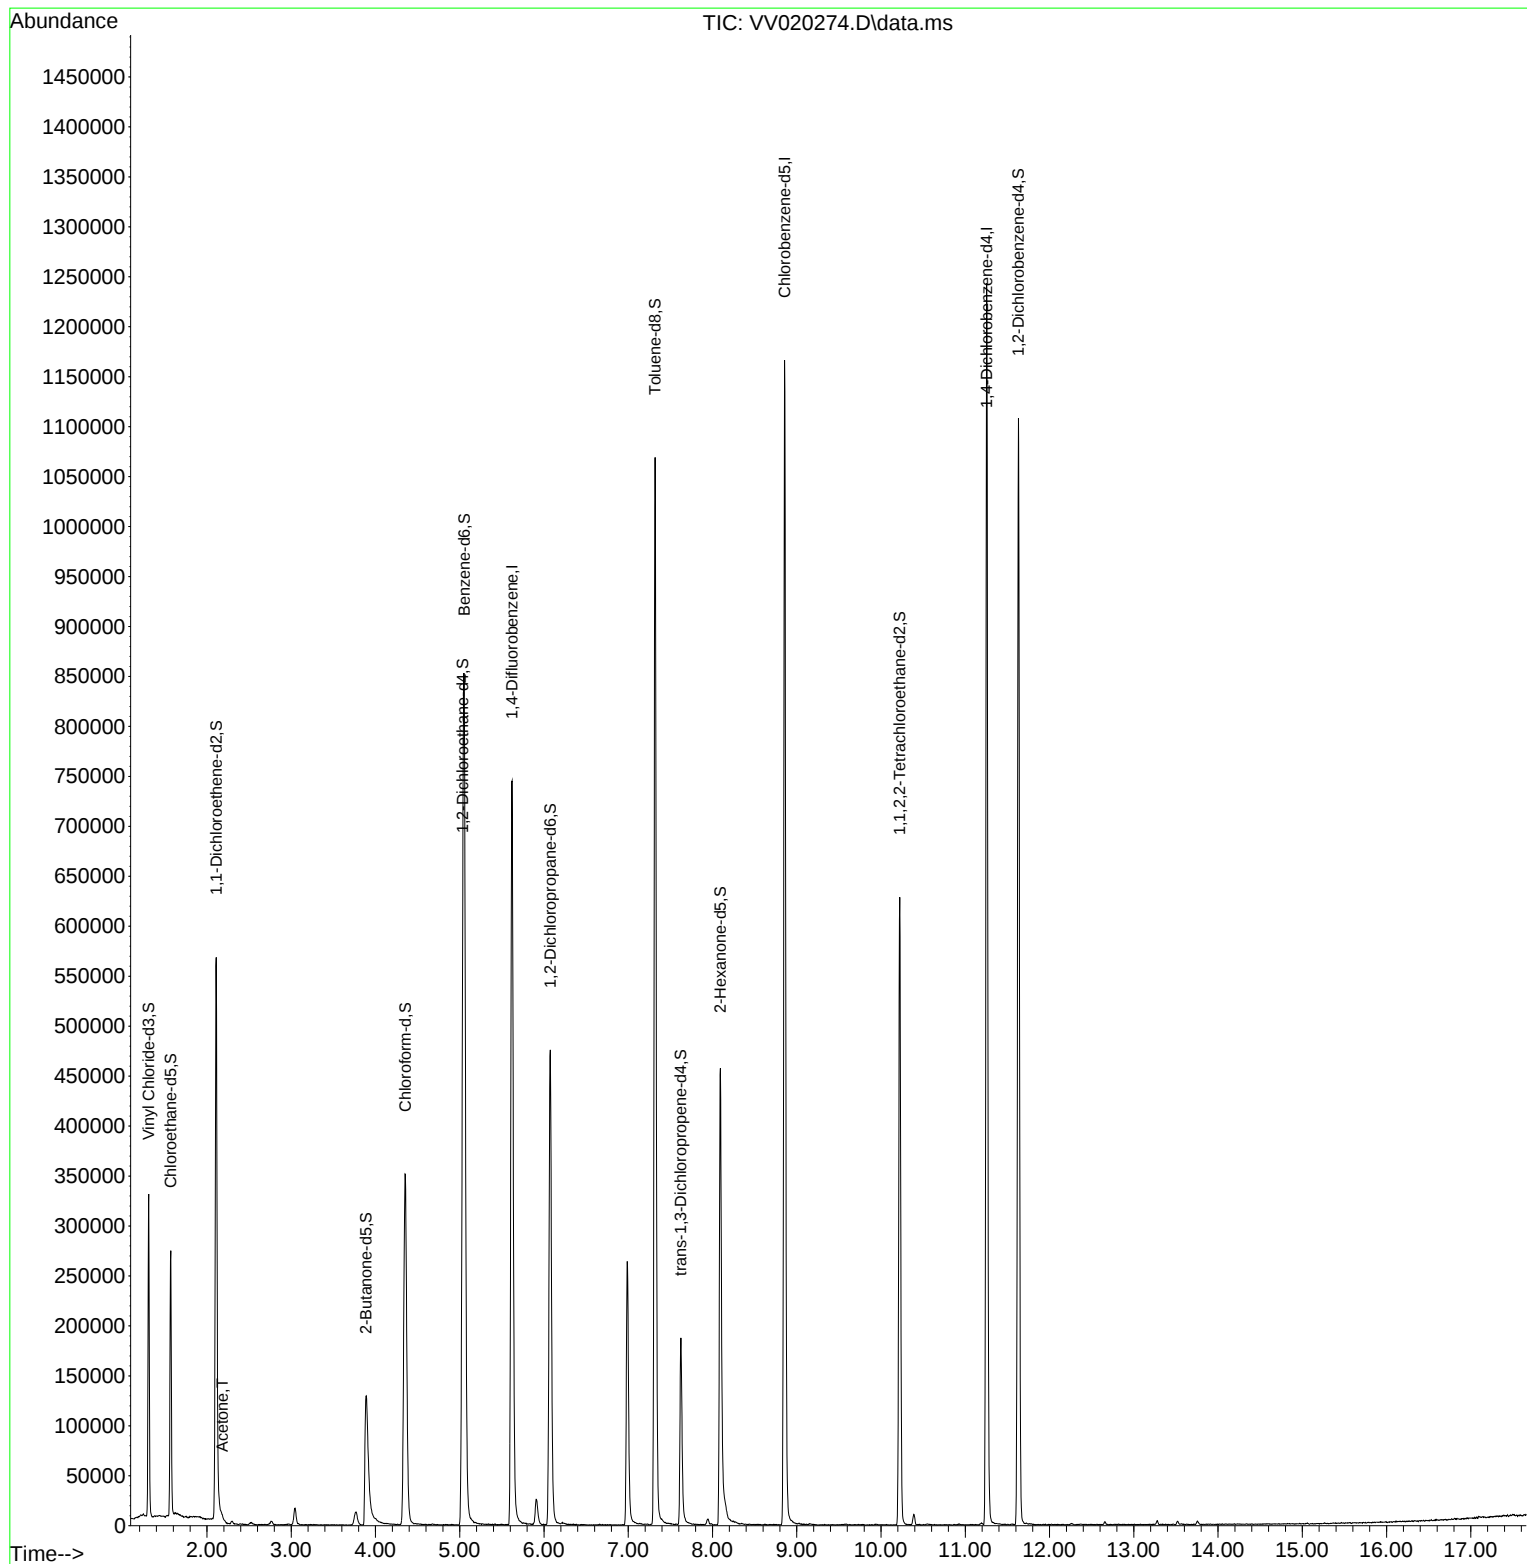

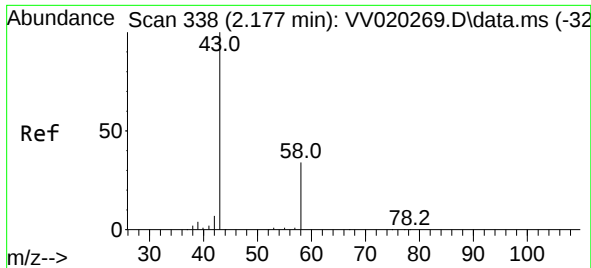

#13
 Acetone
 Concen: 4.77 ug/L
 RT: 2.180 min Scan# 339
 Delta R.T. 0.003 min
 Lab File: VV020274.D
 Acq: 05 Feb 2021 13:53

Instrument :
 MSVOA_V
 ClientSampleId :
 BG504

Tgt Ion: 43 Resp: 8915
 Ion Ratio Lower Upper
 43 100
 58 34.6 0.0 60.2

