

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020521\
 Data File : VW020275.D
 Acq On : 05 Feb 2021 14:16
 Operator : SY/MD
 Sample : M1330-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG511

Quant Time: Feb 06 04:27:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 05 11:56:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.621	114	565205	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.858	117	541503	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.254	152	269877	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.309	65	183352	44.49	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.98%		
7) Chloroethane-d5	1.569	69	153920	45.53	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.06%		
11) 1,1-Dichloroethene-d2	2.110	63	277308	35.60	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.20%		
21) 2-Butanone-d5	3.894	46	215188	93.47	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	93.47%		
24) Chloroform-d	4.354	84	345321	47.09	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.18%		
26) 1,2-Dichloroethane-d4	5.035	65	232131	49.93	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.86%		
32) Benzene-d6	5.055	84	704398	50.21	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.42%		
36) 1,2-Dichloropropane-d6	6.074	67	214290	51.16	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.32%		
41) Toluene-d8	7.318	98	653477	49.56	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.12%		
43) trans-1,3-Dichloroprop...	7.624	79	98775	46.26	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.52%		
47) 2-Hexanone-d5	8.093	63	150917	86.61	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	86.61%		
57) 1,1,2,2-Tetrachloroeth...	10.222	84	270087	44.91	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.82%		
64) 1,2-Dichlorobenzene-d4	11.630	152	262215	51.35	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.70%		
Target Compounds					Qvalue	
13) Acetone	2.184	43	9268	5.70	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
Data File : VV020275.D
Acq On : 05 Feb 2021 14:16
Operator : SY/MD
Sample : M1330-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG511

Quant Time: Feb 06 04:27:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 05 11:56:25 2021
Response via : Initial Calibration

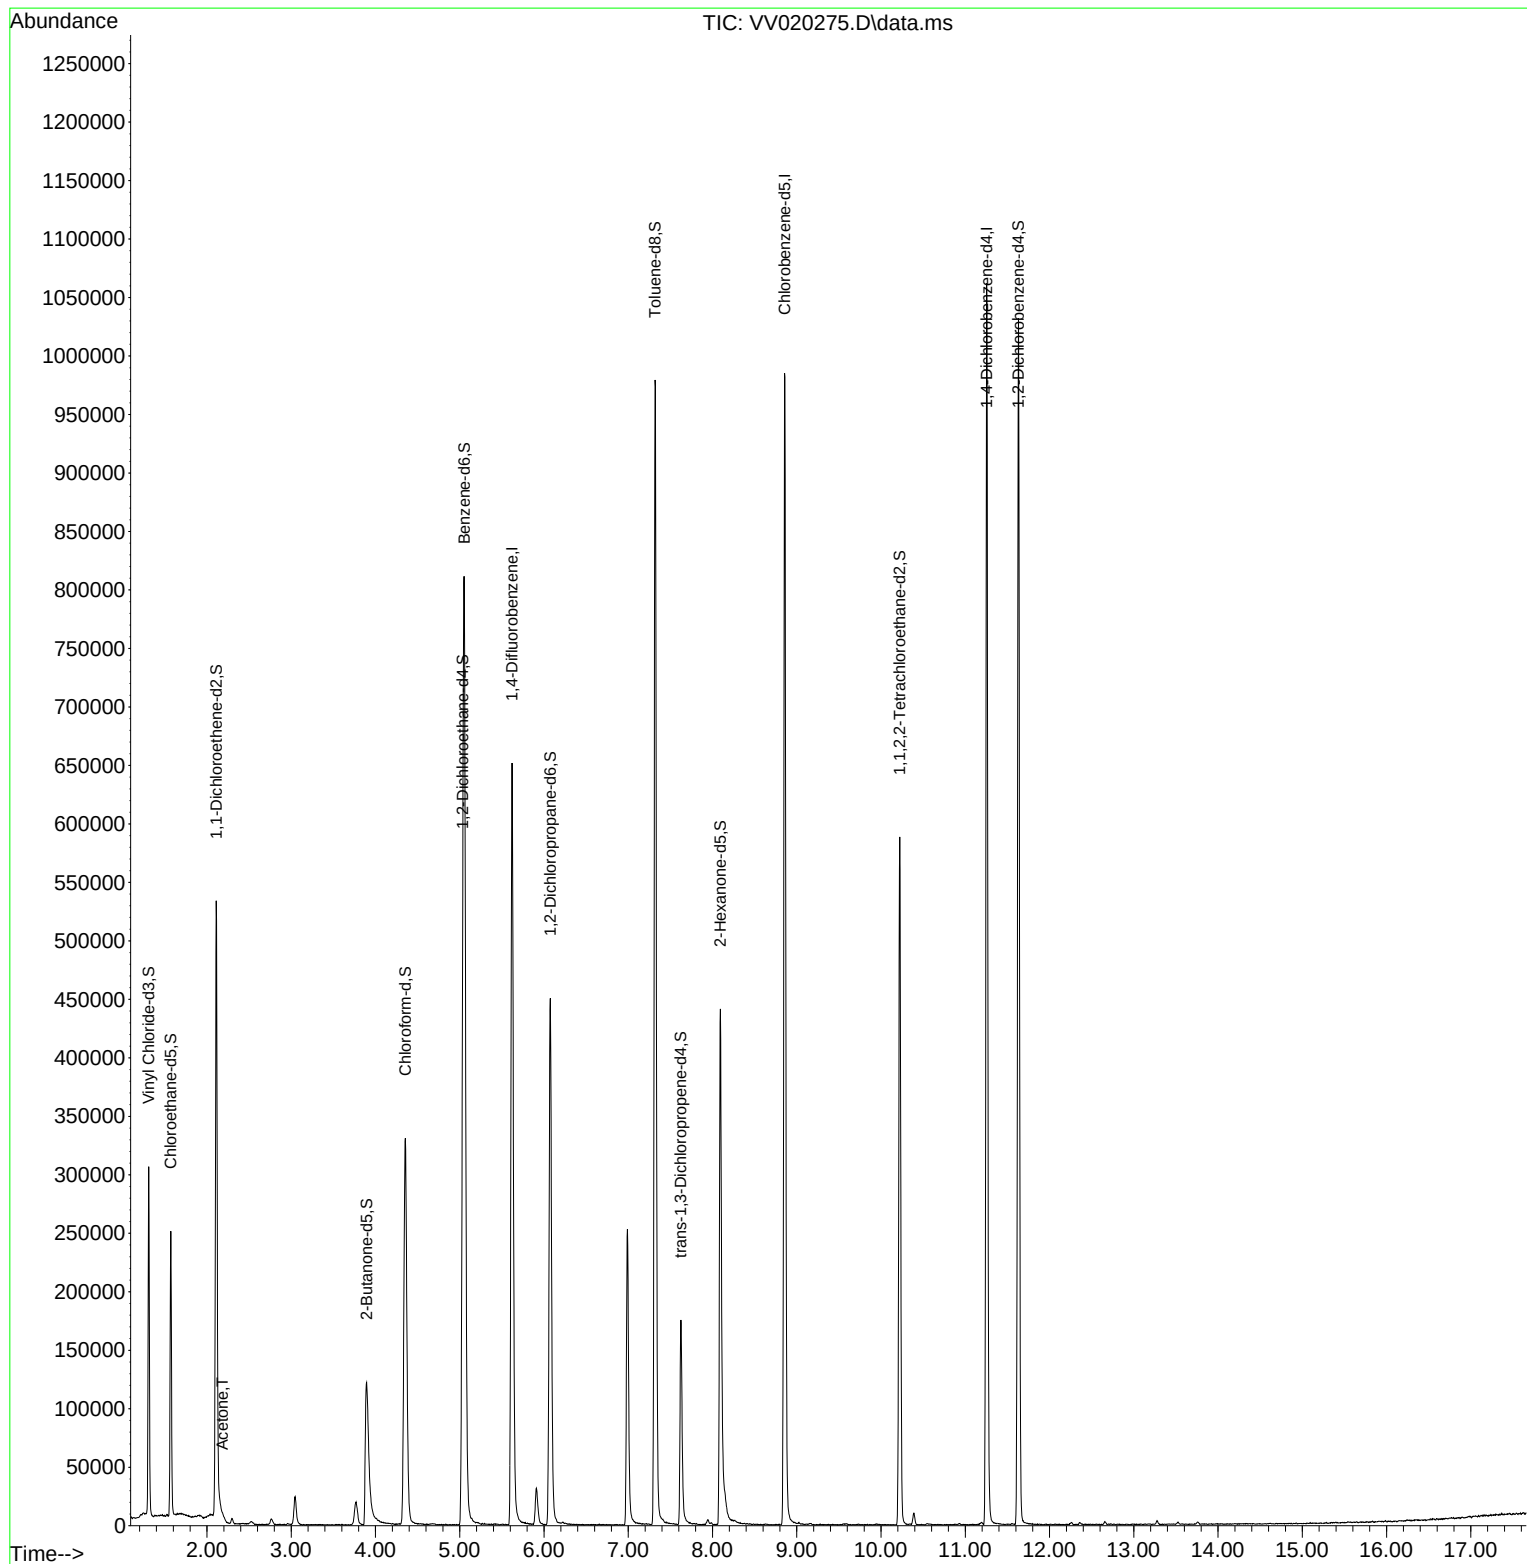

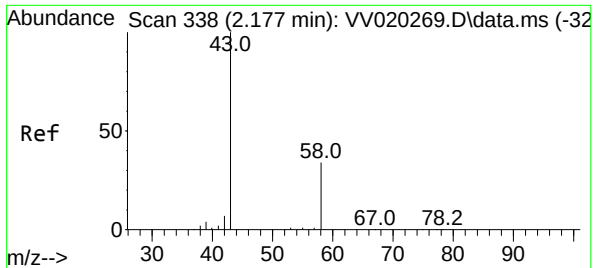

#13
 Acetone
 Concen: 5.70 ug/L
 RT: 2.184 min Scan# 340
 Delta R.T. 0.006 min
 Lab File: VV020275.D
 Acq: 05 Feb 2021 14:16

Instrument :
 MSVOA_V
 ClientSampleId :
 BG511

Tgt Ion: 43 Resp: 9268
 Ion Ratio Lower Upper
 43 100
 58 33.7 0.0 60.2

