

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
 Data File : VV020273.D
 Acq On : 05 Feb 2021 13:28
 Operator : SY/MD
 Sample : VV0205WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	84	rVB	372638	365510	16.10%	2.058%
2	1.569	142	149	163	rVB	288316	322392	14.20%	1.815%
3	2.110	307	317	344	rVB	614518	926319	40.80%	5.216%
4	2.515	435	443	450	rVB6	2995	4463	0.20%	0.025%
5	2.753	514	517	518	rBV2	535	308	0.01%	0.002%
6	2.894	558	561	562	rBV	347	189	0.01%	0.001%
7	2.994	588	592	596	rBV3	499	517	0.02%	0.003%
8	3.110	626	628	633	rVB2	460	301	0.01%	0.002%
9	3.142	636	638	644	rVV4	482	455	0.02%	0.003%
10	3.200	654	656	659	rBV	423	273	0.01%	0.002%
11	3.364	703	707	711	rBV4	434	353	0.02%	0.002%
12	3.428	724	727	728	rBV	219	134	0.01%	0.001%
13	3.560	762	768	769	rBV2	303	262	0.01%	0.001%
14	3.624	786	788	791	rVV	433	227	0.01%	0.001%
15	3.643	791	794	796	rVV2	321	190	0.01%	0.001%
16	3.663	796	800	803	rVV4	517	419	0.02%	0.002%
17	3.685	803	807	810	rVV2	328	229	0.01%	0.001%
18	3.746	824	826	829	rVB2	299	175	0.01%	0.001%
19	3.814	842	847	849	rBV2	613	468	0.02%	0.003%
20	3.891	860	871	910	rBV	147420	436841	19.24%	2.460%
21	4.354	999	1015	1049	rVB	365193	896469	39.48%	5.048%
22	4.601	1089	1092	1095	rBV3	488	368	0.02%	0.002%
23	4.659	1106	1110	1112	rBV2	712	519	0.02%	0.003%
24	4.785	1148	1149	1151	rBV2	396	208	0.01%	0.001%
25	4.814	1155	1158	1159	rVV3	399	167	0.01%	0.001%
26	4.852	1168	1170	1172	rBV2	466	179	0.01%	0.001%
27	4.958	1201	1203	1207	rBV3	567	356	0.02%	0.002%
28	4.987	1210	1212	1213	rBV	396	188	0.01%	0.001%
29	5.052	1214	1232	1265	rBV2	880915	2270434	100.00%	12.785%
30	5.515	1374	1376	1380	rVB4	576	339	0.01%	0.002%
31	5.534	1380	1382	1384	rVB2	601	221	0.01%	0.001%
32	5.547	1384	1386	1390	rBV	702	480	0.02%	0.003%
33	5.566	1390	1392	1396	rBV4	287	252	0.01%	0.001%
34	5.621	1396	1409	1438	rBV	699365	1406463	61.95%	7.920%
35	5.913	1489	1500	1519	rBV5	19438	42994	1.89%	0.242%
36	6.074	1535	1550	1577	rBV	490424	1005034	44.27%	5.660%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
 Data File : VV020273.D
 Acq On : 05 Feb 2021 13:28
 Operator : SY/MD
 Sample : VV0205WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

37	6.293	1616	1618	1620	rVB2	410	145	0.01%	0.001%
38	6.331	1628	1630	1631	rBV2	378	152	0.01%	0.001%
39	6.380	1642	1645	1647	rBV3	311	176	0.01%	0.001%
40	6.399	1649	1651	1655	rBV2	387	192	0.01%	0.001%
41	6.521	1685	1689	1693	rBV3	683	476	0.02%	0.003%
42	6.576	1704	1706	1711	rVB3	491	290	0.01%	0.002%
43	6.605	1711	1715	1717	rBV2	398	311	0.01%	0.002%
44	6.627	1720	1722	1724	rVB	448	198	0.01%	0.001%
45	6.653	1728	1730	1731	rBV	338	158	0.01%	0.001%
46	6.691	1739	1742	1745	rVB	493	274	0.01%	0.002%
47	6.733	1752	1755	1759	rVB3	350	255	0.01%	0.001%
48	6.814	1777	1780	1785	rBV2	342	336	0.01%	0.002%
49	6.836	1785	1787	1790	rBV3	451	301	0.01%	0.002%
50	6.990	1823	1835	1857	rBV2	266234	489529	21.56%	2.757%
51	7.318	1925	1937	1960	rBV	1079489	1864446	82.12%	10.499%
52	7.624	2020	2032	2067	rBV	187990	339826	14.97%	1.914%
53	7.987	2138	2145	2153	rBV4	2299	3113	0.14%	0.018%
54	8.093	2167	2178	2212	rBV	535172	994754	43.81%	5.602%
55	8.624	2338	2343	2344	rBV2	566	409	0.02%	0.002%
56	8.711	2368	2370	2374	rVB2	593	354	0.02%	0.002%
57	8.769	2385	2388	2392	rVB2	437	286	0.01%	0.002%
58	8.855	2403	2415	2442	rBV	1071572	1744933	76.85%	9.826%
59	9.154	2501	2508	2515	rBV5	1758	2265	0.10%	0.013%
60	9.248	2535	2537	2542	rVB2	436	305	0.01%	0.002%
61	9.270	2542	2544	2545	rBV	426	158	0.01%	0.001%
62	9.331	2559	2563	2564	rBV2	359	243	0.01%	0.001%
63	9.524	2617	2623	2626	rBV3	438	394	0.02%	0.002%
64	9.685	2670	2673	2676	rBV2	506	363	0.02%	0.002%
65	9.730	2684	2687	2688	rBV	282	156	0.01%	0.001%
66	9.765	2696	2698	2699	rBV	414	159	0.01%	0.001%
67	9.810	2711	2712	2718	rVB4	632	465	0.02%	0.003%
68	9.846	2718	2723	2726	rBV2	387	390	0.02%	0.002%
69	9.942	2745	2753	2760	rBV4	1345	2273	0.10%	0.013%
70	10.010	2770	2774	2775	rBV2	352	237	0.01%	0.001%
71	10.022	2775	2778	2781	rVV3	449	286	0.01%	0.002%
72	10.103	2802	2803	2809	rVB2	402	208	0.01%	0.001%
73	10.154	2815	2819	2823	rBV2	367	358	0.02%	0.002%
74	10.222	2828	2840	2864	rVV	691520	1071693	47.20%	6.035%
75	10.421	2898	2902	2904	rBV3	482	295	0.01%	0.002%
76	10.547	2937	2941	2949	rVB5	1738	1992	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
 Data File : VV020273.D
 Acq On : 05 Feb 2021 13:28
 Operator : SY/MD
 Sample : VV0205WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK92

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	10.582	2949	2952	2956	rBV3	763	646	0.03%	0.004%
78	10.669	2977	2979	2983	rBV3	526	381	0.02%	0.002%
79	10.749	2999	3004	3007	rBV3	435	412	0.02%	0.002%
80	10.897	3047	3050	3053	rBV2	659	524	0.02%	0.003%
81	11.016	3085	3087	3093	rBV	668	463	0.02%	0.003%
82	11.129	3120	3122	3127	rBV3	350	254	0.01%	0.001%
83	11.170	3132	3135	3136	rBV2	462	217	0.01%	0.001%
84	11.196	3136	3143	3149	rVV5	3400	4701	0.21%	0.026%
85	11.254	3150	3161	3187	rBV	1141743	1748320	77.00%	9.845%
86	11.524	3243	3245	3249	rBV2	341	195	0.01%	0.001%
87	11.543	3249	3251	3253	rVB3	368	135	0.01%	0.001%
88	11.630	3265	3278	3307	rBV	1132982	1768841	77.91%	9.961%
89	11.858	3344	3349	3353	rBV3	664	651	0.03%	0.004%
90	11.955	3376	3379	3380	rBV	282	139	0.01%	0.001%
91	12.019	3397	3399	3401	rVB2	494	163	0.01%	0.001%
92	12.087	3418	3420	3425	rBV2	369	313	0.01%	0.002%
93	12.164	3441	3444	3447	rBV	403	248	0.01%	0.001%
94	12.418	3520	3523	3526	rBV2	372	244	0.01%	0.001%
95	12.656	3591	3597	3607	rVB7	4781	7137	0.31%	0.040%
96	12.781	3633	3636	3637	rBV2	309	156	0.01%	0.001%
97	12.833	3650	3652	3656	rBV	518	336	0.01%	0.002%
98	13.273	3783	3789	3799	rVB5	5234	7931	0.35%	0.045%
99	13.344	3807	3811	3815	rBV4	695	651	0.03%	0.004%
100	13.759	3933	3940	3948	rBV4	5175	7105	0.31%	0.040%




Sum of corrected areas: 17758013

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
Data File : VV020273.D
Acq On : 05 Feb 2021 13:28
Operator : SY/MD
Sample : VV0205WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

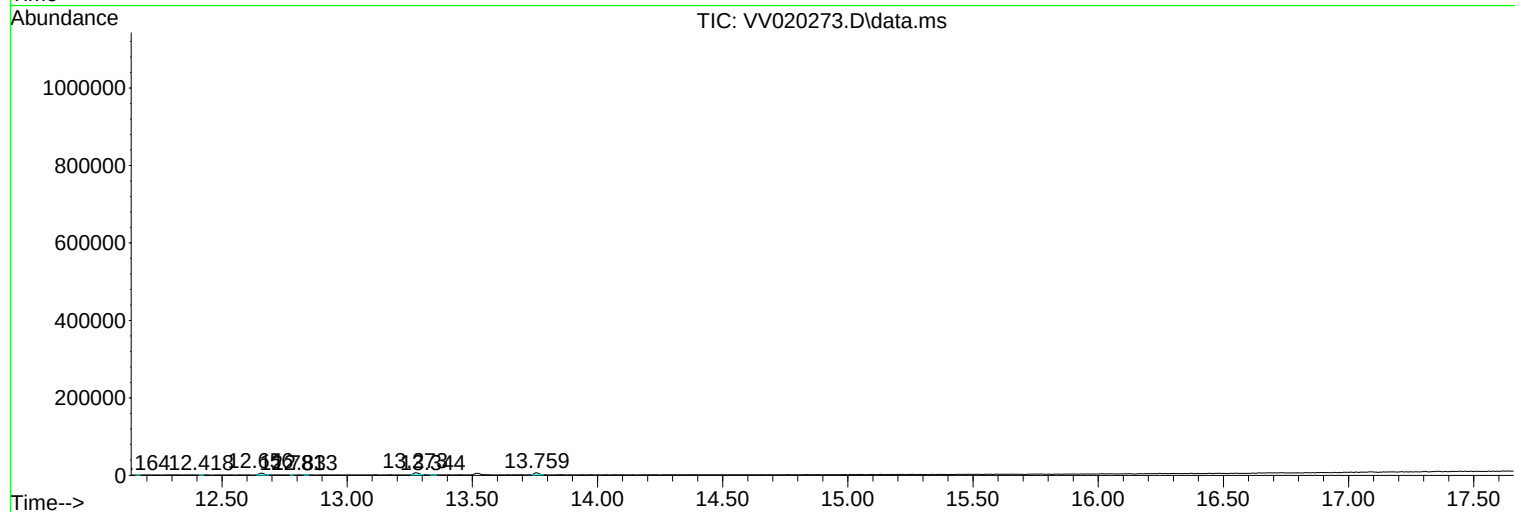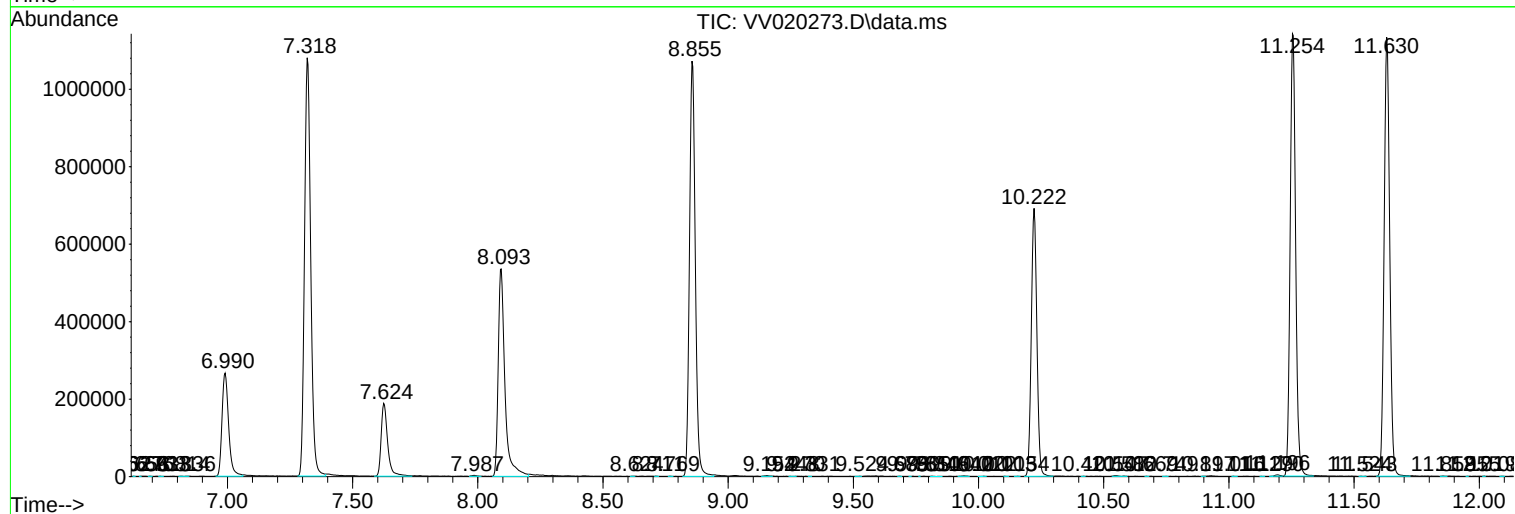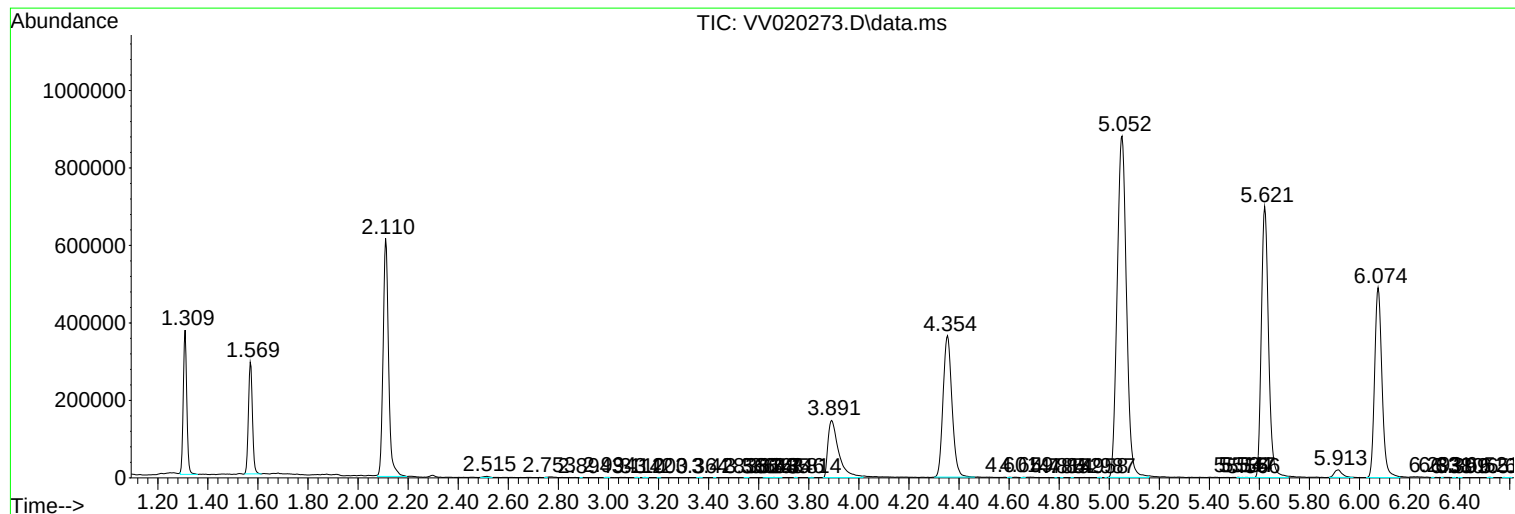

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
Data File : VV020273.D
Acq On : 05 Feb 2021 13:28
Operator : SY/MD
Sample : VV0205WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
Data File : VV020273.D
Acq On : 05 Feb 2021 13:28
Operator : SY/MD
Sample : VV0205WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK92

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
