
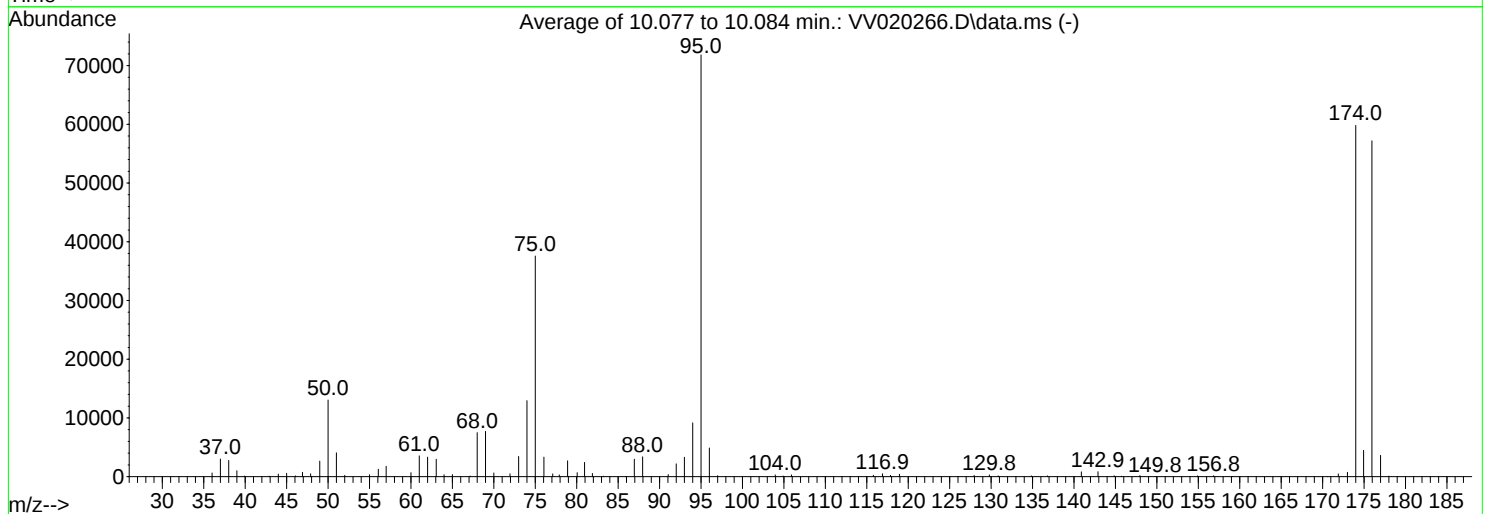


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020521\
 Data File : VV020266.D
 Acq On : 05 Feb 2021 09:13
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis
 Last Update : Fri Feb 05 11:56:25 2021

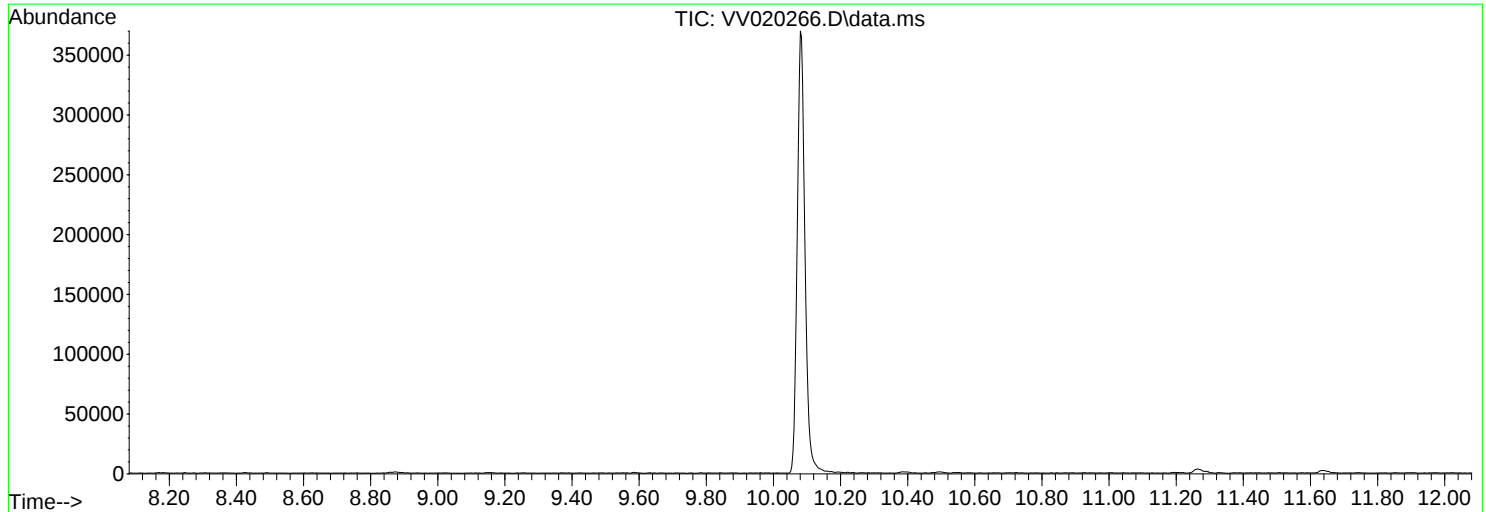

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	13065	PASS
75	95	30	80	52.3	37584	PASS
95	95	100	100	100.0	71829	PASS
96	95	5	9	6.8	4882	PASS
173	174	0.00	2	1.2	731	PASS
174	95	50	120	83.3	59819	PASS
175	174	5	9	7.5	4459	PASS
176	174	95	101	95.6	57184	PASS
177	176	5	9	6.3	3630	PASS

m/z	Abundance
39.10	107.0
39.90	175.0
44.00	469.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	635.0
37.00	2895.0
38.00	2705.0
39.00	963.0
39.90	289.0
44.00	960.0
45.00	515.0
46.00	153.0
46.90	674.0
47.90	521.0
49.00	2582.0
50.00	12710.0
51.00	3927.0
52.00	179.0
55.00	263.0
56.00	1257.0
57.00	1644.0
60.00	685.0
61.00	3391.0
62.00	3181.0
63.00	2753.0
64.00	334.0
65.00	349.0
67.10	175.0
68.00	7325.0
69.00	7148.0
70.00	597.0
71.90	428.0
73.00	3185.0
74.00	12195.0
75.00	35680.0
76.10	3329.0
77.10	460.0
77.90	264.0
78.90	2534.0
80.10	664.0
81.00	2352.0
81.90	481.0
87.00	2934.0
88.00	3277.0
91.10	396.0
92.00	2143.0
93.00	3094.0
94.00	8714.0
95.00	67672.0
96.00	4887.0
97.00	175.0
104.00	280.0
104.90	136.0
105.90	253.0
110.90	104.0
115.80	230.0
116.90	495.0
117.90	217.0
119.00	353.0
128.00	218.0
129.80	322.0
130.90	129.0
134.80	136.0
136.80	151.0
140.90	783.0
142.90	775.0
144.90	158.0
145.70	154.0
148.00	191.0
154.80	127.0
156.90	158.0
171.80	395.0
173.00	734.0
174.00	54736.0
174.90	4225.0
175.90	52312.0
177.00	3408.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	650.0
37.00	3144.0
38.00	2874.0
39.00	1160.0
39.90	300.0
42.90	101.0
44.00	919.0
45.00	578.0
46.10	128.0
46.90	769.0
47.90	491.0
49.00	2696.0
50.00	13551.0
51.00	4193.0
52.00	213.0
55.00	357.0
56.00	1276.0
57.00	1806.0
60.00	698.0
61.00	3673.0
62.00	3426.0
63.10	3099.0
64.00	355.0
65.00	382.0
67.20	195.0
68.00	7826.0
69.00	8065.0
70.00	675.0
72.00	514.0
73.00	3522.0
74.00	13458.0
75.00	39088.0
76.00	3450.0
77.10	488.0
77.90	286.0
78.90	2818.0
80.10	686.0
81.00	2444.0
81.90	538.0
83.20	146.0
85.90	104.0
87.00	3056.0
87.90	3556.0
91.00	364.0
92.00	2222.0
93.00	3394.0
94.00	9534.0
95.00	74528.0
96.00	5100.0
97.00	180.0
104.00	310.0
104.90	128.0
105.90	318.0
111.00	103.0
115.80	262.0
116.90	523.0
117.90	226.0
118.90	442.0
128.00	236.0
129.80	318.0
130.90	164.0
134.80	138.0
136.80	161.0
140.90	813.0
142.90	893.0
144.90	185.0
145.80	122.0
147.90	204.0
154.90	148.0
156.80	188.0
170.60	101.0
171.90	448.0
173.00	774.0
174.00	62128.0
175.00	4634.0
175.90	59280.0
177.00	3763.0
178.00	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
36.00	563.0
37.00	2965.0
38.00	2692.0
39.00	1219.0
39.90	276.0
41.00	108.0
42.90	120.0
44.00	866.0
45.00	597.0
46.10	102.0
46.90	802.0
47.90	441.0
49.00	2624.0
50.00	12933.0
51.00	4028.0
52.00	232.0
55.00	351.0
56.10	1235.0
57.00	1854.0
60.00	639.0
61.00	3563.0
62.00	3389.0
63.10	3033.0
64.00	320.0
65.00	358.0
68.00	7344.0
69.00	7928.0
70.00	652.0
72.00	506.0
73.00	3597.0
74.00	13193.0
75.00	37984.0
76.00	3220.0
77.10	430.0
77.90	316.0
78.90	2737.0
80.00	718.0
80.90	2469.0
81.90	594.0
83.20	118.0
86.90	2934.0
88.00	3273.0
91.00	313.0
92.00	2140.0
93.00	3392.0
94.00	9204.0
95.00	73288.0
96.00	4659.0
97.00	153.0
103.90	344.0
104.90	100.0
105.90	356.0
111.90	104.0
115.00	106.0
115.80	268.0
116.90	467.0
117.80	247.0
118.90	444.0
126.00	113.0
127.80	239.0
129.80	291.0
130.80	143.0
134.90	142.0
136.80	127.0
140.90	854.0
142.90	897.0
144.80	169.0
147.90	170.0
149.80	119.0
155.00	149.0
156.80	172.0
159.10	115.0
161.00	119.0
172.00	530.0
173.00	685.0
174.00	62592.0
175.00	4518.0
176.00	59960.0
177.00	3718.0
178.00	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86