

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020620\
 Data File : VV014518.D
 Acq On : 06 Feb 2020 14:29
 Operator : SY/MD
 Sample : VV0206WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Quant Time: Feb 07 01:50:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Quant Title : VOC Analysis
 QLast Update : Fri Feb 07 01:37:17 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	385807	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	359088	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.29	152	174664	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	98695	47.17	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.34%
7) Chloroethane-d5	1.58	69	70622	48.98	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	97.96%
11) 1,1-Dichloroethene-d2	2.13	63	116129	36.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.10%
21) 2-Butanone-d5	3.92	46	168435	104.29	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.29%
24) Chloroform-d	4.40	84	233606	49.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.08	65	150362	51.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.34%
32) Benzene-d6	5.10	84	504332	50.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.44%
36) 1,2-Dichloropropane-d6	6.11	67	157495	51.66	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.32%
41) Toluene-d8	7.36	98	463242	50.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.20%
43) trans-1,3-Dichloropropene-	7.66	79	81462	49.83	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.66%
47) 2-Hexanone-d5	8.13	63	128993	99.45	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.45%
56) 1,1,2,2-Tetrachloroethane-	10.25	84	204388	51.62	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.24%
66) 1,2-Dichlorobenzene-d4	11.67	152	173951	51.93	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.86%


Target Compounds					Ovalue
13) Acetone	2.19	43	4408	3.260 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020620\
Data File : VV014518.D
Acq On : 06 Feb 2020 14:29
Operator : SY/MD
Sample : VV0206WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Time: Feb 07 01:50:12 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis
QLast Update : Fri Feb 07 01:37:17 2020
Response via : Initial Calibration

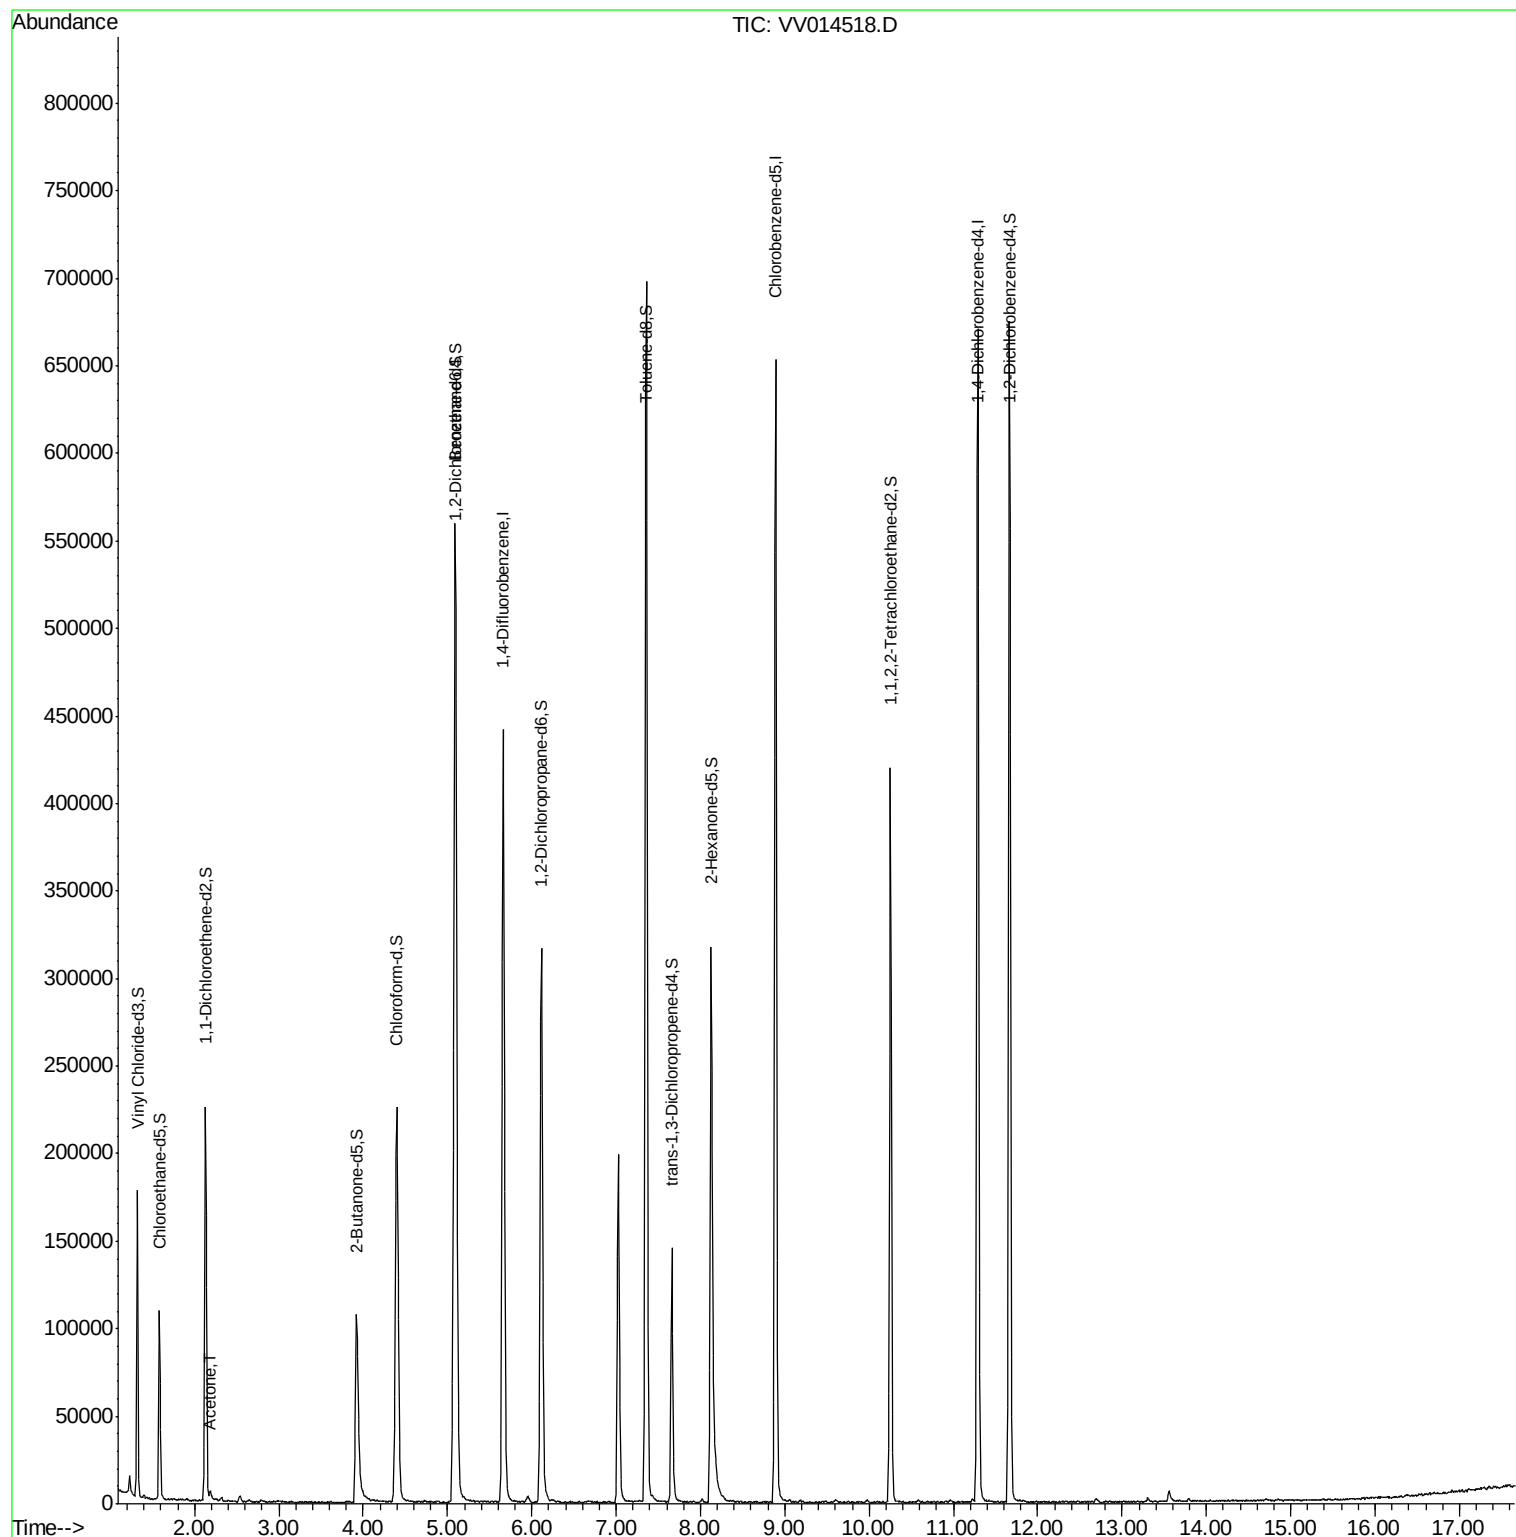

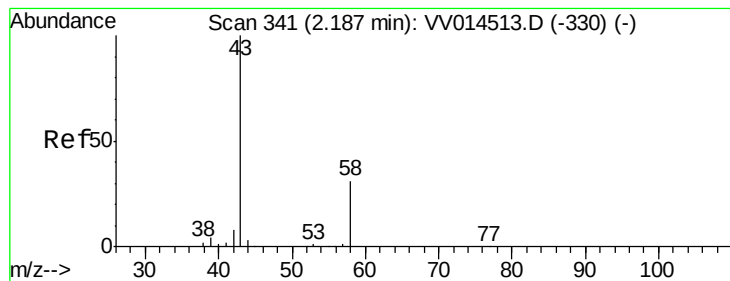

#13
 Acetone
 Concen: 3.260 ug/L
 RT: 2.19 min Scan# 341
 Delta R.T. 0.00 min
 Lab File: VV014518.D
 Acq: 06 Feb 2020 14:29

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Tot Ion: 43 Resp: 4408
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 61.8

