

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020620\
 Data File : VV014518.D
 Acq On : 06 Feb 2020 14:29
 Operator : SY/MD
 Sample : VV0206WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	81	rVB	174548	168091	11.82%	1.563%
2	1.582	146	153	169	rVB	107595	130060	9.14%	1.209%
3	1.971	270	274	278	rBV5	1017	966	0.07%	0.009%
4	2.132	313	324	335	rBV	224749	322868	22.70%	3.002%
5	2.383	399	402	404	rBV2	653	489	0.03%	0.005%
6	2.537	442	450	460	rBV7	3492	6484	0.46%	0.060%
7	2.618	472	475	477	rBV2	699	357	0.03%	0.003%
8	2.647	480	484	488	rBV5	1064	1221	0.09%	0.011%
9	2.775	521	524	525	rBV3	491	283	0.02%	0.003%
10	2.881	554	557	564	rVB4	672	609	0.04%	0.006%
11	2.978	580	587	588	rBV2	564	630	0.04%	0.006%
12	3.196	652	655	657	rBV2	367	268	0.02%	0.002%
13	3.331	695	697	701	rVB3	543	286	0.02%	0.003%
14	3.357	701	705	711	rBV2	524	521	0.04%	0.005%
15	3.386	711	714	716	rBV3	576	294	0.02%	0.003%
16	3.425	721	726	728	rVB3	376	278	0.02%	0.003%
17	3.470	738	740	749	rVB2	510	538	0.04%	0.005%
18	3.511	749	753	756	rBV2	576	417	0.03%	0.004%
19	3.579	770	774	775	rBV	639	328	0.02%	0.003%
20	3.637	789	792	794	rBV	292	256	0.02%	0.002%
21	3.794	840	841	844	rVB2	570	258	0.02%	0.002%
22	3.920	870	880	911	rVV	107184	274229	19.28%	2.549%
23	4.396	1008	1028	1054	rBV	225542	552543	38.84%	5.137%
24	4.601	1090	1092	1096	rBV3	531	390	0.03%	0.004%
25	4.653	1106	1108	1112	rBV3	453	333	0.02%	0.003%
26	4.695	1117	1121	1123	rBV3	607	465	0.03%	0.004%
27	4.714	1123	1127	1129	rBV3	697	560	0.04%	0.005%
28	4.727	1129	1131	1134	rBV3	781	457	0.03%	0.004%
29	4.782	1146	1148	1152	rVB	754	472	0.03%	0.004%
30	4.804	1154	1155	1158	rBV	465	313	0.02%	0.003%
31	4.865	1171	1174	1178	rBV3	610	542	0.04%	0.005%
32	5.016	1219	1221	1223	rBV	707	369	0.03%	0.003%
33	5.093	1227	1245	1268	rBV2	559019	1422487	100.00%	13.225%
34	5.386	1333	1336	1338	rBV2	604	431	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020620\
 Data File : VV014518.D
 Acq On : 06 Feb 2020 14:29
 Operator : SY/MD
 Sample : VV0206WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

35	5.470	1360	1362	1368	rVB4	541	429	0.03%	0.004%
36	5.560	1387	1390	1392	rBV2	460	259	0.02%	0.002%
37	5.589	1396	1399	1403	rBV3	431	288	0.02%	0.003%
38	5.659	1408	1421	1453	rBV	441146	875416	61.54%	8.139%
39	6.113	1546	1562	1593	rBV	316538	649268	45.64%	6.036%
40	6.296	1616	1619	1624	rBV4	663	408	0.03%	0.004%
41	6.396	1647	1650	1653	rBV3	448	327	0.02%	0.003%
42	6.453	1664	1668	1669	rBV2	485	245	0.02%	0.002%
43	6.479	1673	1676	1681	rVB3	502	329	0.02%	0.003%
44	6.553	1696	1699	1701	rBV2	530	386	0.03%	0.004%
45	6.653	1727	1730	1731	rBV	431	238	0.02%	0.002%
46	6.769	1762	1766	1769	rBV3	587	449	0.03%	0.004%
47	6.852	1789	1792	1794	rBV	516	291	0.02%	0.003%
48	6.929	1813	1816	1819	rVB3	549	364	0.03%	0.003%
49	7.026	1834	1846	1871	rBV	198912	355143	24.97%	3.302%
50	7.206	1899	1902	1905	rBV3	556	369	0.03%	0.003%
51	7.273	1921	1923	1927	rBV2	948	670	0.05%	0.006%
52	7.357	1936	1949	1968	rBV	696909	1208828	84.98%	11.238%
53	7.659	2031	2043	2061	rBV	145359	243016	17.08%	2.259%
54	7.820	2091	2093	2097	rBV2	457	320	0.02%	0.003%
55	7.913	2114	2122	2128	rVB8	1060	1028	0.07%	0.010%
56	7.939	2128	2130	2133	rBV	346	258	0.02%	0.002%
57	7.974	2138	2141	2144	rBV2	344	235	0.02%	0.002%
58	8.023	2150	2156	2161	rVB6	1708	2065	0.15%	0.019%
59	8.090	2174	2177	2178	rBV2	416	230	0.02%	0.002%
60	8.125	2178	2188	2226	rVV	317284	660848	46.46%	6.144%
61	8.412	2275	2277	2280	rVB2	629	319	0.02%	0.003%
62	8.428	2280	2282	2285	rBV2	381	247	0.02%	0.002%
63	8.531	2309	2314	2317	rBV3	606	465	0.03%	0.004%
64	8.598	2331	2335	2339	rVB2	517	400	0.03%	0.004%
65	8.653	2347	2352	2356	rBV3	793	735	0.05%	0.007%
66	8.740	2376	2379	2383	rVB3	484	310	0.02%	0.003%
67	8.762	2383	2386	2389	rVB2	471	302	0.02%	0.003%
68	8.794	2393	2396	2398	rVB2	439	244	0.02%	0.002%
69	8.891	2413	2426	2459	rBV	652538	1057734	74.36%	9.834%
70	9.048	2473	2475	2477	rBV	993	476	0.03%	0.004%
71	9.119	2494	2497	2498	rBV	528	262	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020620\
 Data File : VV014518.D
 Acq On : 06 Feb 2020 14:29
 Operator : SY/MD
 Sample : VV0206WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK202

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

72	9.183	2508	2517	2520	rBV5	1690	2242	0.16%	0.021%
73	9.408	2584	2587	2590	rVB2	534	275	0.02%	0.003%
74	9.441	2594	2597	2599	rBV3	573	255	0.02%	0.002%
75	9.553	2630	2632	2635	rBV2	649	366	0.03%	0.003%
76	9.579	2637	2640	2641	rBV	812	446	0.03%	0.004%
77	9.707	2677	2680	2683	rBV3	510	416	0.03%	0.004%
78	9.804	2708	2710	2716	rVB3	706	519	0.04%	0.005%
79	9.910	2739	2743	2745	rBV2	608	357	0.03%	0.003%
80	10.161	2817	2821	2822	rBV	468	228	0.02%	0.002%
81	10.254	2838	2850	2869	rBV	419558	658520	46.29%	6.122%
82	10.572	2943	2949	2950	rBV2	882	765	0.05%	0.007%
83	10.624	2962	2965	2966	rBV3	579	357	0.03%	0.003%
84	10.762	3004	3008	3010	rBV3	591	381	0.03%	0.004%
85	10.868	3038	3041	3045	rBV	423	262	0.02%	0.002%
86	10.897	3046	3050	3054	rBV2	651	628	0.04%	0.006%
87	11.183	3136	3139	3142	rBV2	405	252	0.02%	0.002%
88	11.225	3146	3152	3155	rBV5	2072	2148	0.15%	0.020%
89	11.289	3160	3172	3193	rBV	669460	1056346	74.26%	9.821%
90	11.566	3256	3258	3261	rBV3	405	256	0.02%	0.002%
91	11.665	3276	3289	3308	rBV	674395	1063038	74.73%	9.883%
92	11.913	3364	3366	3370	rBV2	501	326	0.02%	0.003%
93	12.010	3394	3396	3402	rVB2	384	307	0.02%	0.003%
94	12.376	3507	3510	3513	rBV3	453	319	0.02%	0.003%
95	12.437	3526	3529	3532	rBV3	645	342	0.02%	0.003%
96	12.688	3601	3607	3608	rBV5	2039	1755	0.12%	0.016%
97	13.247	3778	3781	3785	rVB2	586	322	0.02%	0.003%
98	13.270	3786	3788	3791	rBV2	583	414	0.03%	0.004%
99	13.556	3872	3877	3889	rVB3	5274	9435	0.66%	0.088%
100	13.791	3944	3950	3958	rBV7	1672	2669	0.19%	0.025%


Sum of corrected areas: 10756240

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020620\
Data File : VV014518.D
Acq On : 06 Feb 2020 14:29
Operator : SY/MD
Sample : VV0206WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

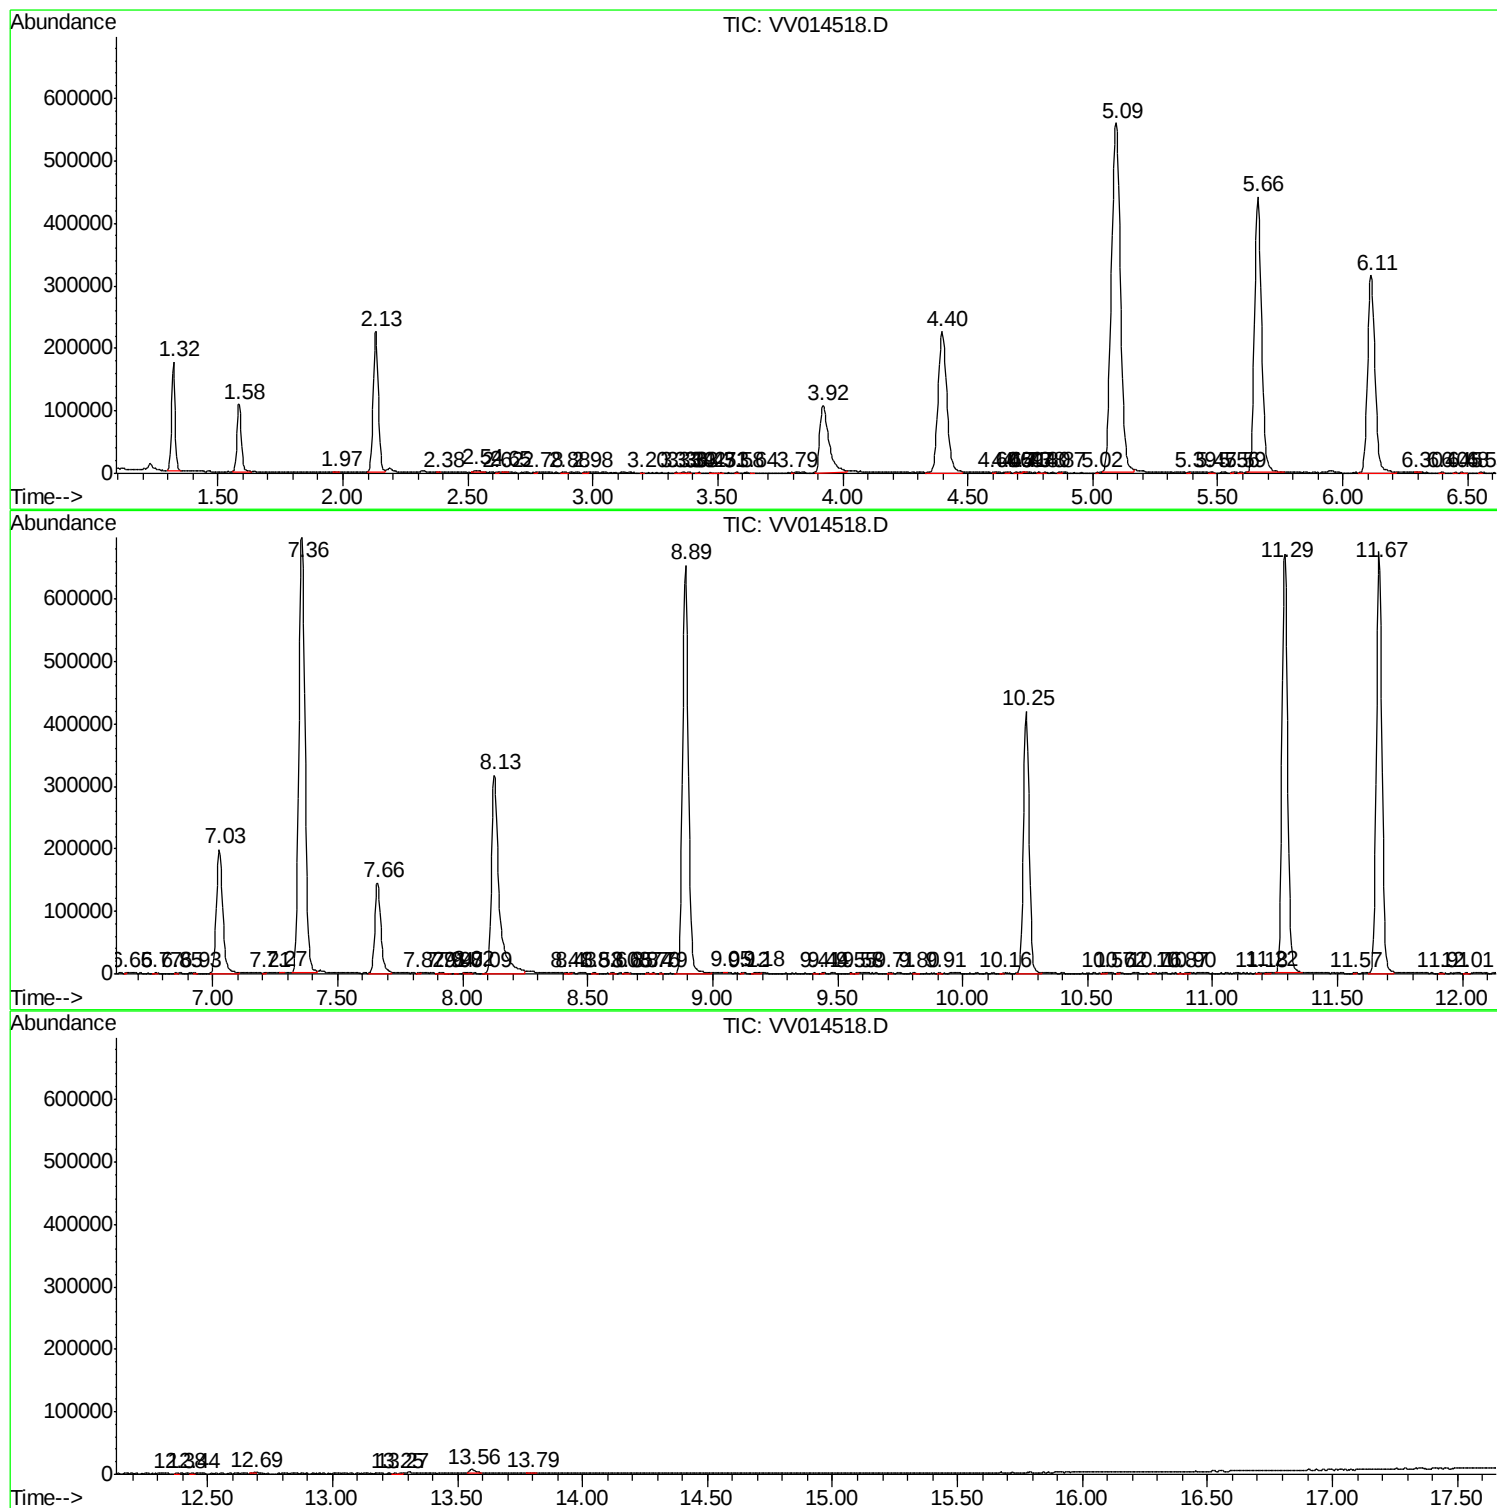

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV020620\
Data File : VV014518.D
Acq On : 06 Feb 2020 14:29
Operator : SY/MD
Sample : VV0206WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK202

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV020620\
Data File : VV014518.D
Acq On : 06 Feb 2020 14:29
Operator : SY/MD
Sample : VV0206WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK202

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc