


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV020620\
 Data File : VV014510.D
 Acq On : 06 Feb 2020 09:34
 Operator : SY/MD
 Sample : BFB88
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB201

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis
 Last Update : Fri Feb 07 01:37:17 2020

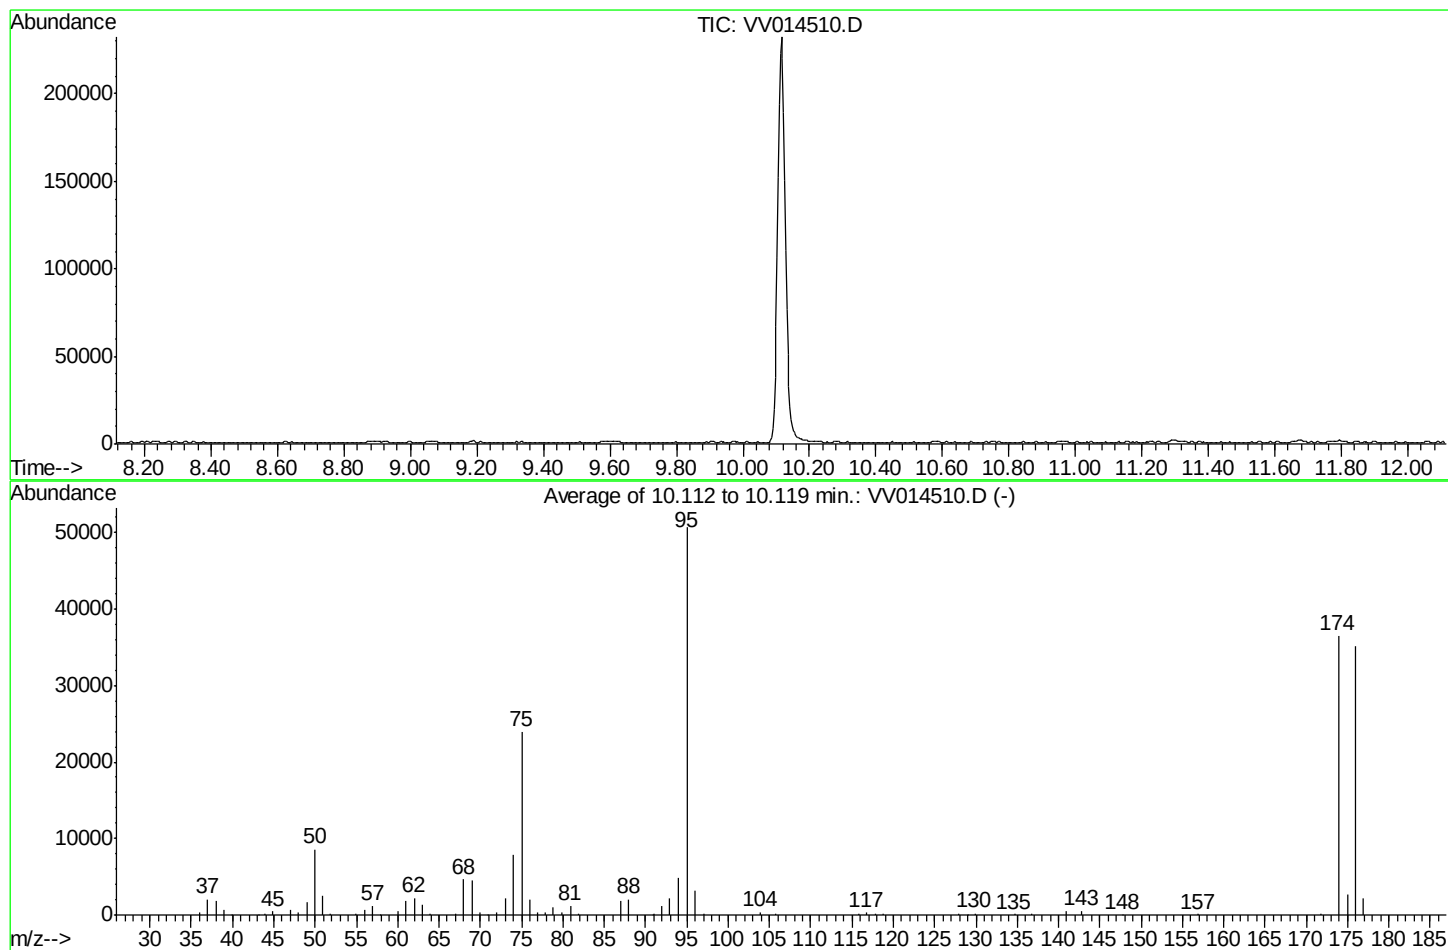

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	8568	PASS
75	95	30	80	47.2	23944	PASS
95	95	100	100	100.0	50677	PASS
96	95	5	9	6.5	3269	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.1	36544	PASS
175	174	5	9	7.6	2762	PASS
176	174	95	101	96.3	35197	PASS
177	176	5	9	6.4	2248	PASS

m/z	Abundance
35.90	335.0
37.00	2142.0
38.00	1882.0
38.90	724.0
39.90	383.0
43.10	106.0
43.90	694.0
44.90	413.0
47.00	576.0
48.00	344.0
49.10	1598.0
50.00	8564.0
51.00	2396.0
51.90	160.0
55.00	204.0
56.00	715.0
57.00	1300.0
60.00	453.0
61.00	1842.0
62.00	2219.0
63.00	1410.0
64.00	179.0
66.90	143.0
68.00	4572.0
69.00	4656.0
69.90	394.0
72.00	307.0
73.00	2230.0
74.00	7902.0
75.00	24008.0
76.00	2052.0
77.00	329.0
77.90	251.0
78.90	1065.0
79.90	311.0
80.90	1209.0
81.90	290.0
87.00	1827.0
87.90	2125.0
90.80	202.0
91.90	1274.0
93.00	2018.0
94.00	4702.0
95.00	50128.0
96.00	3455.0
97.20	141.0
104.00	351.0
105.70	173.0
115.80	221.0
116.80	331.0
117.90	179.0
118.80	246.0
127.80	203.0
129.00	115.0
129.90	204.0
134.70	102.0
136.70	132.0
140.90	509.0
142.80	512.0
147.80	110.0
156.80	117.0
171.90	149.0
173.90	35488.0
175.00	2740.0
175.90	34536.0
177.00	2166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	352.0
37.00	2116.0
38.00	1970.0
39.00	739.0
39.90	377.0
44.00	698.0
44.90	493.0
47.00	602.0
48.00	365.0
49.00	1700.0
50.00	8875.0
50.90	2530.0
51.90	173.0
55.00	207.0
56.00	751.0
57.00	1274.0
60.00	480.0
61.00	1805.0
62.00	2354.0
63.00	1433.0
63.90	195.0
67.00	153.0
68.00	4807.0
69.00	4711.0
69.90	393.0
70.90	104.0
72.00	317.0
73.00	2183.0
74.00	8044.0
75.00	24888.0
76.00	1999.0
77.00	370.0
77.90	327.0
78.90	1121.0
79.80	326.0
80.90	1246.0
81.90	249.0
87.00	1952.0
88.00	2167.0
91.00	197.0
91.90	1254.0
93.00	2198.0
94.00	4973.0
95.00	52368.0
96.10	3385.0
97.10	143.0
104.00	367.0
105.80	226.0
115.80	221.0
116.80	317.0
117.90	199.0
118.70	237.0
127.80	189.0
129.90	245.0
134.70	142.0
136.70	136.0
140.90	568.0
142.80	562.0
147.70	104.0
156.90	108.0
171.80	113.0
173.90	37784.0
175.00	2850.0
175.90	36432.0
177.00	2330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

m/z	Abundance
36.00	364.0
37.00	1990.0
38.00	1800.0
39.00	726.0
39.90	360.0
44.00	730.0
44.90	433.0
47.00	603.0
47.90	327.0
49.00	1686.0
50.00	8266.0
50.90	2464.0
51.90	178.0
54.90	178.0
56.00	747.0
56.90	1077.0
57.90	102.0
60.00	429.0
61.00	1688.0
62.00	2219.0
63.00	1346.0
64.00	241.0
67.00	147.0
68.00	4521.0
69.00	4347.0
69.90	376.0
71.90	322.0
73.00	2050.0
74.00	7462.0
75.00	22936.0
76.00	1905.0
77.00	372.0
77.90	383.0
78.80	1061.0
79.80	340.0
80.90	1070.0
81.80	189.0
87.00	1994.0
88.00	1983.0
91.00	238.0
91.90	1193.0
92.90	2125.0
94.00	4853.0
95.00	49536.0
96.00	2967.0
97.00	116.0
103.90	325.0
105.80	245.0
115.90	219.0
116.80	267.0
117.90	198.0
118.70	227.0
127.90	198.0
129.90	245.0
134.60	163.0
136.80	117.0
140.90	554.0
142.90	571.0
157.00	113.0
171.70	106.0
173.90	36360.0
175.00	2696.0
175.90	34624.0
176.90	2248.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201

Scan 2795 (10.077 min): VV014510.D
BFB88

m/z	Abundance
40.00	352.0
40.90	115.0
44.00	538.0

Instrument :
MSVOA_V
ClientSampleId :
BFB201