

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
 Data File : VV034006.D
 Acq On : 06 Feb 2024 12:44
 Operator : SY/MD
 Sample : P1289-02DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rVB	44257	47278	15.76%	1.754%
2	1.532	146	153	165	rBV	39796	48601	16.20%	1.803%
3	2.063	307	318	340	rVB2	106213	176778	58.94%	6.559%
4	2.449	429	438	450	rBV3	3982	6380	2.13%	0.237%
5	3.114	631	645	661	rBV	59777	126108	42.05%	4.679%
6	3.818	855	864	892	rBV	14679	52226	17.41%	1.938%
7	4.253	983	999	1030	rVB	51011	130856	43.63%	4.855%
8	4.513	1064	1080	1100	rBV2	44804	113680	37.90%	4.218%
9	4.960	1204	1219	1247	rBV3	120753	299930	100.00%	11.128%
10	5.535	1387	1398	1419	rBV	99475	205926	68.66%	7.640%
11	5.989	1528	1539	1562	rBV	63496	133700	44.58%	4.960%
12	6.918	1818	1828	1854	rBV2	30547	60519	20.18%	2.245%
13	7.243	1918	1929	1961	rBV	147801	267786	89.28%	9.935%
14	7.561	2018	2028	2047	rBV2	16683	31387	10.46%	1.164%
15	8.027	2165	2173	2222	rBV	90566	227371	75.81%	8.436%
16	8.786	2399	2409	2439	rBV	147918	251377	83.81%	9.326%
17	10.156	2825	2835	2851	rBV	39211	64193	21.40%	2.382%
18	11.185	3146	3155	3180	rBV	150827	239433	79.83%	8.883%
19	11.561	3259	3272	3296	rBV	132775	211854	70.63%	7.860%




Sum of corrected areas: 2695383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034006.D
Acq On : 06 Feb 2024 12:44
Operator : SY/MD
Sample : P1289-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

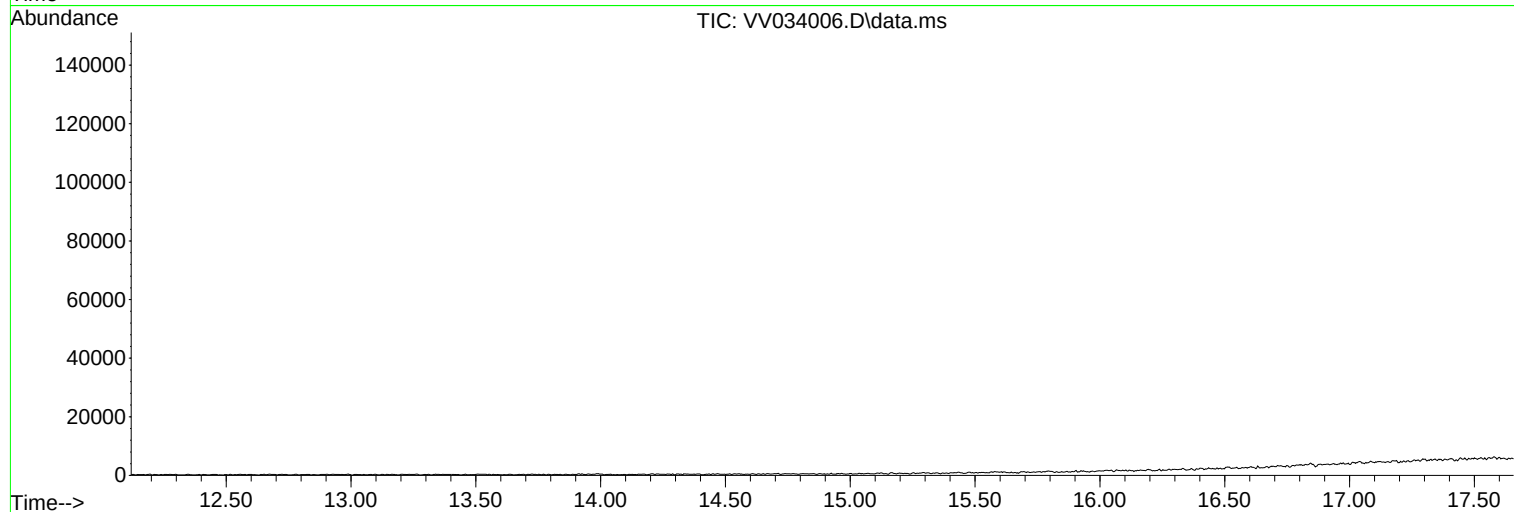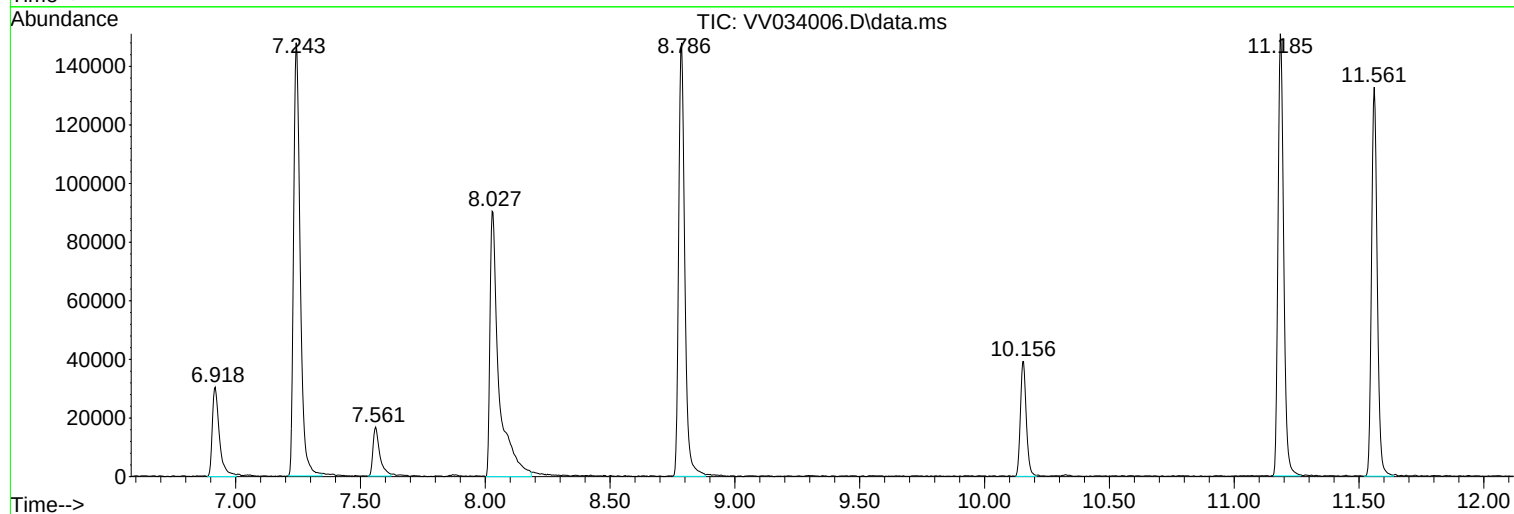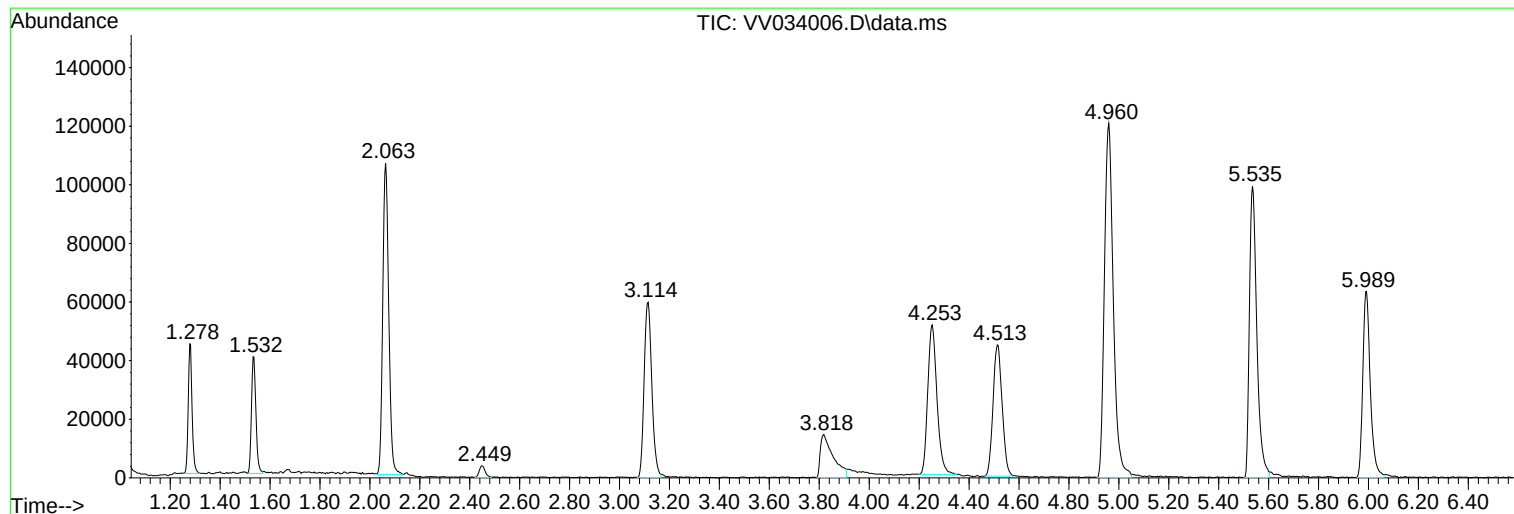

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034006.D
Acq On : 06 Feb 2024 12:44
Operator : SY/MD
Sample : P1289-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034006.D
Acq On : 06 Feb 2024 12:44
Operator : SY/MD
Sample : P1289-02DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc