

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
 Data File : VV034007.D
 Acq On : 06 Feb 2024 13:08
 Operator : SY/MD
 Sample : P1289-04DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AG1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rBV	41600	44639	15.45%	1.688%
2	1.536	146	154	167	rVB	39606	47286	16.37%	1.788%
3	2.063	308	318	335	rBV2	104878	172381	59.66%	6.519%
4	2.452	431	439	450	rVB	4780	7354	2.55%	0.278%
5	3.118	634	646	667	rVB2	7711	16026	5.55%	0.606%
6	3.818	853	864	903	rBV2	14609	56883	19.69%	2.151%
7	4.253	984	999	1023	rVB2	49886	126588	43.81%	4.787%
8	4.513	1063	1080	1101	rBV2	76773	198064	68.55%	7.490%
9	4.960	1204	1219	1243	rBV3	114436	288917	100.00%	10.926%
10	5.535	1387	1398	1423	rBV	101367	210015	72.69%	7.942%
11	5.844	1485	1494	1509	rVB6	2806	6026	2.09%	0.228%
12	5.992	1528	1540	1562	rBV2	62158	131271	45.44%	4.964%
13	6.918	1818	1828	1850	rBV2	29843	57367	19.86%	2.169%
14	7.243	1919	1929	1957	rBV	143873	258377	89.43%	9.771%
15	7.561	2020	2028	2049	rBV2	15652	30239	10.47%	1.144%
16	8.027	2165	2173	2216	rBV	92140	223342	77.30%	8.446%
17	8.786	2399	2409	2432	rBV	152289	253832	87.86%	9.599%
18	10.156	2825	2835	2853	rBV	38478	63942	22.13%	2.418%
19	11.185	3145	3155	3176	rBV	156422	243002	84.11%	9.189%
20	11.561	3260	3272	3299	rBV	131381	208824	72.28%	7.897%




Sum of corrected areas: 2644375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034007.D
Acq On : 06 Feb 2024 13:08
Operator : SY/MD
Sample : P1289-04DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

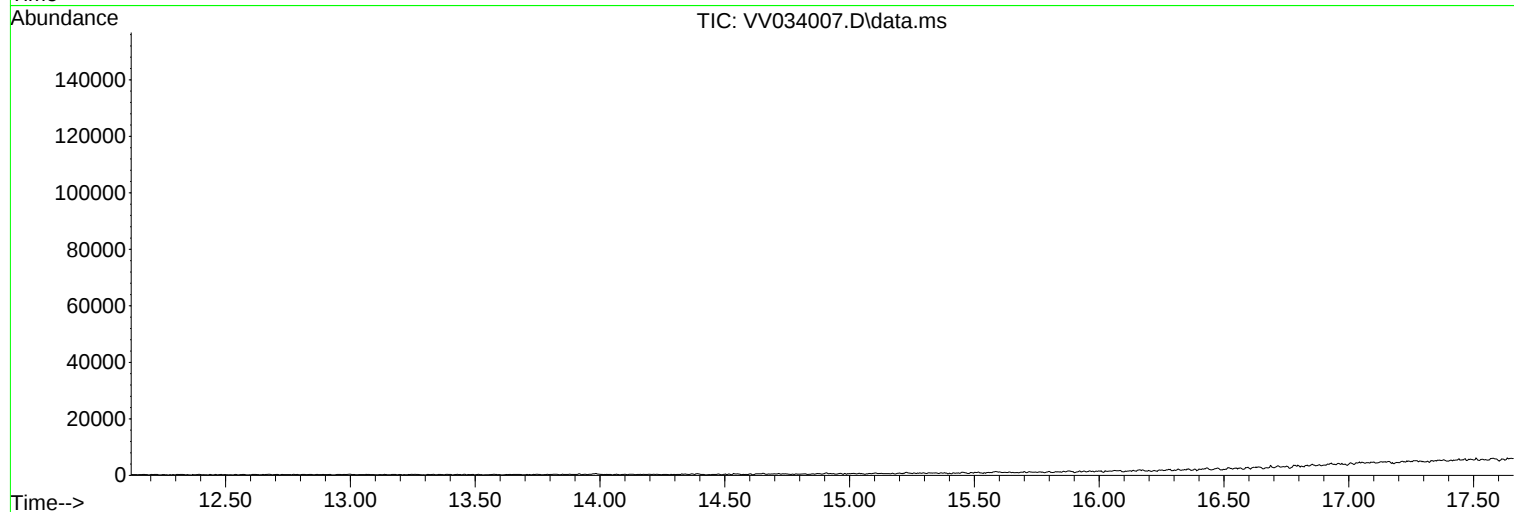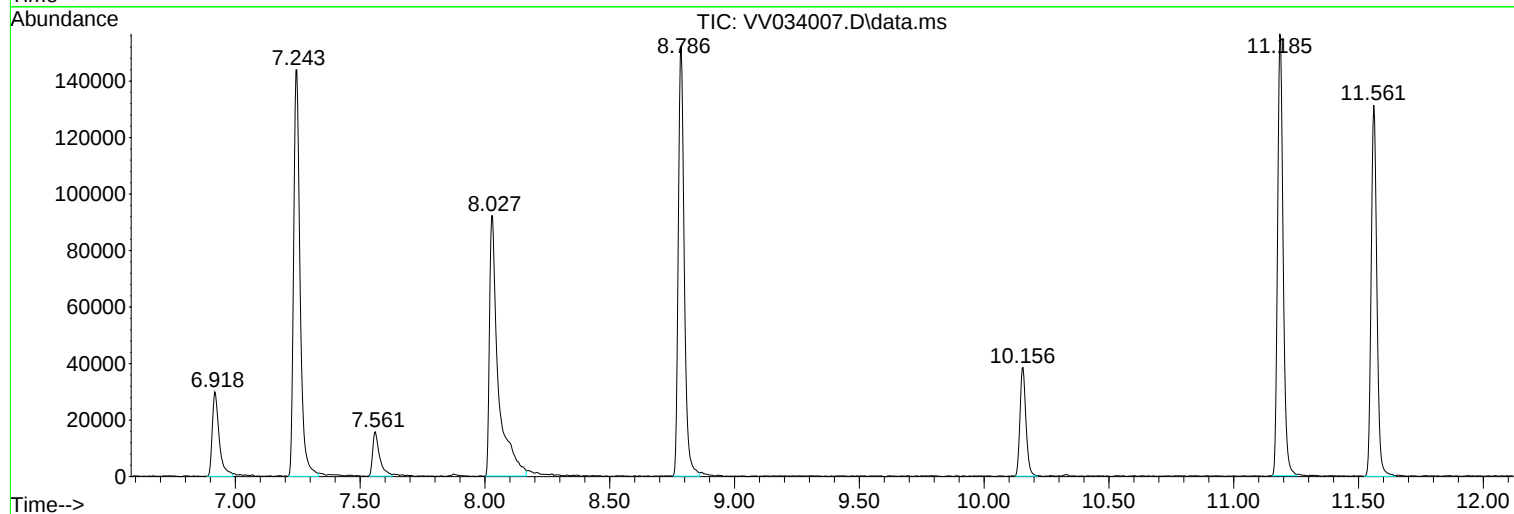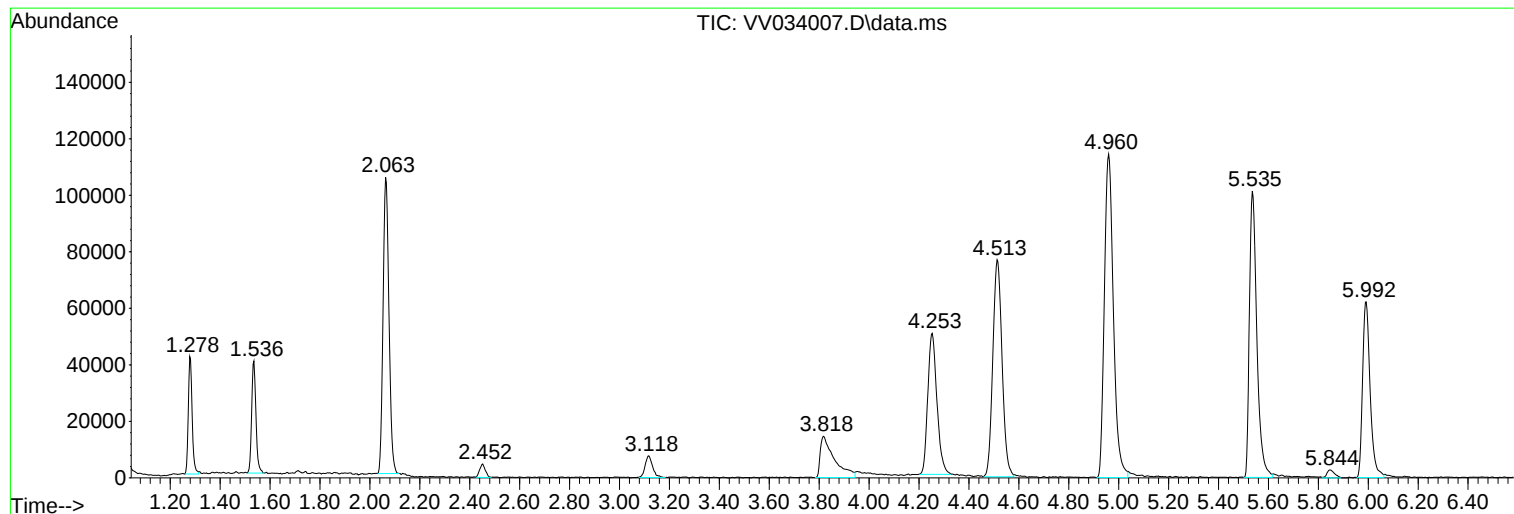

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034007.D
Acq On : 06 Feb 2024 13:08
Operator : SY/MD
Sample : P1289-04DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034007.D
Acq On : 06 Feb 2024 13:08
Operator : SY/MD
Sample : P1289-04DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AG1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc