

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
 Data File : VV034011.D
 Acq On : 06 Feb 2024 15:31
 Operator : SY/MD
 Sample : P1289-12DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	89	rBV	39007	42104	15.17%	1.670%
2	1.532	146	153	168	rBV	37859	45301	16.32%	1.797%
3	2.060	306	317	335	rBV	80081	120338	43.35%	4.774%
4	2.449	428	438	450	rBV2	10748	17715	6.38%	0.703%
5	3.117	633	646	660	rBV2	8537	18056	6.50%	0.716%
6	3.831	858	868	900	rBV2	13779	62988	22.69%	2.499%
7	4.252	984	999	1023	rBV2	47079	120833	43.52%	4.794%
8	4.513	1064	1080	1102	rBV2	50390	131715	47.44%	5.226%
9	4.960	1204	1219	1252	rBV3	110010	277622	100.00%	11.014%
10	5.535	1388	1398	1426	rBV	105763	221326	79.72%	8.781%
11	5.992	1529	1540	1562	rBV2	59320	124014	44.67%	4.920%
12	6.918	1820	1828	1850	rBV2	28029	54308	19.56%	2.155%
13	7.246	1919	1930	1952	rBV	135712	244426	88.04%	9.697%
14	7.561	2020	2028	2047	rBV	13897	27688	9.97%	1.098%
15	8.030	2166	2174	2217	rBV	100377	222280	80.07%	8.819%
16	8.786	2395	2409	2435	rBV	160465	268866	96.85%	10.667%
17	10.152	2825	2834	2849	rBV	36808	60391	21.75%	2.396%
18	11.188	3145	3156	3175	rBV	165585	260278	93.75%	10.326%
19	11.561	3258	3272	3295	rBV	126504	200312	72.15%	7.947%




Sum of corrected areas: 2520561

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034011.D
Acq On : 06 Feb 2024 15:31
Operator : SY/MD
Sample : P1289-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

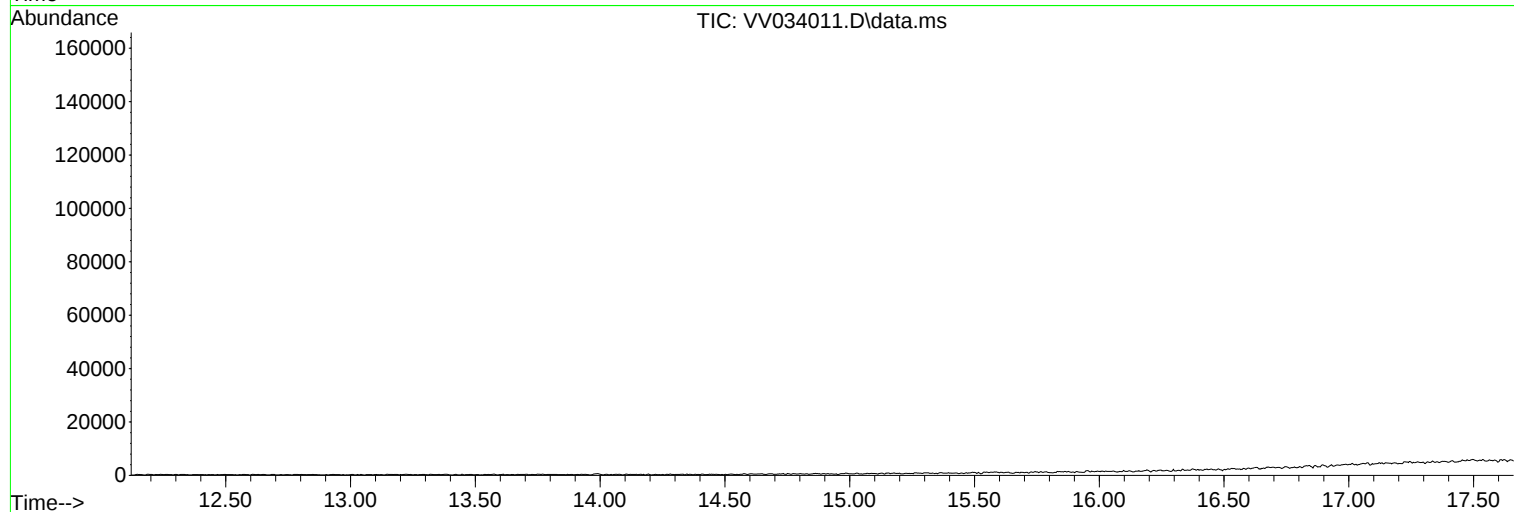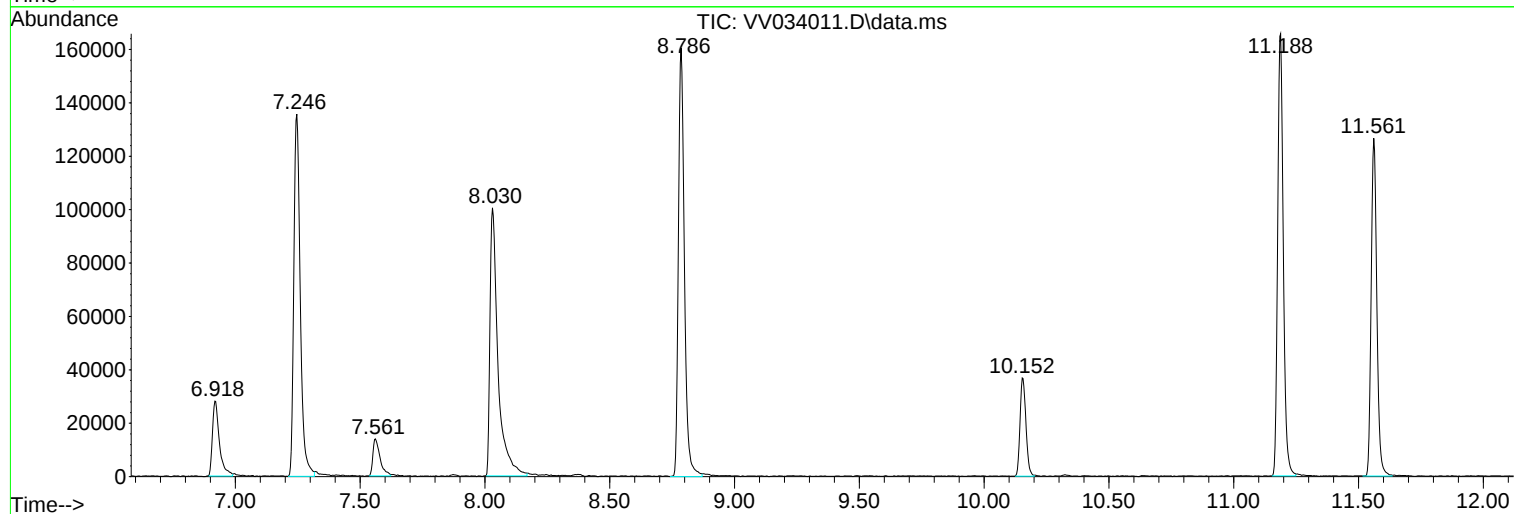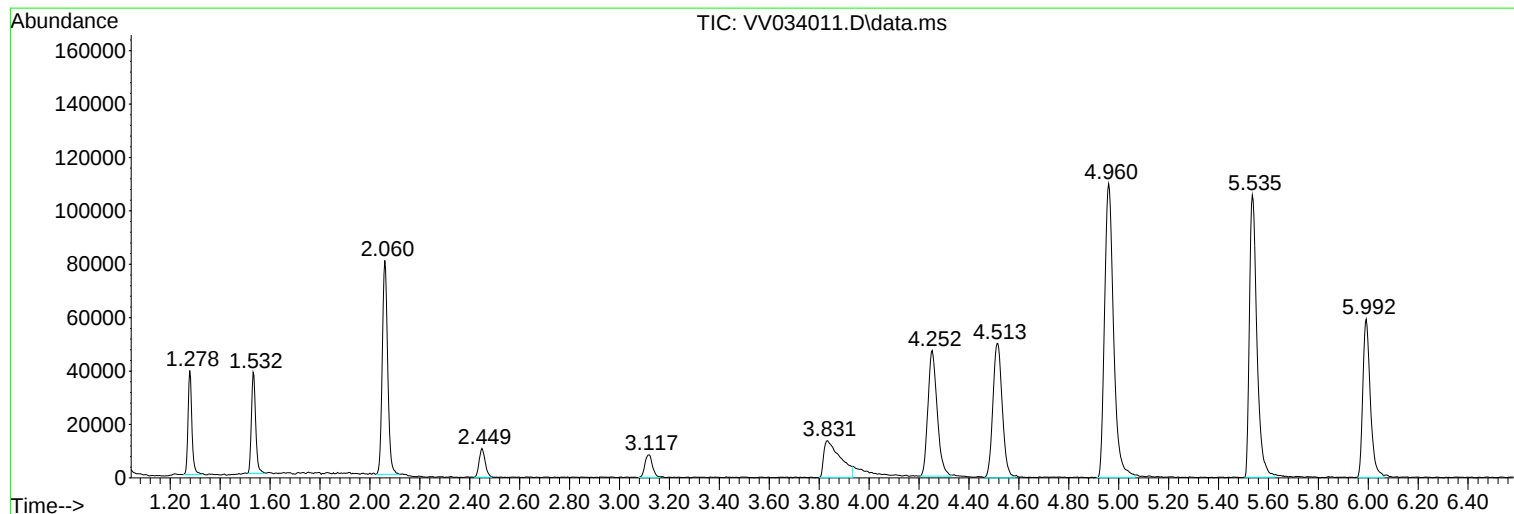

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034011.D
Acq On : 06 Feb 2024 15:31
Operator : SY/MD
Sample : P1289-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034011.D
Acq On : 06 Feb 2024 15:31
Operator : SY/MD
Sample : P1289-12DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc