

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034012.D
Acq On : 06 Feb 2024 15:55
Operator : SY/MD
Sample : P1289-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	87	rBV	39824	42071	14.90%	1.623%
2	1.536	145	154	165	rBV	37576	44803	15.86%	1.728%
3	2.060	307	317	333	rBV	81035	122274	43.29%	4.717%
4	2.449	429	438	452	rBV	11072	18215	6.45%	0.703%
5	3.114	633	645	663	rVB2	2330	4703	1.67%	0.181%
6	3.831	856	868	914	rBV2	13313	74044	26.22%	2.856%
7	4.253	984	999	1025	rBV2	46366	119620	42.35%	4.615%
8	4.513	1063	1080	1106	rBV2	77018	203065	71.90%	7.834%
9	4.960	1202	1219	1256	rBV3	111045	282436	100.00%	10.896%
10	5.535	1388	1398	1430	rBV	102974	213697	75.66%	8.244%
11	5.992	1527	1540	1566	rBV2	60374	127652	45.20%	4.925%
12	6.918	1819	1828	1853	rBV2	27911	56624	20.05%	2.184%
13	7.246	1920	1930	1959	rBV	138948	247466	87.62%	9.547%
14	7.561	2020	2028	2054	rBV2	15344	29257	10.36%	1.129%
15	8.031	2165	2174	2207	rBV	105008	223376	79.09%	8.617%
16	8.786	2398	2409	2437	rBV	159053	261059	92.43%	10.071%
17	10.156	2825	2835	2853	rBV2	39639	62019	21.96%	2.393%
18	11.185	3146	3155	3180	rBV	162396	257609	91.21%	9.938%
19	11.561	3262	3272	3296	rBV	126132	202156	71.58%	7.799%




Sum of corrected areas: 2592146

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034012.D
Acq On : 06 Feb 2024 15:55
Operator : SY/MD
Sample : P1289-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

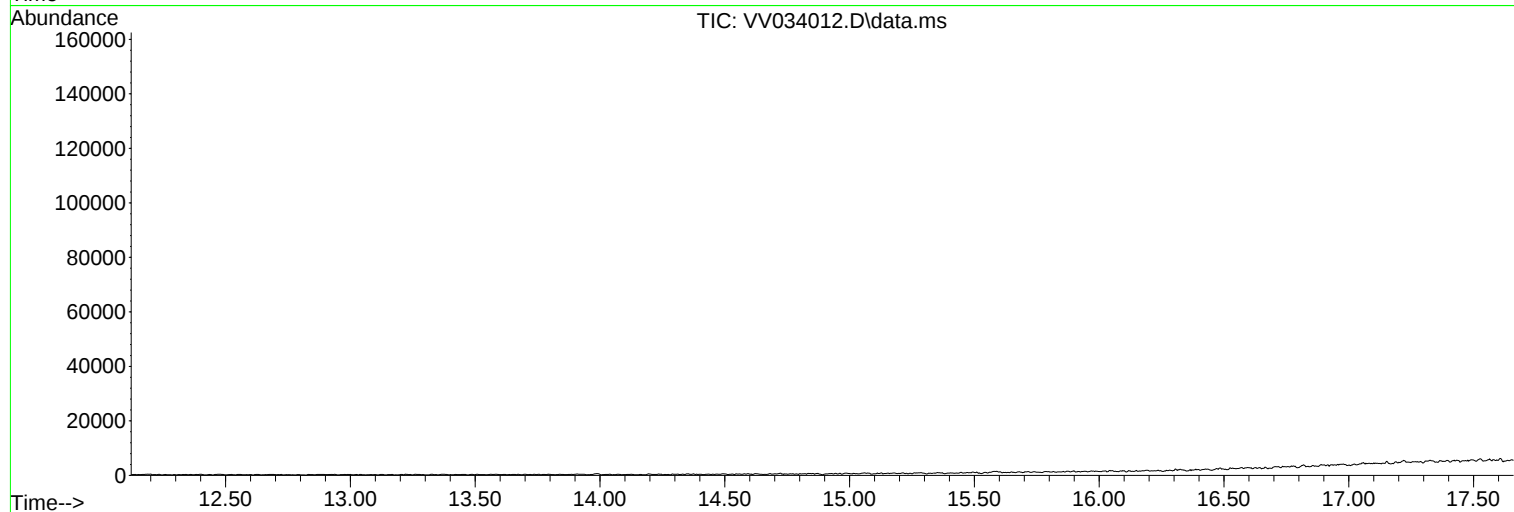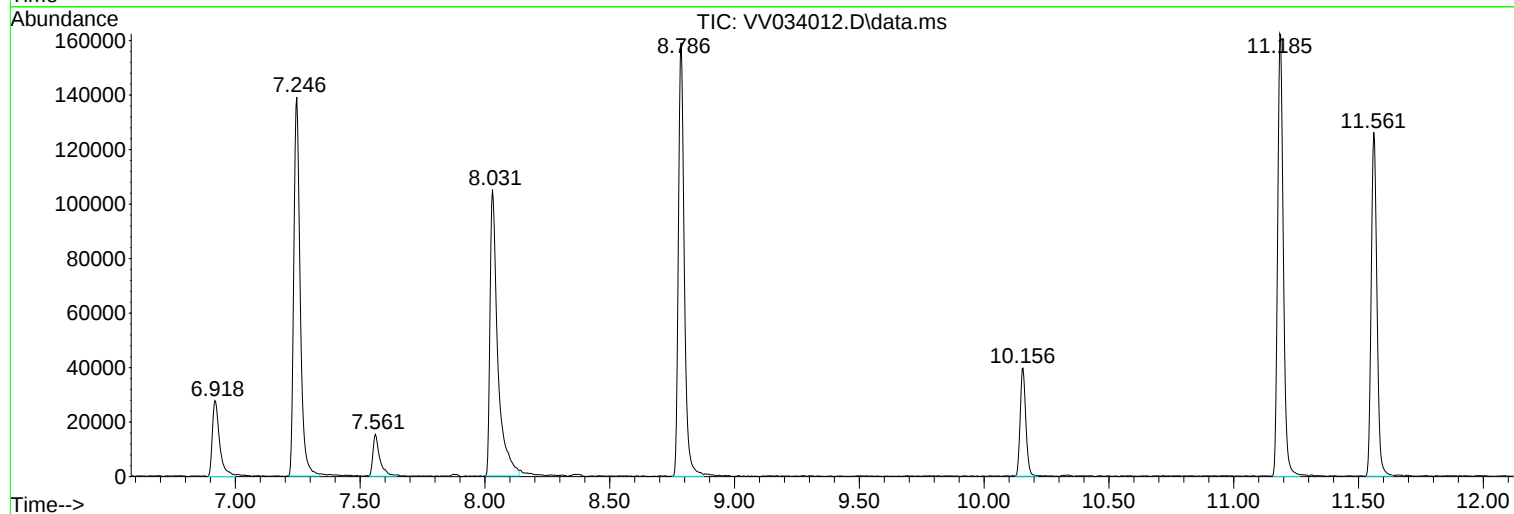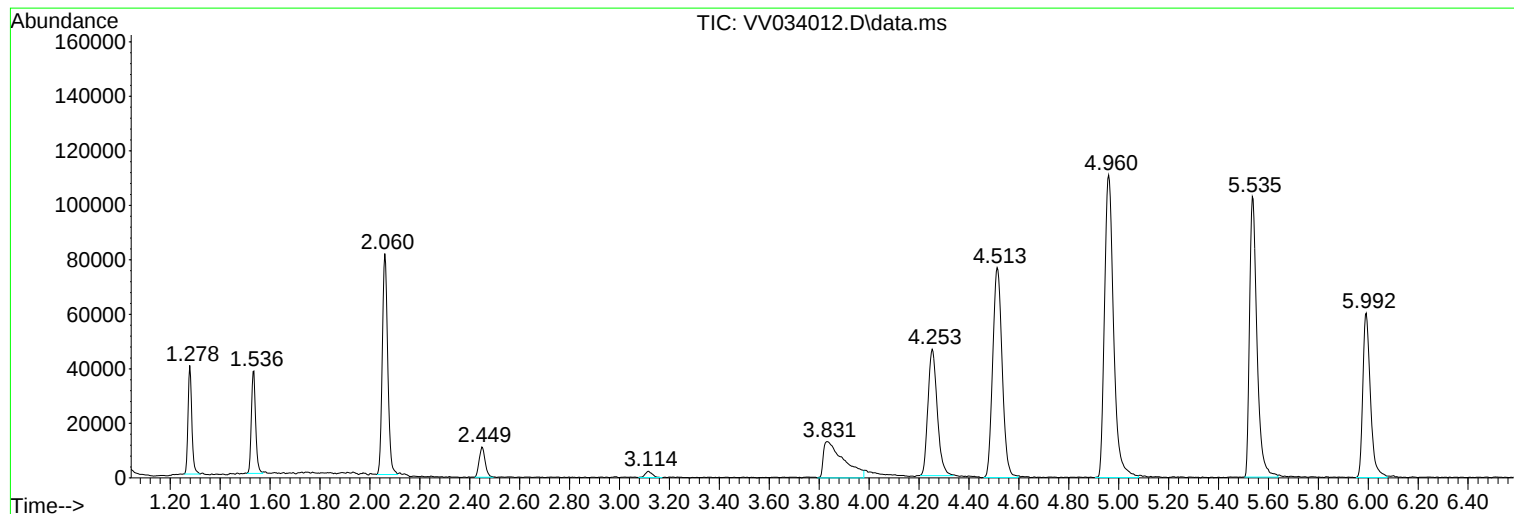

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034012.D
Acq On : 06 Feb 2024 15:55
Operator : SY/MD
Sample : P1289-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034012.D
Acq On : 06 Feb 2024 15:55
Operator : SY/MD
Sample : P1289-13DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc