
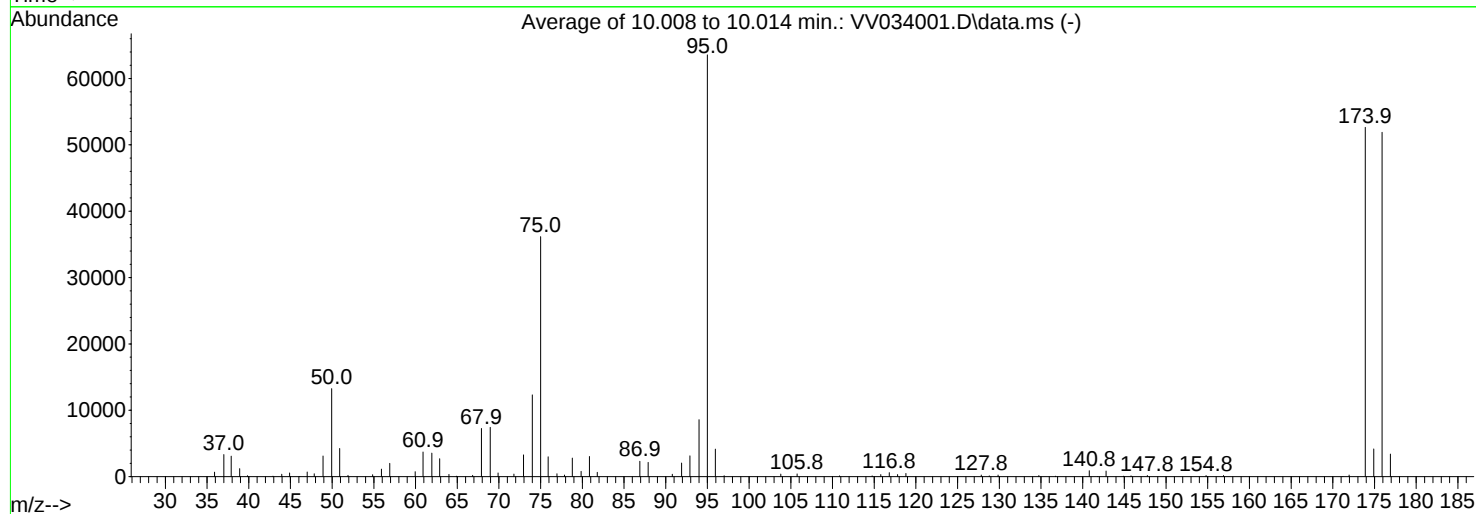


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020624\
Data File : VV034001.D
Acq On : 06 Feb 2024 09:00
Operator : SY/MD
Sample : BFB246
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB246

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Feb 08 04:46:29 2024

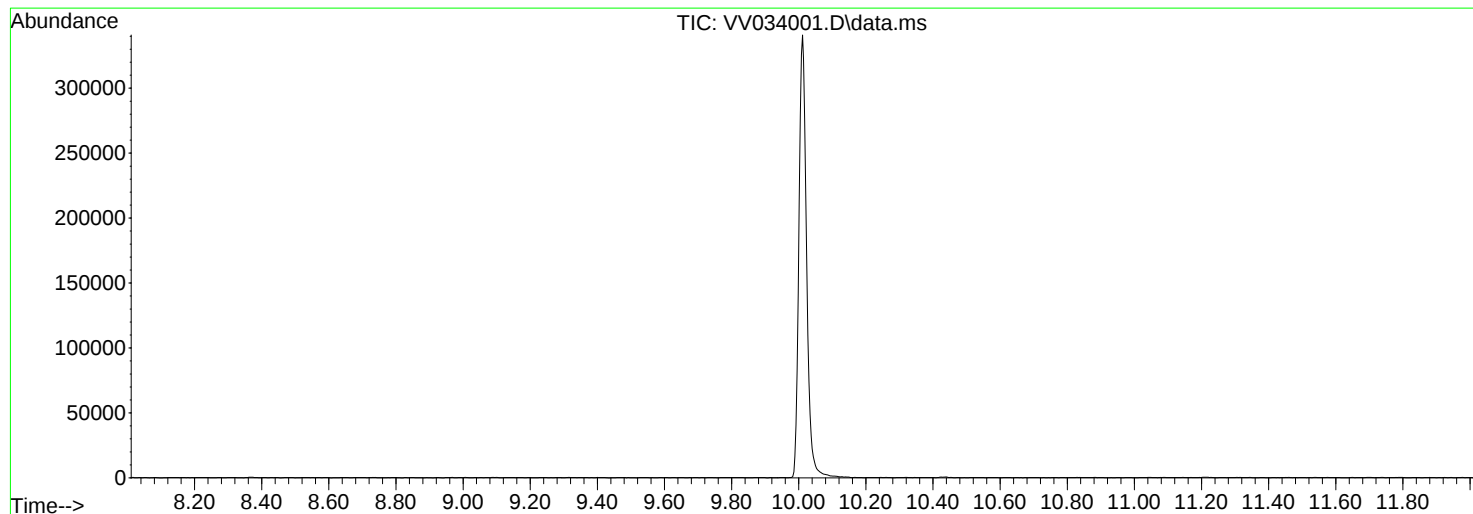

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	13263	PASS
75	95	30	80	56.9	36179	PASS
95	95	100	100	100.0	63565	PASS
96	95	5	9	6.5	4147	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.8	52632	PASS
175	174	5	9	7.9	4161	PASS
176	174	95	105	98.6	51885	PASS
177	176	5	10	6.5	3393	PASS

m/z	Abundance
44.00	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
35.90	654.0
37.00	3341.0
37.90	3194.0
38.90	1276.0
39.80	158.0
43.90	468.0
44.90	584.0
46.10	109.0
47.00	693.0
47.80	475.0
48.90	3149.0
50.00	13649.0
50.90	4274.0
51.90	196.0
54.80	278.0
55.90	1198.0
56.90	1961.0
59.90	707.0
60.90	3636.0
62.00	3617.0
62.90	2663.0
64.00	370.0
64.90	138.0
66.90	207.0
67.90	7214.0
69.00	7425.0
69.90	586.0
71.80	384.0
73.00	3332.0
74.00	12283.0
75.00	36032.0
75.90	3026.0
76.90	433.0
77.80	275.0
78.80	2718.0
79.90	719.0
80.90	2967.0
81.80	659.0
86.90	2296.0
87.90	2247.0
90.80	362.0
91.90	2095.0
92.90	3079.0
94.00	8412.0
95.00	63168.0
95.90	4071.0
97.00	157.0
103.80	396.0
105.70	371.0
110.90	113.0
114.70	107.0
115.80	335.0
116.80	558.0
117.80	305.0
118.80	503.0
127.80	269.0
128.70	151.0
129.80	224.0
134.70	181.0
136.80	106.0
140.80	874.0
142.80	796.0
145.80	110.0
147.80	152.0
154.80	180.0
156.90	137.0
172.00	244.0
173.90	51160.0
174.90	4157.0
175.90	50072.0
176.90	3320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
35.90	700.0
37.00	3466.0
37.90	3220.0
38.90	1236.0
39.80	159.0
42.90	107.0
44.00	492.0
44.90	572.0
47.00	724.0
47.90	464.0
48.90	3241.0
49.90	13693.0
50.90	4385.0
51.90	194.0
54.90	293.0
55.90	1164.0
56.90	2048.0
60.00	774.0
60.90	3849.0
61.90	3689.0
62.90	2752.0
64.00	355.0
64.90	113.0
66.90	182.0
67.90	7533.0
68.90	7690.0
69.90	577.0
71.80	406.0
72.90	3382.0
74.00	12751.0
75.00	37392.0
75.90	3059.0
77.00	453.0
77.90	237.0
78.80	2896.0
79.90	826.0
80.90	3155.0
81.80	673.0
86.90	2361.0
87.90	2199.0
90.80	374.0
91.90	2134.0
92.90	3270.0
94.00	8890.0
95.00	65928.0
96.00	4353.0
97.00	145.0
103.80	409.0
105.80	414.0
110.80	115.0
114.70	121.0
115.80	330.0
116.80	616.0
117.80	342.0
118.80	516.0
127.90	241.0
128.80	122.0
129.90	249.0
134.80	177.0
140.80	911.0
141.80	104.0
142.80	869.0
144.90	104.0
145.80	118.0
147.80	172.0
154.80	188.0
156.90	174.0
171.20	104.0
172.00	253.0
173.90	54424.0
174.90	4282.0
175.90	53496.0
176.90	3525.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246

m/z	Abundance
35.90	654.0
37.00	3191.0
37.90	2876.0
38.90	1096.0
39.90	159.0
42.90	120.0
44.00	532.0
44.90	501.0
47.00	721.0
47.90	402.0
48.90	2947.0
49.90	12447.0
50.90	4092.0
51.90	170.0
54.90	295.0
55.90	1041.0
56.90	1972.0
60.00	779.0
60.90	3691.0
61.90	3330.0
62.90	2714.0
64.00	304.0
66.80	172.0
67.90	7022.0
68.90	7179.0
69.90	538.0
71.80	384.0
72.90	3122.0
74.00	11942.0
75.00	35112.0
75.90	2884.0
77.00	402.0
77.90	217.0
78.80	2792.0
79.80	882.0
80.80	3014.0
81.80	620.0
86.90	2300.0
87.90	2031.0
90.80	358.0
91.90	1954.0
92.90	3062.0
94.00	8464.0
95.00	61600.0
96.00	4017.0
97.00	120.0
103.80	378.0
105.80	423.0
110.80	107.0
114.80	108.0
115.80	294.0
116.80	634.0
117.80	329.0
118.80	455.0
127.80	228.0
128.90	112.0
129.90	265.0
134.80	165.0
136.70	104.0
140.80	925.0
142.80	870.0
144.90	110.0
145.80	108.0
147.70	173.0
154.80	173.0
156.90	170.0
171.90	221.0
173.90	52312.0
174.90	4043.0
175.90	52088.0
176.90	3333.0

Instrument :
MSVOA_V
ClientSampleId :
BFB246