


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV020720\
 Data File : VV014522.D
 Acq On : 06 Feb 2020 16:43
 Operator : SY/MD
 Sample : BFB89
 Misc : 5.00G/10ML/MSVOA V/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB89

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM020720S.M
 Title : VOC Analysis
 Last Update : Fri Feb 07 03:49:49 2020

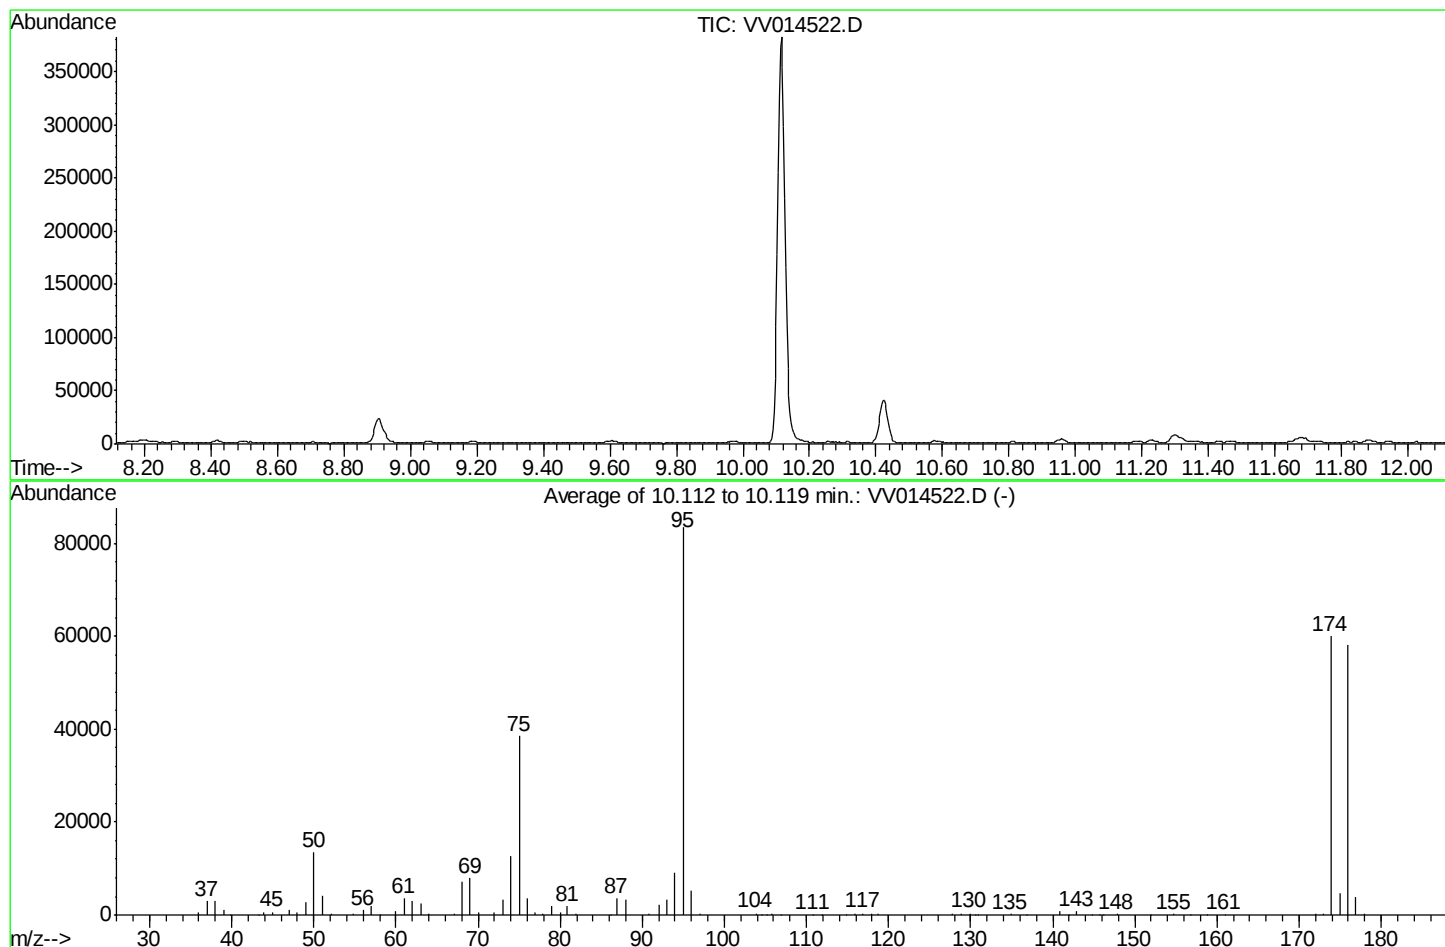

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	13497	PASS
75	95	30	80	46.2	38546	PASS
95	95	100	100	100.0	83472	PASS
96	95	5	9	6.3	5274	PASS
173	174	0.00	2	0.5	271	PASS
174	95	50	120	71.9	60056	PASS
175	174	5	9	7.9	4731	PASS
176	174	95	101	97.0	58245	PASS
177	176	5	9	6.8	3987	PASS

Scan 2794 (10.074 min): VV014522.D
BFB89

m/z	Abundance
39.90	315.0
40.70	137.0
41.30	117.0
43.90	362.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
36.00	578.0
37.00	2796.0
38.00	2708.0
39.00	997.0
39.90	363.0
44.00	938.0
44.90	531.0
46.90	1050.0
47.90	489.0
49.00	2610.0
50.00	12661.0
51.00	3978.0
52.10	193.0
54.80	232.0
56.00	972.0
56.90	1862.0
58.00	110.0
59.90	695.0
61.00	3280.0
62.00	2832.0
63.00	2310.0
64.00	238.0
67.00	253.0
68.00	6754.0
69.00	7505.0
70.10	532.0
72.00	448.0
73.00	3094.0
74.00	11938.0
75.00	36360.0
76.00	3230.0
77.00	502.0
77.90	359.0
78.90	1825.0
80.00	620.0
80.90	1853.0
81.80	386.0
86.10	123.0
86.90	3292.0
88.00	3199.0
90.80	336.0
92.00	2036.0
93.00	3224.0
94.00	8600.0
95.00	79520.0
96.00	4845.0
96.90	136.0
103.90	344.0
104.60	116.0
105.10	102.0
105.80	233.0
106.80	116.0
110.80	109.0
111.80	111.0
114.80	125.0
115.90	265.0
116.90	373.0
118.00	296.0
118.80	323.0
127.70	261.0
128.90	171.0
129.90	304.0
134.90	164.0
136.90	132.0
140.90	710.0
141.90	116.0
142.90	852.0
144.70	102.0
146.10	133.0
147.90	179.0
154.70	226.0
156.70	123.0
160.90	110.0
172.00	251.0
173.90	58752.0
175.00	4514.0
175.90	57192.0
176.90	3765.0
178.00	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
36.00	680.0
37.00	3130.0
38.00	3051.0
39.00	1036.0
39.80	345.0
44.00	927.0
44.90	610.0
47.00	1087.0
48.00	529.0
49.00	2922.0
50.00	14013.0
51.00	4345.0
52.10	203.0
54.80	243.0
56.00	1155.0
56.90	2063.0
58.00	114.0
59.90	724.0
61.00	3589.0
62.00	3243.0
63.00	2434.0
64.00	324.0
67.10	294.0
68.00	7521.0
69.00	8189.0
70.10	616.0
72.00	478.0
73.00	3360.0
74.00	13327.0
75.00	39928.0
76.00	3625.0
77.00	518.0
77.90	411.0
78.90	1953.0
80.00	681.0
80.90	1916.0
81.90	413.0
86.10	134.0
86.90	3597.0
88.00	3454.0
90.90	329.0
92.00	2197.0
93.00	3381.0
94.00	9290.0
95.00	86184.0
96.00	5414.0
97.10	184.0
103.90	390.0
105.80	267.0
106.80	108.0
110.80	101.0
111.90	117.0
114.80	113.0
116.00	253.0
116.90	406.0
118.00	363.0
118.70	305.0
127.70	249.0
128.90	195.0
129.90	314.0
130.50	118.0
130.90	111.0
134.90	171.0
136.80	147.0
140.90	793.0
142.90	818.0
145.60	141.0
146.10	128.0
147.80	239.0
151.90	126.0
154.80	224.0
156.70	125.0
158.80	102.0
160.90	118.0
172.00	232.0
173.90	62152.0
175.00	4960.0
175.90	60176.0
176.90	4159.0
178.00	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89

m/z	Abundance
35.90	698.0
37.00	3108.0
38.00	3177.0
39.00	993.0
39.80	329.0
43.20	119.0
44.00	824.0
44.90	621.0
47.00	1029.0
48.00	511.0
49.00	2938.0
50.00	13819.0
51.00	4350.0
52.10	193.0
54.90	230.0
56.00	1183.0
57.00	2046.0
59.90	695.0
61.00	3623.0
62.00	3360.0
63.00	2375.0
64.00	379.0
67.10	318.0
68.00	7503.0
69.00	7913.0
70.00	617.0
72.00	430.0
73.00	3362.0
74.00	13072.0
75.00	39352.0
76.00	3603.0
77.00	492.0
77.90	442.0
78.90	1882.0
80.00	671.0
80.90	1834.0
81.90	402.0
86.90	3479.0
88.00	3514.0
90.90	252.0
92.00	2026.0
93.00	3203.0
94.00	9152.0
95.00	84712.0
96.00	5565.0
97.10	188.0
103.90	380.0
105.90	298.0
110.80	114.0
115.90	220.0
116.90	412.0
118.00	348.0
118.80	318.0
127.90	274.0
128.90	181.0
129.90	305.0
134.90	162.0
136.80	146.0
140.90	803.0
142.90	780.0
145.70	141.0
147.80	252.0
151.90	122.0
154.80	195.0
156.80	117.0
160.90	112.0
172.10	213.0
173.00	813.0
173.90	59264.0
175.00	4720.0
175.90	57368.0
176.90	4037.0
177.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB89