

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020724\
 Data File : VW034032.D
 Acq On : 07 Feb 2024 15:42
 Operator : SY/MD
 Sample : P1383-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0YB3

Quant Time: Feb 08 04:50:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Feb 08 04:46:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	86044	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	78843	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	40874	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	23923	3.590	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	71.800%	
7) Chloroethane-d5	1.532	69	23074	3.953	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	79.000%	
11) 1,1-Dichloroethene-d2	2.060	65	12918	4.020	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.400%	
20) 2-Butanone-d5	3.796	46	52769	47.150	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.300%	
24) Chloroform-d	4.252	84	53798	4.443	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.800%	
26) 1,2-Dichloroethane-d4	4.947	65	27037	4.778	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.600%	
32) Benzene-d6	4.963	84	102961	4.353	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.000%	
36) 1,2-Dichloropropane-d6	5.992	67	29308	4.432	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	88.600%	
41) Toluene-d8	7.246	98	94229	4.334	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.600%	
43) trans-1,3-Dichloroprop...	7.558	79	10950	4.386	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	87.800%	
46) 2-Hexanone-d5	8.024	63	46903	52.623	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	105.240%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84	19697	4.914	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152	34523	4.644	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.800%	
Target Compounds					Qvalue	
42) Toluene	7.326	91	7170	0.284	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020724\
Data File : VV034032.D
Acq On : 07 Feb 2024 15:42
Operator : SY/MD
Sample : P1383-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0YB3

Quant Time: Feb 08 04:50:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Feb 08 04:46:29 2024
Response via : Initial Calibration

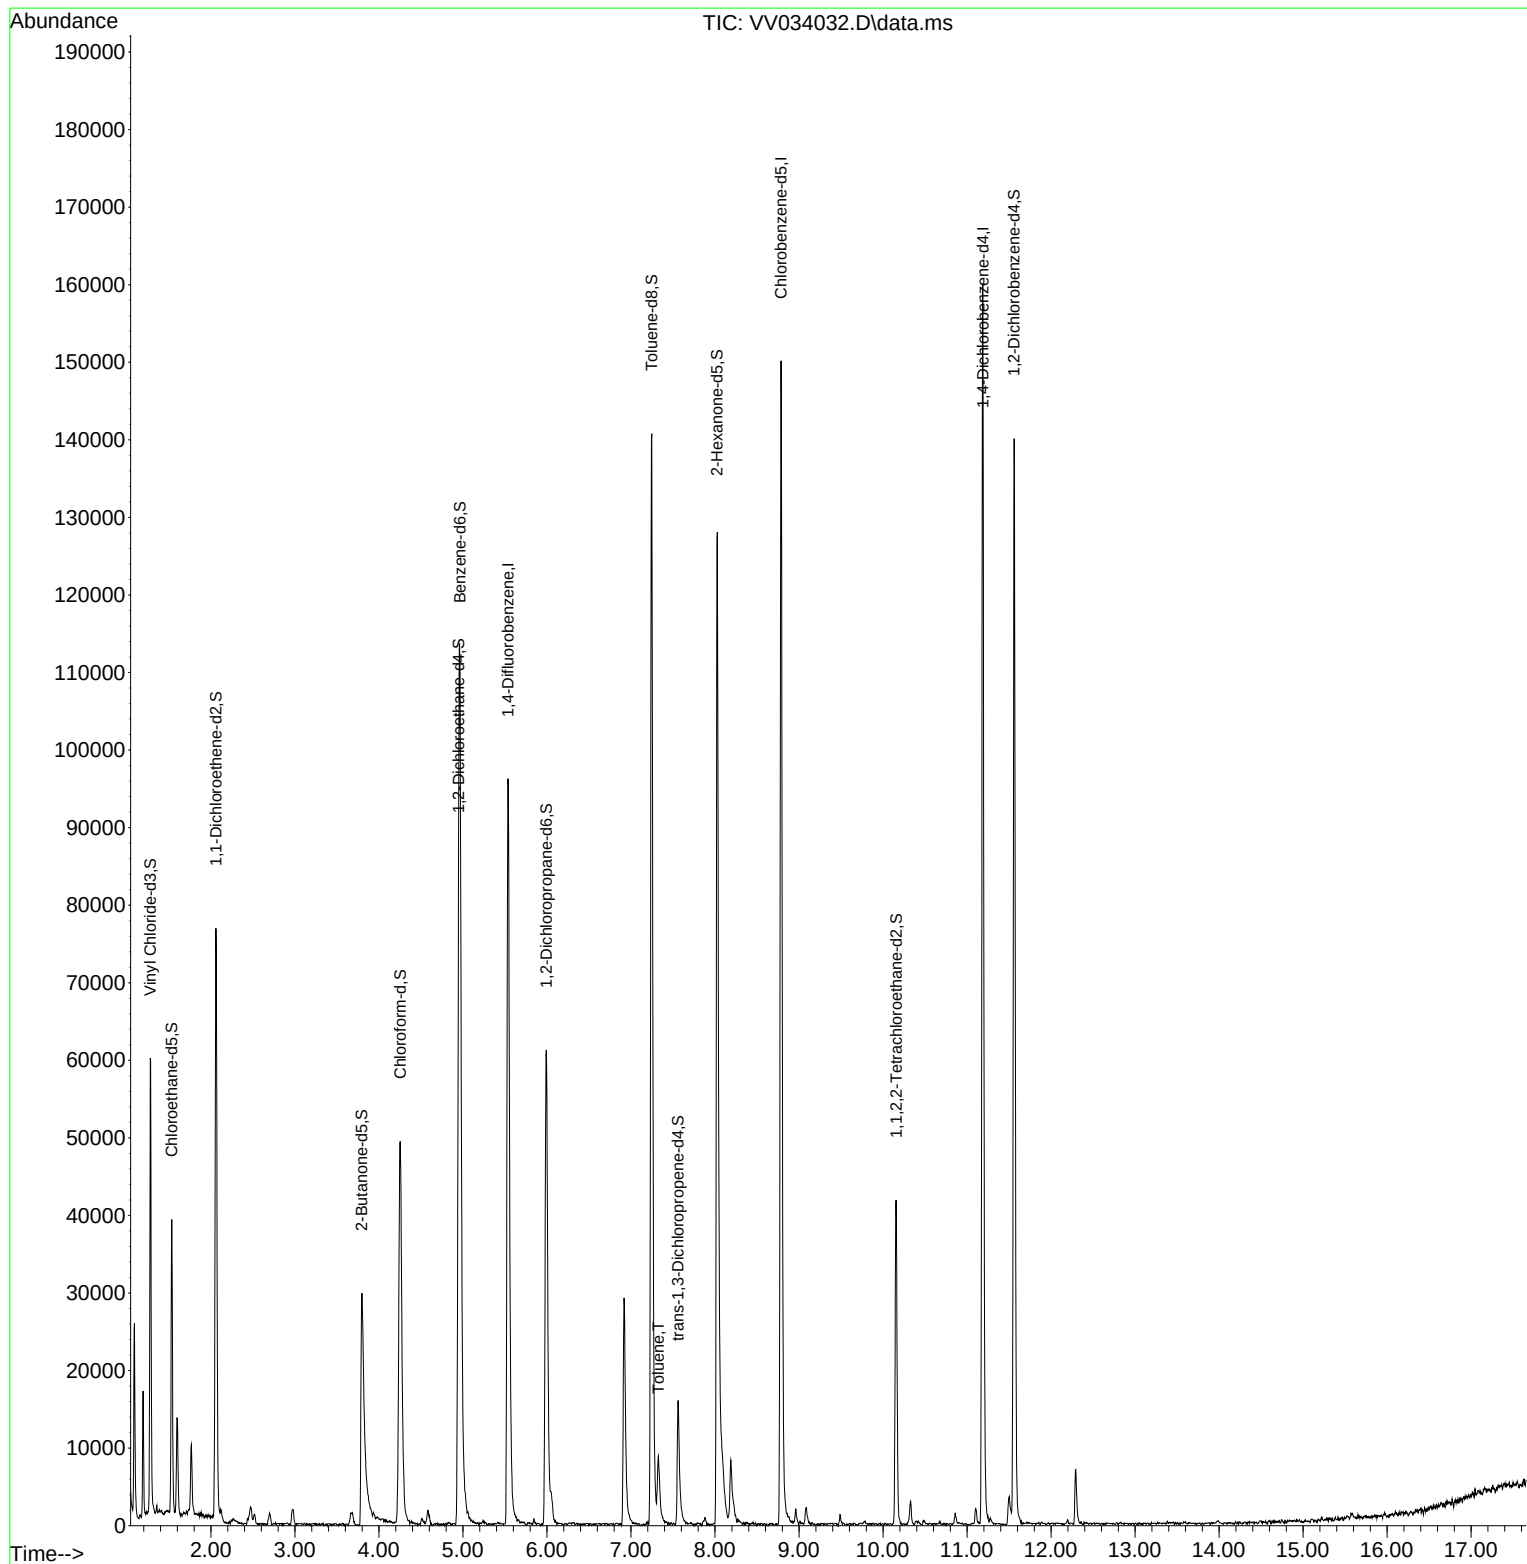

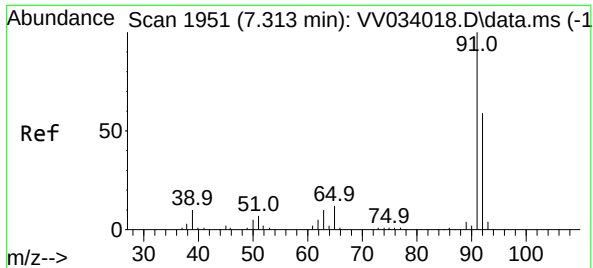

#42
Toluene
Concen: 0.284 ug/L
RT: 7.326 min Scan# 1955
Delta R.T. 0.013 min
Lab File: VV034032.D
Acq: 07 Feb 2024 15:42

Instrument :
MSVOA_V
ClientSampleId :
E0YB3

Tgt Ion: 91 Resp: 7170
Ion Ratio Lower Upper
91 100
92 59.3 42.1 78.3

