

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020724\
 Data File : VV034024.D
 Acq On : 07 Feb 2024 12:33
 Operator : SY/MD
 Sample : P1289-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	88	rBV	42875	44250	9.07%	1.381%
2	1.535	147	154	169	rVB	38125	44720	9.17%	1.396%
3	2.066	308	319	337	rBV2	109679	183729	37.68%	5.734%
4	3.114	631	645	669	rBV	96652	204813	42.00%	6.392%
5	3.831	857	868	903	rBV2	15691	73749	15.12%	2.302%
6	4.252	984	999	1033	rVB	49027	126256	25.89%	3.941%
7	4.513	1063	1080	1105	rBV	189903	487622	100.00%	15.219%
8	4.960	1205	1219	1252	rBV2	113640	287912	59.04%	8.986%
9	5.538	1388	1399	1421	rBV	102114	213404	43.76%	6.660%
10	5.847	1487	1495	1506	rBV7	2649	5078	1.04%	0.158%
11	5.992	1528	1540	1567	rBV2	62108	131568	26.98%	4.106%
12	6.918	1819	1828	1852	rBV2	28536	56021	11.49%	1.748%
13	7.246	1919	1930	1950	rBV	141672	253442	51.98%	7.910%
14	7.561	2020	2028	2049	rBV2	15606	31026	6.36%	0.968%
15	8.030	2164	2174	2206	rBV	112412	237731	48.75%	7.420%
16	8.786	2399	2409	2437	rBV	158929	263659	54.07%	8.229%
17	10.156	2825	2835	2847	rBV	40851	63855	13.10%	1.993%
18	10.326	2877	2888	2898	rVB2	5057	7753	1.59%	0.242%
19	11.185	3146	3155	3176	rBV	165569	263450	54.03%	8.222%
20	11.496	3244	3252	3262	rBV4	5495	11275	2.31%	0.352%
21	11.561	3262	3272	3290	rVB	133944	212740	43.63%	6.640%




Sum of corrected areas: 3204053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020724\
Data File : VV034024.D
Acq On : 07 Feb 2024 12:33
Operator : SY/MD
Sample : P1289-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

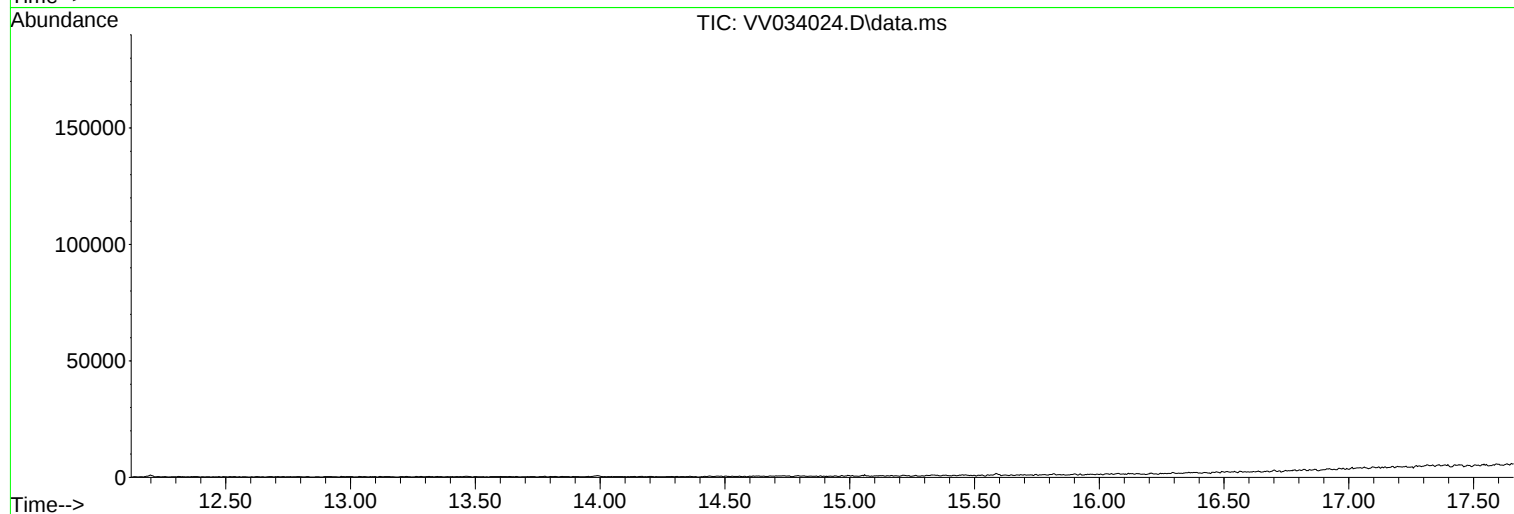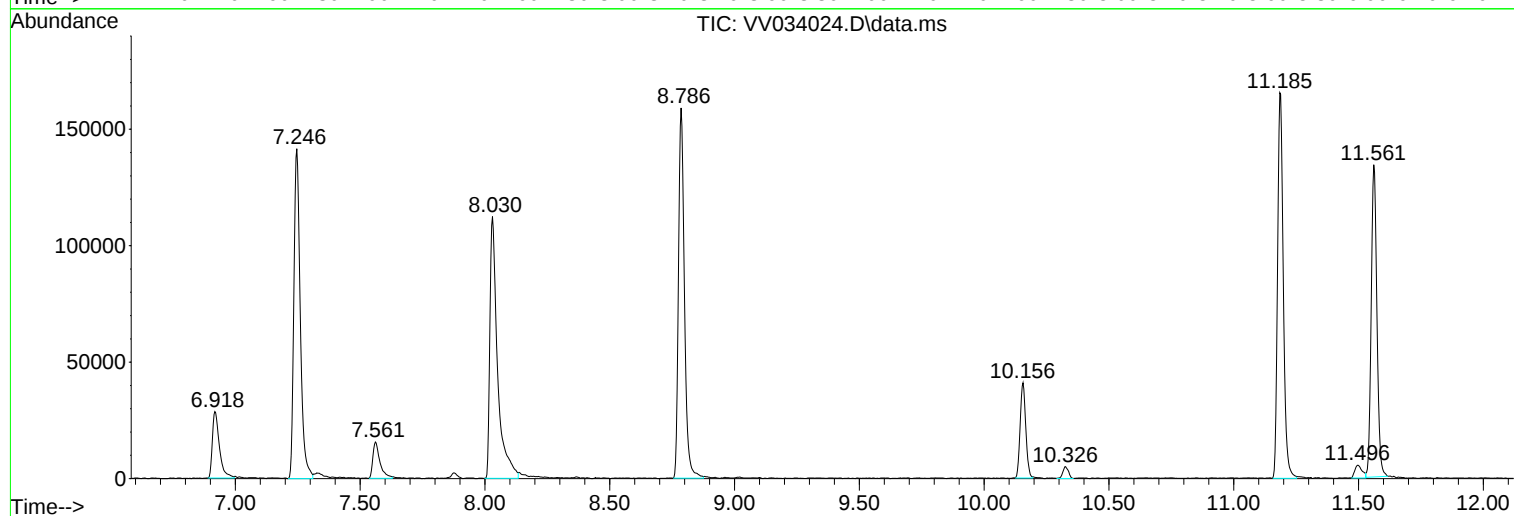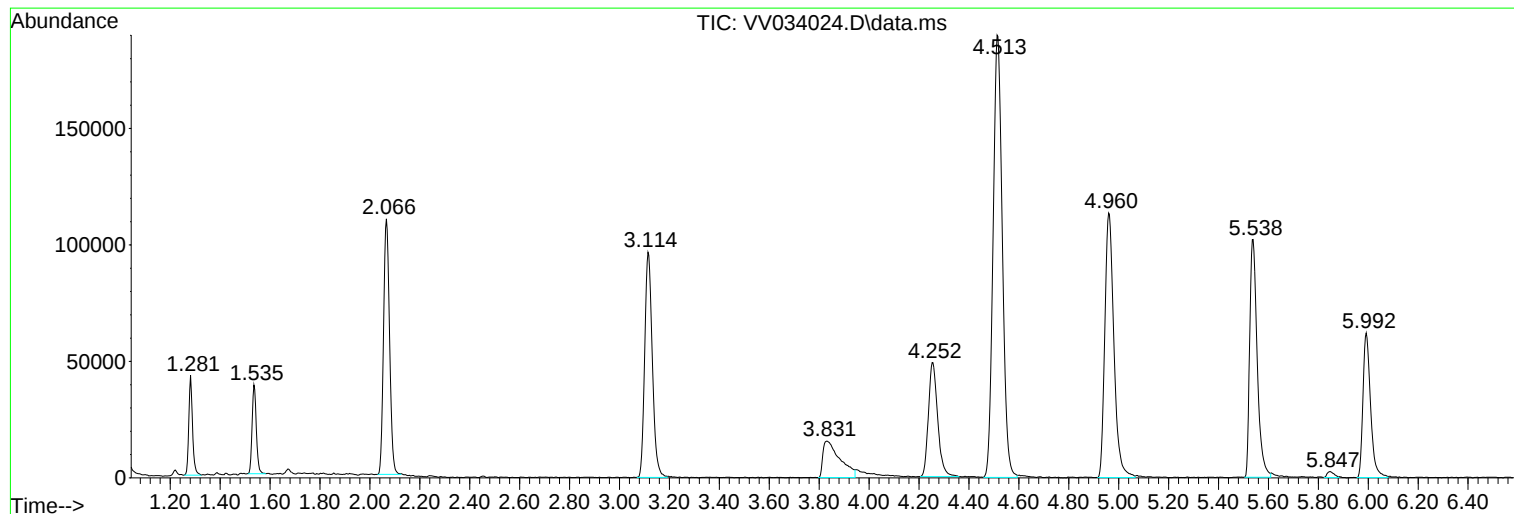

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020724\
Data File : VV034024.D
Acq On : 07 Feb 2024 12:33
Operator : SY/MD
Sample : P1289-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020724\
Data File : VV034024.D
Acq On : 07 Feb 2024 12:33
Operator : SY/MD
Sample : P1289-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------