

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020725\
 Data File : VV038647.D
 Acq On : 07 Feb 2025 15:49
 Operator : SY/MD
 Sample : Q1334-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E29A6

Quant Time: Feb 12 13:22:52 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Feb 12 13:18:31 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	173037	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	191211	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	74796	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	87489	4.89	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.80%
7) Chloroethane-d5	1.532	69	67723	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.056	65	36715	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.20%
20) 2-Butanone-d5	3.799	46	140303	45.16	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.32%
24) Chloroform-d	4.243	84	145168	5.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.40%
26) 1,2-Dichloroethane-d4	4.937	65	71358	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.20%
32) Benzene-d6	4.953	84	270913	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	5.982	67	87221	5.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.20%
41) Toluene-d8	7.239	98	212301	4.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.00%
43) trans-1,3-Dichloroprop...	7.558	79	24784	4.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.40%
46) 2-Hexanone-d5	8.021	63	112429	47.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.40%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	69259	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.20%
66) 1,2-Dichlorobenzene-d4	11.554	152	78138	6.03	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	120.60%#
Target Compounds					Qvalue	
13) Acetone	2.133	43	26328	11.54	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020725\
Data File : VV038647.D
Acq On : 07 Feb 2025 15:49
Operator : SY/MD
Sample : Q1334-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E29A6

Quant Time: Feb 12 13:22:52 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Feb 12 13:18:31 2025
Response via : Initial Calibration

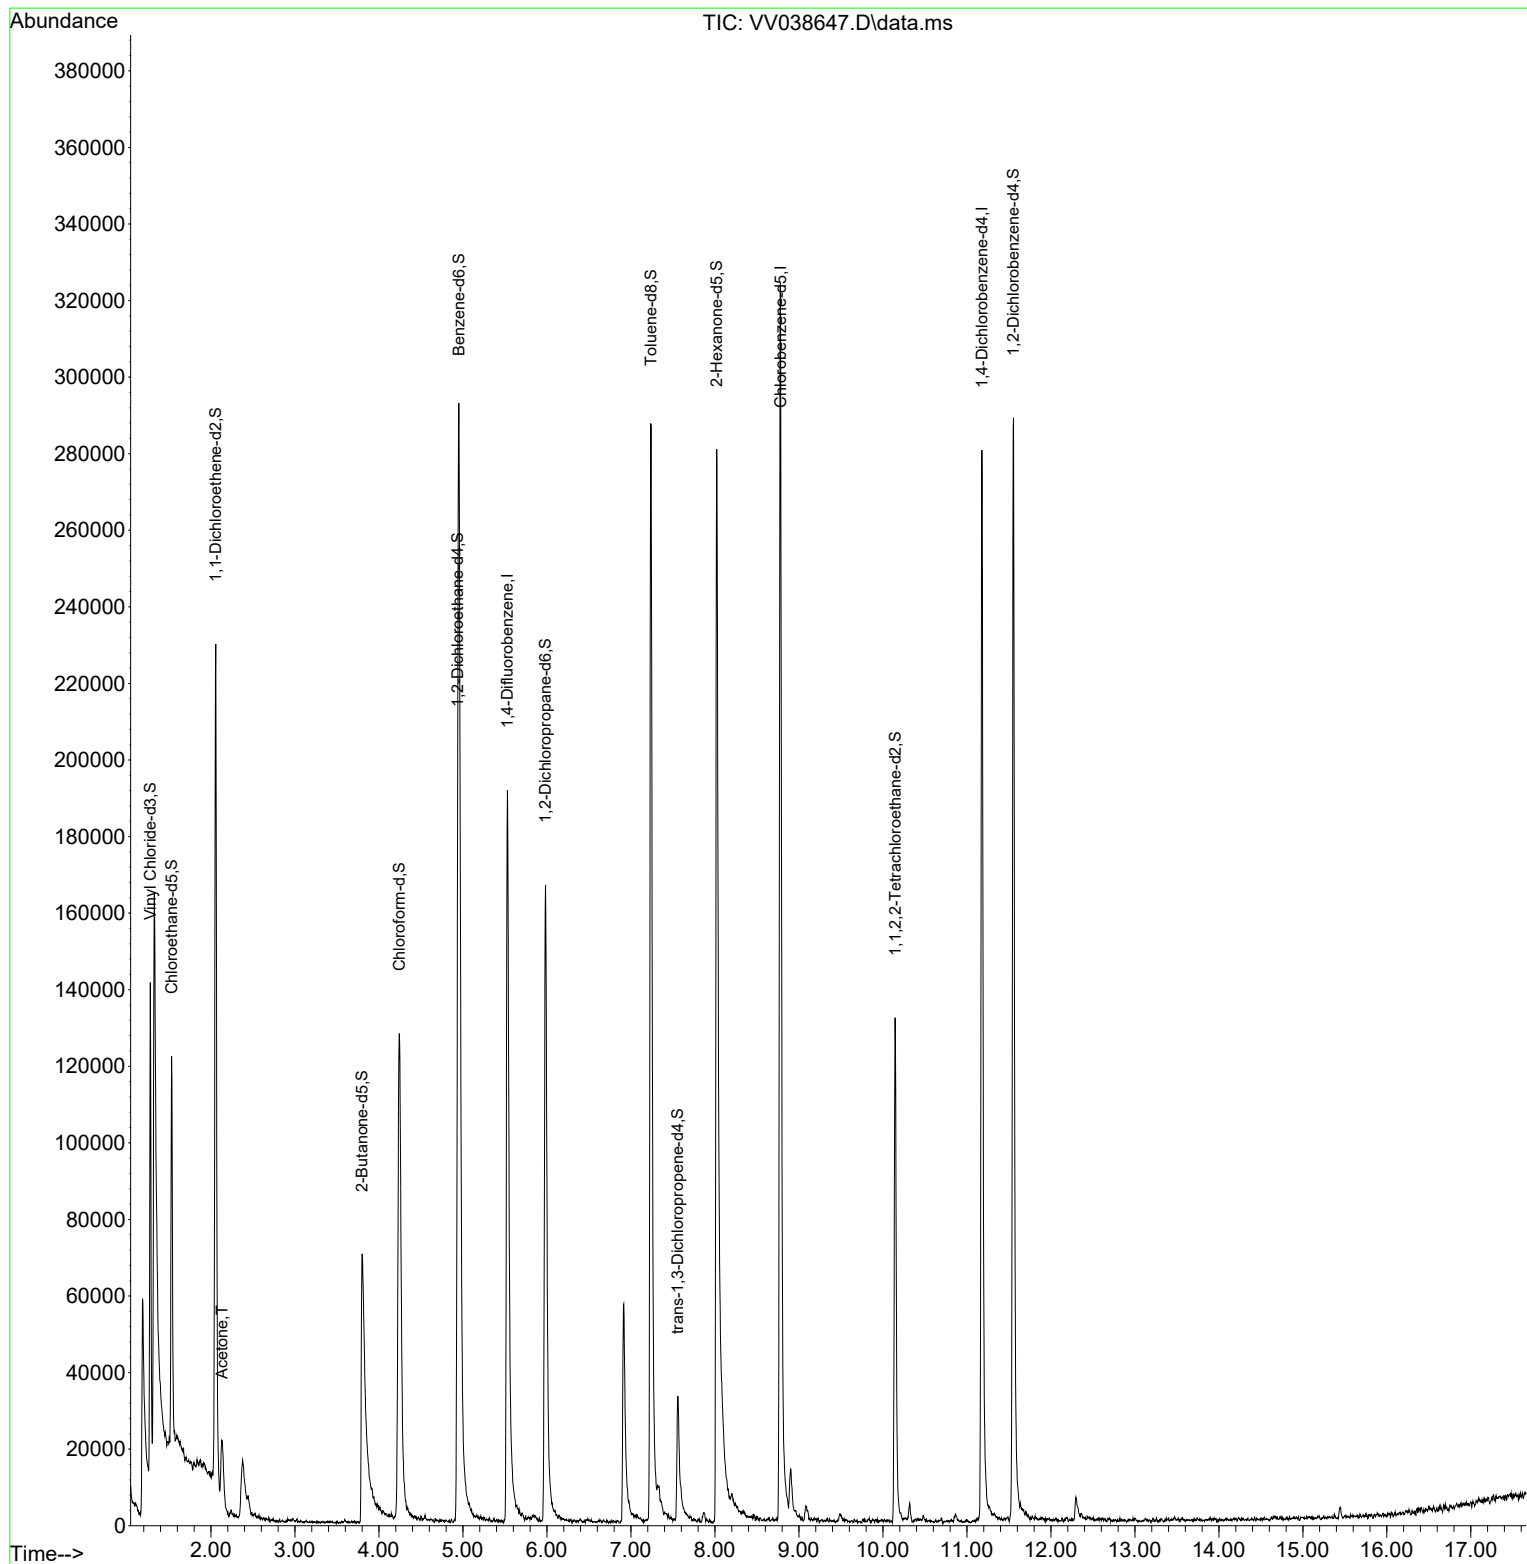

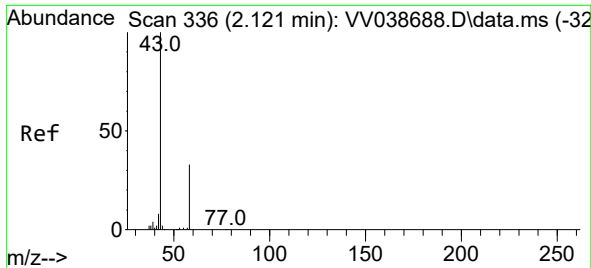

#13
Acetone
Concen: 11.54 ug/L
RT: 2.133 min Scan# 34
Delta R.T. -0.026 min
Lab File: VV038647.D
Acq: 07 Feb 2025 15:49

Instrument :
MSVOA_V
ClientSampleId :
E29A6

Tgt Ion: 43 Resp: 26328
Ion Ratio Lower Upper
43 100
58 34.9 0.0 67.4

