
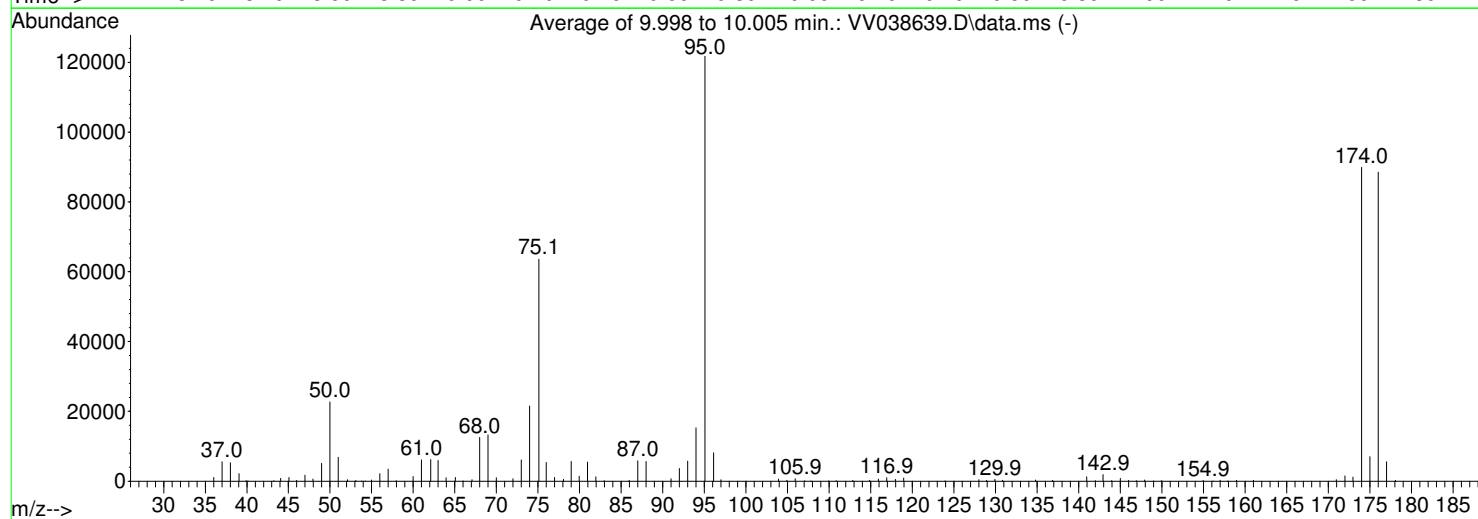


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV020725\
Data File : VV038639.D
Acq On : 07 Feb 2025 09:40
Operator : SY/MD
Sample : BFB202
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB202

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020625WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Feb 17 10:31:04 2025

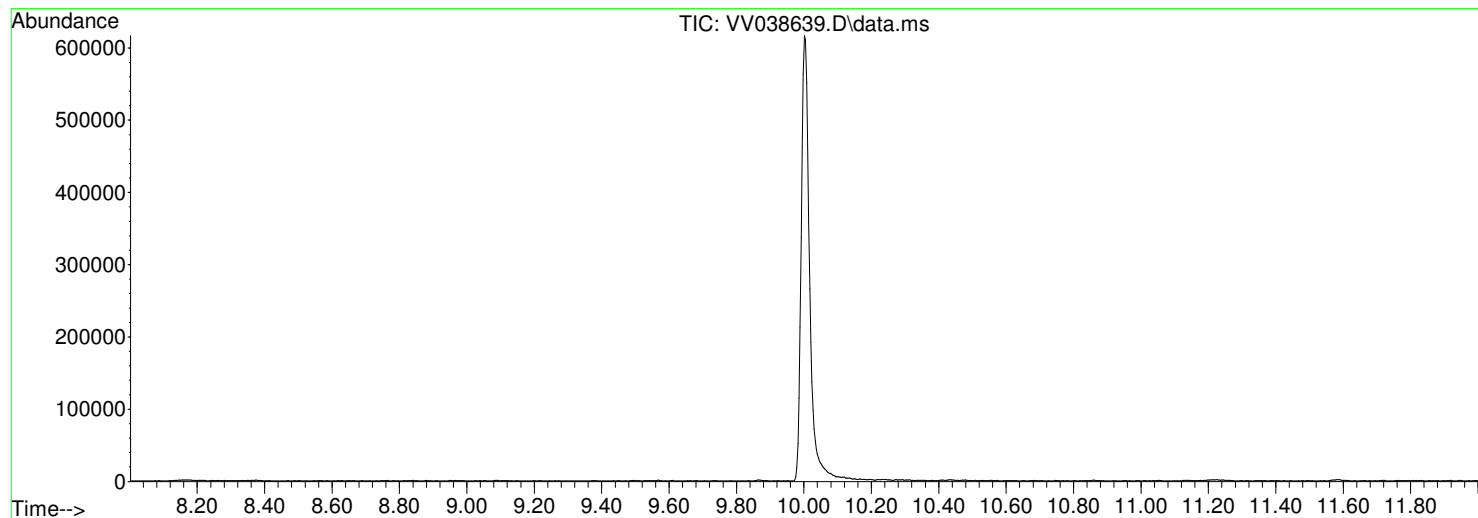

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	22672	PASS
75	95	30	80	52.2	63587	PASS
95	95	100	100	100.0	121741	PASS
96	95	5	9	6.7	8157	PASS
173	174	0.00	2	1.3	1136	PASS
174	95	50	120	73.9	89944	PASS
175	174	5	9	7.8	7016	PASS
176	174	95	105	98.4	88528	PASS
177	176	5	10	6.3	5550	PASS

m/z	Abundance
39.90	138.0
43.90	392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	877.0
37.00	3496.0
38.00	3326.0
39.00	1414.0
39.90	267.0
40.10	263.0
44.00	712.0
45.10	645.0
46.20	212.0
47.00	1122.0
48.00	453.0
49.00	3268.0
50.00	15196.0
51.00	4751.0
52.00	301.0
52.90	170.0
54.90	230.0
56.00	1266.0
57.00	2470.0
58.10	148.0
59.90	730.0
61.00	4438.0
62.00	4118.0
63.10	3778.0
64.00	946.0
65.00	636.0
66.80	242.0
68.00	8324.0
69.00	8070.0
70.00	568.0
72.00	606.0
73.00	3677.0
74.00	13990.0
75.00	39256.0
76.00	3798.0
77.10	472.0
78.00	507.0
79.00	3795.0
79.90	919.0
81.00	4200.0
81.90	830.0
85.80	138.0
87.00	3361.0
87.90	3474.0
90.90	468.0
92.00	2100.0
93.00	3814.0
94.10	9332.0
95.00	77904.0
96.00	5142.0
97.00	143.0
103.90	496.0
104.80	108.0
106.00	409.0
106.80	125.0
109.90	106.0
112.90	115.0
114.90	148.0
115.90	367.0
117.00	801.0
117.90	426.0
118.90	668.0
127.90	335.0
128.80	183.0
129.80	255.0
131.00	181.0
134.80	129.0
137.00	153.0
140.90	893.0
141.90	144.0
142.90	1222.0
143.90	159.0
144.90	780.0
145.80	152.0
147.80	208.0
155.00	366.0
160.80	103.0
170.90	324.0
171.90	1025.0
173.10	1102.0
174.00	55632.0
175.00	4393.0
176.00	52480.0
177.00	3736.0
178.00	151.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	985.0
37.00	3643.0
38.00	3830.0
39.00	1736.0
39.80	283.0
40.20	287.0
42.80	122.0
43.90	820.0
45.10	684.0
46.20	181.0
47.00	1247.0
48.00	506.0
49.00	3554.0
50.00	16648.0
51.00	5254.0
51.90	288.0
52.70	149.0
53.10	151.0
54.10	104.0
54.90	303.0
56.00	1415.0
57.00	2602.0
58.10	142.0
59.90	814.0
61.00	4815.0
62.00	4618.0
63.10	4053.0
64.00	1005.0
65.10	724.0
66.00	116.0
66.90	264.0
68.00	8742.0
69.00	9060.0
70.00	642.0
71.20	112.0
72.00	722.0
73.00	4223.0
74.00	15551.0
75.00	43952.0
76.10	4092.0
77.10	605.0
78.00	538.0
78.90	4383.0
79.90	1012.0
81.00	4680.0
81.90	917.0
83.00	125.0
85.80	192.0
87.00	3763.0
88.00	3506.0
91.00	504.0
92.00	2499.0
93.00	4127.0
94.10	10600.0
95.00	87288.0
96.00	5624.0
97.10	168.0
103.90	512.0
104.70	105.0
105.90	488.0
106.80	127.0
112.80	103.0
114.90	117.0
115.90	398.0
117.00	913.0
118.00	453.0
118.80	749.0
127.90	440.0
128.90	176.0
129.80	351.0
130.90	161.0
134.80	174.0
137.10	195.0
140.90	985.0
142.00	209.0
143.00	1511.0
143.90	139.0
144.90	900.0
145.80	187.0
147.80	278.0
155.00	409.0
157.00	114.0
170.90	407.0
172.00	1143.0
173.10	1305.0
174.00	64112.0
175.00	5247.0
176.00	61152.0
177.00	4200.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	980.0
37.00	3499.0
38.00	3915.0
39.00	1952.0
39.90	278.0
40.20	288.0
42.90	152.0
44.00	926.0
45.10	697.0
45.90	212.0
47.00	1296.0
48.00	507.0
49.00	3447.0
50.00	16349.0
51.10	5225.0
52.00	244.0
52.70	160.0
53.10	139.0
54.10	160.0
55.00	306.0
56.00	1452.0
57.00	2469.0
58.10	114.0
60.00	779.0
61.00	4647.0
62.00	4692.0
63.10	3988.0
64.00	924.0
65.10	731.0
66.10	113.0
66.90	316.0
68.00	8885.0
69.00	9508.0
70.00	688.0
72.00	735.0
73.00	4371.0
74.00	15366.0
75.00	44512.0
76.10	3877.0
77.10	614.0
78.00	493.0
78.90	4690.0
80.00	1112.0
81.00	4672.0
81.90	824.0
83.00	133.0
85.90	147.0
87.00	3980.0
88.00	3501.0
91.00	474.0
92.00	2777.0
93.00	4053.0
94.10	10757.0
95.00	87720.0
96.00	5698.0
97.10	234.0
104.00	508.0
104.80	131.0
105.90	562.0
106.90	142.0
110.90	116.0
112.80	119.0
115.90	394.0
117.00	879.0
118.00	402.0
118.80	754.0
127.90	501.0
128.90	186.0
129.80	411.0
130.80	181.0
134.90	172.0
137.10	202.0
140.90	1007.0
142.00	228.0
143.00	1690.0
143.90	143.0
144.90	814.0
146.00	213.0
147.80	300.0
155.00	355.0
156.90	125.0
170.80	465.0
172.00	1135.0
173.10	1325.0
174.00	66496.0
175.00	5453.0
176.00	64784.0
177.00	4225.0
177.90	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202