
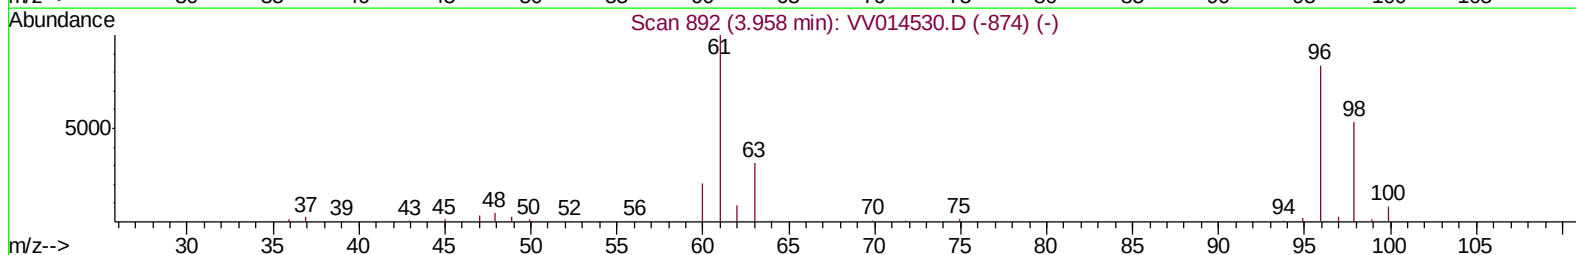
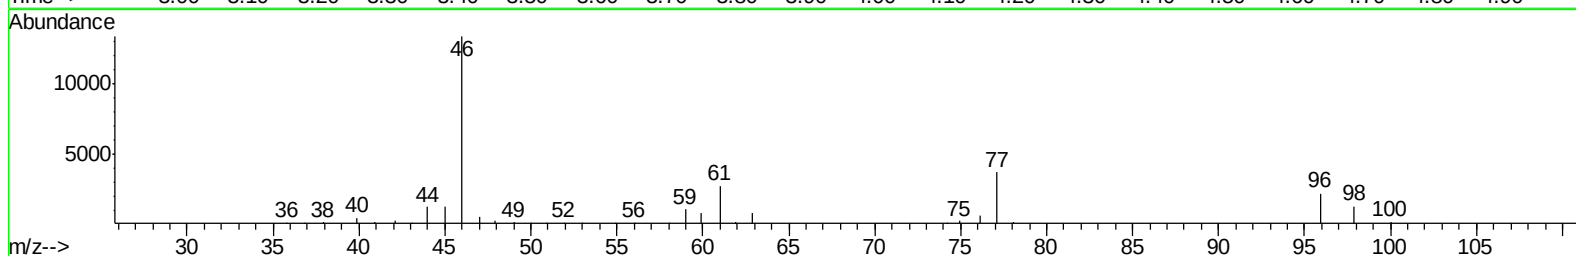


Data File : VV014537.D
Acq On : 07 Feb 2020 14:32
Operator : SY/MD
Sample : MDL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 08 00:06:41 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 00:03:07 2020
Response via : Initial Calibration

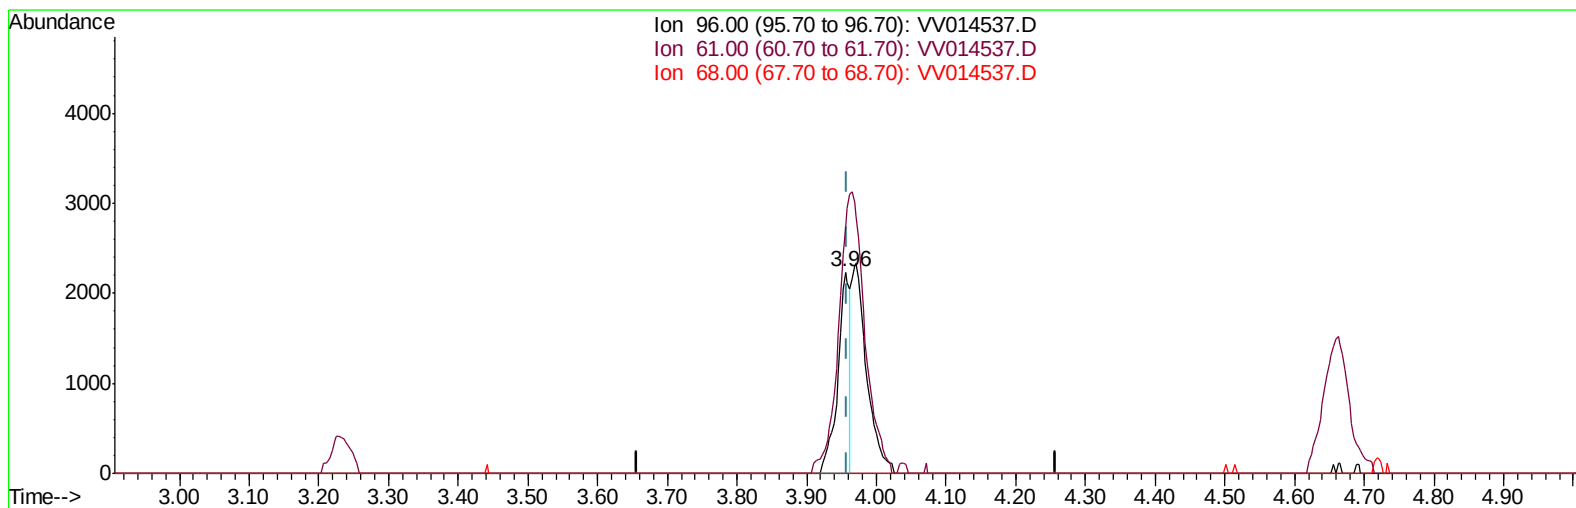

TIC: VV014537.D

(20) cis-1,2-Dichloroethene (T)

3.955min (-0.003) 1.02ug/L

response 2680

Ion	Exp%	Act%
96.00	100	100
61.00	121.70	122.66
68.00	0.00	0.00
0.00	0.00	0.00