
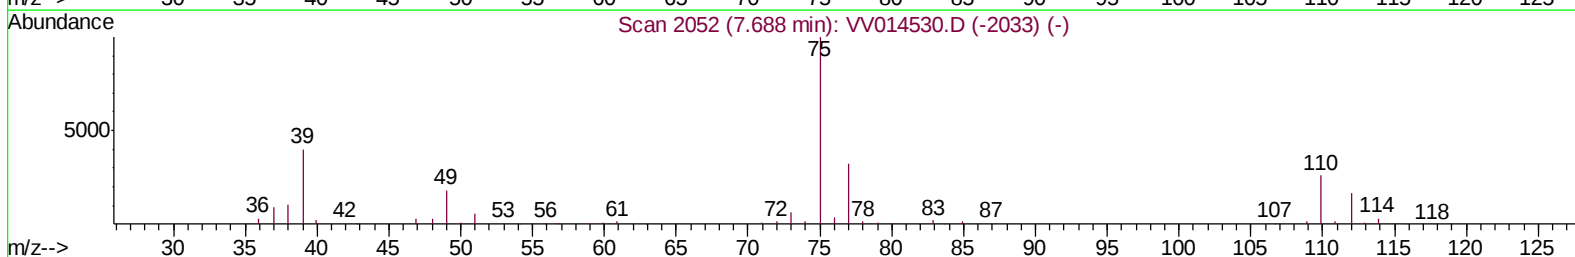
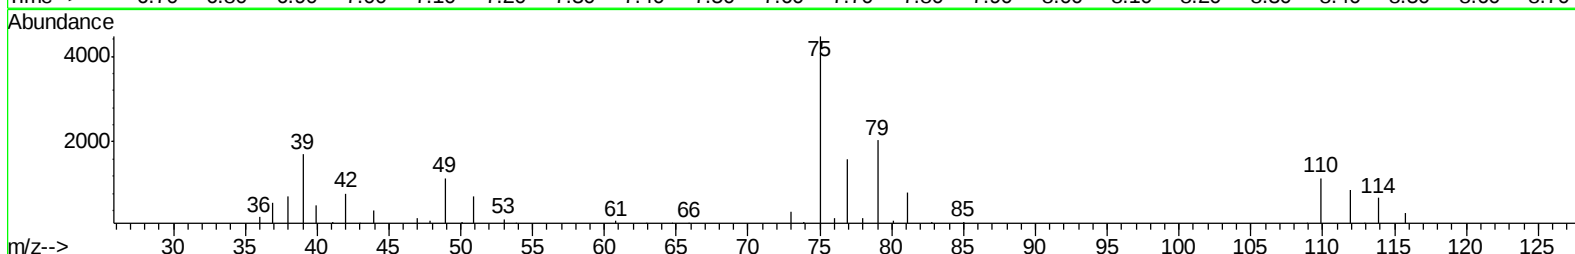


Data File : VV014538.D
Acq On : 07 Feb 2020 14:56
Operator : SY/MD
Sample : MDL02
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 08 00:07:07 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis
QLast Update : Sat Feb 08 00:03:07 2020
Response via : Initial Calibration

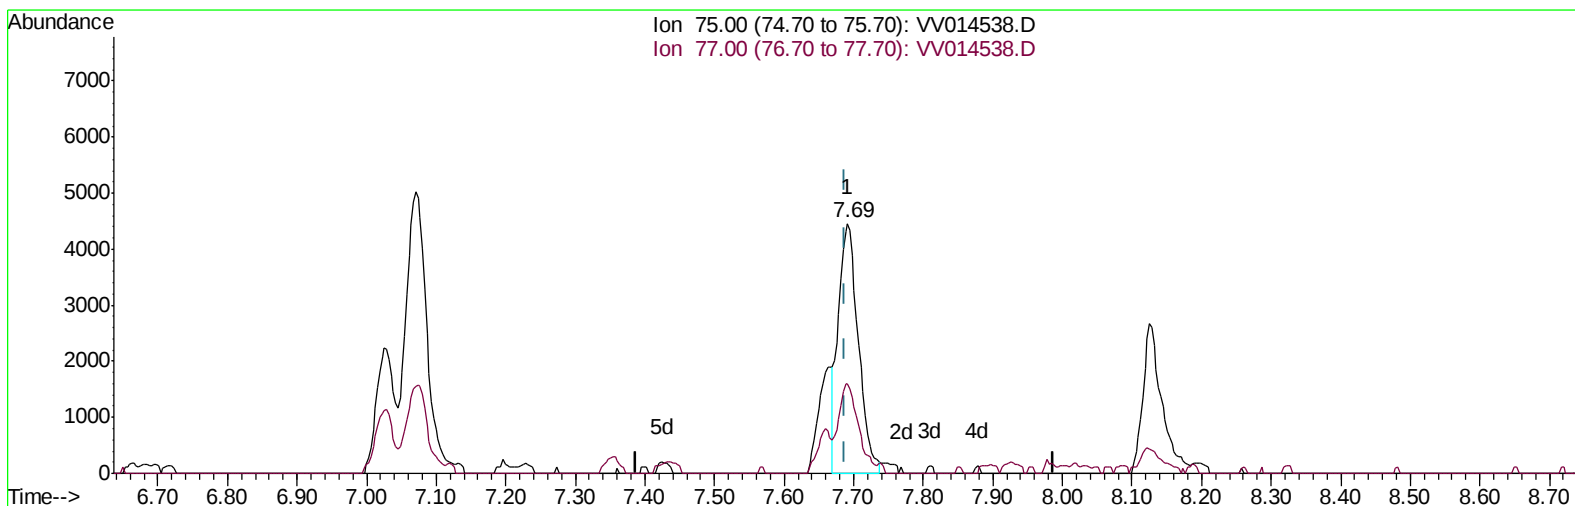

TIC: VV014538.D

(44) trans-1,3-Dichloropropene (T)

7.691min (+0.003) 2.46ug/L m

response 8987

Ion	Exp%	Act%
75.00	100	100
77.00	31.70	35.87
0.00	0.00	0.00
0.00	0.00	0.00