

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020820\
 Data File : VV014532.D
 Acq On : 07 Feb 2020 12:33
 Operator : SY/MD
 Sample : VV0208MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	83	rVB	145584	141753	11.24%	1.468%
2	1.582	146	153	167	rVB	88532	108200	8.58%	1.121%
3	2.081	306	308	312	rBV3	502	384	0.03%	0.004%
4	2.132	312	324	336	rBV	192825	276793	21.94%	2.867%
5	2.534	445	449	460	rVB7	2800	4670	0.37%	0.048%
6	2.733	508	511	512	rBV2	336	174	0.01%	0.002%
7	2.791	526	529	530	rBV2	766	489	0.04%	0.005%
8	3.000	589	594	598	rBV3	779	806	0.06%	0.008%
9	3.094	620	623	626	rBV2	449	312	0.02%	0.003%
10	3.167	644	646	652	rVB	608	362	0.03%	0.004%
11	3.209	656	659	662	rBV4	521	323	0.03%	0.003%
12	3.309	687	690	695	rBV2	351	396	0.03%	0.004%
13	3.692	806	809	810	rBV2	532	168	0.01%	0.002%
14	3.701	810	812	816	rVB3	629	298	0.02%	0.003%
15	3.740	821	824	827	rVB2	253	168	0.01%	0.002%
16	3.798	838	842	844	rBV	585	346	0.03%	0.004%
17	3.849	853	858	861	rBV2	427	318	0.03%	0.003%
18	3.923	870	881	908	rBV	98235	254547	20.18%	2.636%
19	4.177	958	960	962	rVB	509	176	0.01%	0.002%
20	4.331	1006	1008	1010	rBV2	313	168	0.01%	0.002%
21	4.399	1011	1029	1058	rVV	197953	490394	38.87%	5.079%
22	4.630	1099	1101	1103	rBV2	681	367	0.03%	0.004%
23	4.669	1111	1113	1116	rBV3	421	232	0.02%	0.002%
24	4.772	1139	1145	1146	rBV2	793	655	0.05%	0.007%
25	4.839	1162	1166	1167	rBV	650	410	0.03%	0.004%
26	4.884	1178	1180	1185	rVB	353	285	0.02%	0.003%
27	4.910	1185	1188	1190	rBV2	325	174	0.01%	0.002%
28	4.978	1204	1209	1213	rBV4	477	431	0.03%	0.004%
29	5.010	1217	1219	1222	rBV	358	244	0.02%	0.003%
30	5.093	1227	1245	1274	rBV2	497272	1261639	100.00%	13.066%
31	5.302	1308	1310	1312	rBV2	528	230	0.02%	0.002%
32	5.360	1326	1328	1330	rVB2	704	192	0.02%	0.002%
33	5.463	1358	1360	1365	rBV	487	269	0.02%	0.003%
34	5.499	1369	1371	1375	rBV3	522	485	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020820\
 Data File : VV014532.D
 Acq On : 07 Feb 2020 12:33
 Operator : SY/MD
 Sample : VV0208MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

35	5.576	1391	1395	1397	rVV2	234	238	0.02%	0.002%
36	5.659	1408	1421	1450	rBV	390178	773790	61.33%	8.014%
37	5.913	1498	1500	1503	rBV4	343	208	0.02%	0.002%
38	5.952	1503	1512	1522	rVB9	3267	6449	0.51%	0.067%
39	6.000	1525	1527	1532	rBV3	582	360	0.03%	0.004%
40	6.026	1532	1535	1540	rBV4	383	398	0.03%	0.004%
41	6.113	1549	1562	1590	rVV	282954	572185	45.35%	5.926%
42	6.511	1681	1686	1688	rBV	440	292	0.02%	0.003%
43	6.589	1707	1710	1712	rBV3	437	280	0.02%	0.003%
44	6.621	1716	1720	1723	rBV4	418	346	0.03%	0.004%
45	6.656	1726	1731	1734	rBV4	470	497	0.04%	0.005%
46	6.740	1754	1757	1761	rBV3	519	315	0.02%	0.003%
47	6.781	1765	1770	1772	rBV2	361	236	0.02%	0.002%
48	6.794	1772	1774	1776	rBV2	378	188	0.01%	0.002%
49	6.894	1801	1805	1809	rVB4	411	314	0.02%	0.003%
50	6.949	1818	1822	1825	rVB3	316	252	0.02%	0.003%
51	6.971	1825	1829	1831	rBV4	569	505	0.04%	0.005%
52	7.026	1834	1846	1871	rBV	176545	315965	25.04%	3.272%
53	7.158	1885	1887	1891	rVB2	627	351	0.03%	0.004%
54	7.357	1935	1949	1967	rBV	620149	1076889	85.36%	11.153%
55	7.659	2032	2043	2066	rBV2	128231	218336	17.31%	2.261%
56	7.968	2137	2139	2140	rBV2	619	277	0.02%	0.003%
57	8.003	2148	2150	2152	rBV	368	180	0.01%	0.002%
58	8.125	2178	2188	2229	rBV	310370	620954	49.22%	6.431%
59	8.373	2263	2265	2267	rBV2	452	195	0.02%	0.002%
60	8.479	2295	2298	2300	rBV	291	181	0.01%	0.002%
61	8.498	2300	2304	2310	rVB6	653	662	0.05%	0.007%
62	8.540	2314	2317	2319	rVV2	444	280	0.02%	0.003%
63	8.579	2327	2329	2332	rBV2	500	257	0.02%	0.003%
64	8.682	2358	2361	2362	rBV2	352	201	0.02%	0.002%
65	8.730	2372	2376	2378	rBV	398	337	0.03%	0.003%
66	8.746	2378	2381	2384	rBV2	366	263	0.02%	0.003%
67	8.891	2414	2426	2448	rBV	581486	942582	74.71%	9.762%
68	9.080	2483	2485	2487	rVB	593	243	0.02%	0.003%
69	9.093	2487	2489	2495	rBV	415	362	0.03%	0.004%
70	9.164	2508	2511	2513	rBV2	662	477	0.04%	0.005%
71	9.244	2534	2536	2541	rVB3	442	300	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020820\
 Data File : VV014532.D
 Acq On : 07 Feb 2020 12:33
 Operator : SY/MD
 Sample : VV0208MBL01
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK204

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

72	9.289	2548	2550	2553	rBV2	482	360	0.03%	0.004%
73	9.579	2639	2640	2641	rBV	509	190	0.02%	0.002%
74	9.881	2731	2734	2737	rBV2	359	288	0.02%	0.003%
75	9.981	2758	2765	2767	rBV3	642	860	0.07%	0.009%
76	10.045	2784	2785	2788	rVB	349	165	0.01%	0.002%
77	10.135	2811	2813	2817	rVV2	335	196	0.02%	0.002%
78	10.167	2821	2823	2828	rVB2	587	332	0.03%	0.003%
79	10.254	2836	2850	2869	rBV	388210	612246	48.53%	6.341%
80	10.322	2869	2871	2873	rBV2	659	222	0.02%	0.002%
81	10.450	2909	2911	2915	rVB	798	352	0.03%	0.004%
82	10.543	2937	2940	2945	rBV3	585	378	0.03%	0.004%
83	10.582	2946	2952	2957	rVB3	721	922	0.07%	0.010%
84	10.720	2993	2995	2998	rBV2	407	168	0.01%	0.002%
85	10.781	3012	3014	3019	rVB2	505	376	0.03%	0.004%
86	10.852	3032	3036	3038	rBV2	376	218	0.02%	0.002%
87	10.868	3038	3041	3045	rBV3	665	508	0.04%	0.005%
88	10.891	3045	3048	3051	rVV	407	211	0.02%	0.002%
89	10.952	3064	3067	3070	rBV3	590	471	0.04%	0.005%
90	11.045	3092	3096	3098	rBV	555	364	0.03%	0.004%
91	11.151	3127	3129	3131	rBV2	447	236	0.02%	0.002%
92	11.289	3159	3172	3193	rBV	613736	967926	76.72%	10.024%
93	11.444	3219	3220	3222	rBV	451	209	0.02%	0.002%
94	11.511	3238	3241	3242	rBV	582	301	0.02%	0.003%
95	11.543	3249	3251	3252	rBV	342	164	0.01%	0.002%
96	11.666	3276	3289	3312	rVV	610937	978069	77.52%	10.129%
97	11.939	3372	3374	3380	rVB2	498	371	0.03%	0.004%
98	11.981	3384	3387	3390	rBV	642	391	0.03%	0.004%
99	12.241	3465	3468	3470	rBV	379	236	0.02%	0.002%
100	13.556	3870	3877	3885	rBV6	3509	6093	0.48%	0.063%


Sum of corrected areas: 9655826

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV020820\
Data File : VV014532.D
Acq On : 07 Feb 2020 12:33
Operator : SY/MD
Sample : VV0208MBL01
Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

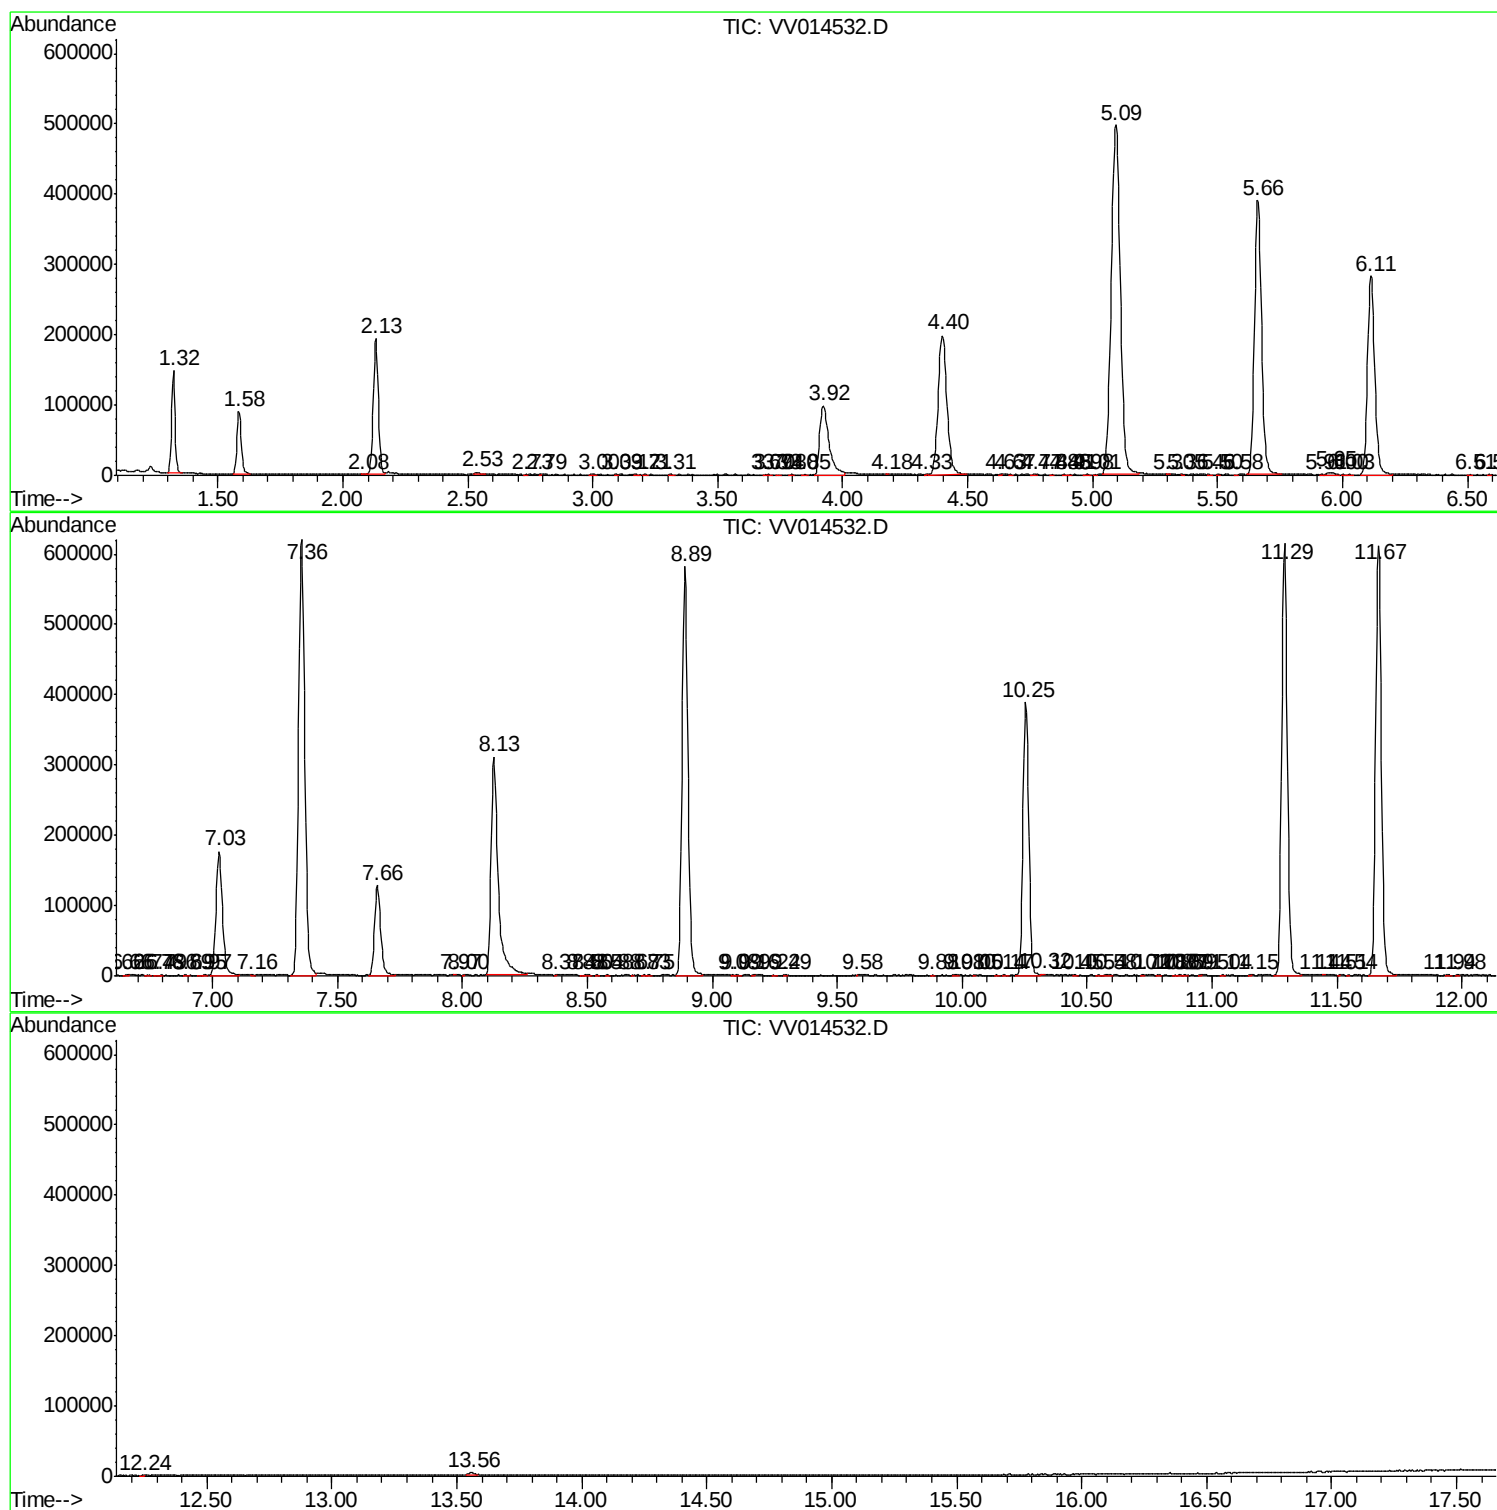

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV020820\
Data File : VV014532.D
Acq On : 07 Feb 2020 12:33
Operator : SY/MD
Sample : VV0208MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV020820\
Data File : VV014532.D
Acq On : 07 Feb 2020 12:33
Operator : SY/MD
Sample : VV0208MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK204

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc