

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020820\
 Data File : VV014534.D
 Acq On : 07 Feb 2020 13:21
 Operator : SY/MD
 Sample : VV0208MBL02
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK206

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	82	rVB	132279	129751	11.01%	1.431%
2	1.582	145	153	165	rBV	84990	100359	8.51%	1.107%
3	2.129	312	323	336	rBV	179002	257160	21.82%	2.836%
4	2.515	441	443	444	rBV2	608	325	0.03%	0.004%
5	2.598	464	469	473	rBV3	899	1089	0.09%	0.012%
6	2.766	519	521	525	rBV4	450	330	0.03%	0.004%
7	2.836	538	543	545	rBV3	777	417	0.04%	0.005%
8	2.856	547	549	551	rVV2	460	231	0.02%	0.003%
9	2.869	551	553	562	rVB3	716	720	0.06%	0.008%
10	2.907	562	565	568	rBV2	373	237	0.02%	0.003%
11	2.930	569	572	575	rBV3	524	326	0.03%	0.004%
12	2.987	587	590	593	rBV3	639	529	0.04%	0.006%
13	3.068	614	615	619	rVB2	545	226	0.02%	0.002%
14	3.103	624	626	629	rBV3	387	214	0.02%	0.002%
15	3.209	656	659	662	rBV3	466	422	0.04%	0.005%
16	3.274	674	679	681	rBV2	529	433	0.04%	0.005%
17	3.351	700	703	706	rBV	357	222	0.02%	0.002%
18	3.370	706	709	711	rBV	506	267	0.02%	0.003%
19	3.431	724	728	730	rBV3	337	283	0.02%	0.003%
20	3.479	741	743	749	rVB2	558	384	0.03%	0.004%
21	3.643	792	794	799	rVB2	571	312	0.03%	0.003%
22	3.692	806	809	810	rBV2	420	283	0.02%	0.003%
23	3.852	854	859	864	rBV4	477	581	0.05%	0.006%
24	3.920	869	880	913	rBV	92083	239190	20.29%	2.638%
25	4.238	977	979	981	rVB3	664	221	0.02%	0.002%
26	4.396	1012	1028	1050	rBV	186495	458257	38.88%	5.054%
27	4.582	1084	1086	1089	rVB	521	233	0.02%	0.003%
28	4.704	1122	1124	1127	rVB2	688	391	0.03%	0.004%
29	4.730	1127	1132	1135	rBV3	595	536	0.05%	0.006%
30	4.820	1156	1160	1162	rBV2	371	245	0.02%	0.003%
31	4.923	1190	1192	1196	rVB2	629	380	0.03%	0.004%
32	4.975	1206	1208	1210	rBV	495	248	0.02%	0.003%
33	5.090	1226	1244	1272	rBV2	458831	1178645	100.00%	12.998%
34	5.319	1312	1315	1318	rBV2	849	363	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020820\
 Data File : VV014534.D
 Acq On : 07 Feb 2020 13:21
 Operator : SY/MD
 Sample : VV0208MBL02
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 VBLK206

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

35	5.376	1329	1333	1337	rBV4	585	589	0.05%	0.006%
36	5.412	1341	1344	1347	rVB2	895	616	0.05%	0.007%
37	5.428	1347	1349	1351	rBV3	447	216	0.02%	0.002%
38	5.492	1366	1369	1372	rBV3	635	411	0.03%	0.005%
39	5.573	1392	1394	1396	rBV2	496	240	0.02%	0.003%
40	5.659	1407	1421	1442	rBV	378413	748291	63.49%	8.252%
41	5.814	1466	1469	1470	rBV	514	290	0.02%	0.003%
42	5.897	1490	1495	1498	rBV3	492	366	0.03%	0.004%
43	5.952	1501	1512	1521	rBV5	2253	4557	0.39%	0.050%
44	6.113	1544	1562	1582	rVV	267885	536800	45.54%	5.920%
45	6.328	1627	1629	1633	rBV3	444	441	0.04%	0.005%
46	6.470	1670	1673	1676	rBV2	289	219	0.02%	0.002%
47	6.573	1701	1705	1708	rVB3	677	450	0.04%	0.005%
48	6.592	1708	1711	1713	rBV3	365	226	0.02%	0.002%
49	6.772	1763	1767	1770	rBV4	430	431	0.04%	0.005%
50	6.881	1797	1801	1803	rBV2	401	300	0.03%	0.003%
51	7.026	1833	1846	1867	rBV	165085	297355	25.23%	3.279%
52	7.187	1893	1896	1898	rBV2	632	412	0.03%	0.005%
53	7.357	1935	1949	1969	rBV	581729	1007475	85.48%	11.111%
54	7.605	2023	2026	2027	rBV	379	234	0.02%	0.003%
55	7.659	2031	2043	2068	rBV	120574	207628	17.62%	2.290%
56	7.955	2132	2135	2137	rBV3	579	412	0.03%	0.005%
57	8.048	2160	2164	2166	rBV	432	317	0.03%	0.003%
58	8.126	2177	2188	2227	rBV	282372	571815	48.51%	6.306%
59	8.527	2310	2313	2316	rBV3	451	315	0.03%	0.003%
60	8.608	2334	2338	2340	rBV3	372	281	0.02%	0.003%
61	8.688	2361	2363	2366	rVB	477	227	0.02%	0.003%
62	8.746	2379	2381	2384	rVB2	384	223	0.02%	0.002%
63	8.772	2386	2389	2391	rVB2	462	223	0.02%	0.002%
64	8.817	2401	2403	2408	rVB2	382	230	0.02%	0.003%
65	8.839	2408	2410	2413	rBV	341	223	0.02%	0.002%
66	8.891	2413	2426	2444	rBV	560012	897638	76.16%	9.899%
67	9.138	2501	2503	2505	rBV	717	378	0.03%	0.004%
68	9.180	2512	2516	2518	rBV2	757	618	0.05%	0.007%
69	9.579	2637	2640	2643	rBV2	452	390	0.03%	0.004%
70	9.592	2643	2644	2650	rVB3	801	688	0.06%	0.008%
71	9.643	2658	2660	2663	rVB	397	229	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV020820\
 Data File : VV014534.D
 Acq On : 07 Feb 2020 13:21
 Operator : SY/MD
 Sample : VV0208MBL02
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK206

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

72	9.717	2681	2683	2685	rBV	505	258	0.02%	0.003%
73	9.746	2689	2692	2694	rBV2	464	289	0.02%	0.003%
74	9.891	2733	2737	2740	rVV3	612	485	0.04%	0.005%
75	9.913	2740	2744	2749	rVB3	579	624	0.05%	0.007%
76	9.942	2749	2753	2755	rBV2	603	424	0.04%	0.005%
77	9.974	2762	2763	2767	rVB	609	232	0.02%	0.003%
78	10.016	2772	2776	2777	rBV2	424	256	0.02%	0.003%
79	10.132	2809	2812	2815	rBV3	586	304	0.03%	0.003%
80	10.151	2816	2818	2821	rVB2	630	325	0.03%	0.004%
81	10.171	2821	2824	2828	rBV2	376	260	0.02%	0.003%
82	10.203	2830	2834	2835	rBV	496	278	0.02%	0.003%
83	10.254	2838	2850	2866	rBV	364519	566838	48.09%	6.251%
84	10.379	2887	2889	2892	rVB3	410	220	0.02%	0.002%
85	10.402	2894	2896	2900	rVV2	507	328	0.03%	0.004%
86	10.421	2900	2902	2907	rVV4	440	305	0.03%	0.003%
87	10.447	2907	2910	2917	rVB3	438	301	0.03%	0.003%
88	10.505	2926	2928	2933	rVB2	424	248	0.02%	0.003%
89	10.531	2933	2936	2938	rBV2	484	321	0.03%	0.004%
90	10.576	2944	2950	2957	rVB5	869	941	0.08%	0.010%
91	10.711	2990	2992	2996	rBV2	433	286	0.02%	0.003%
92	10.775	3008	3012	3015	rBV3	456	332	0.03%	0.004%
93	10.894	3047	3049	3054	rVV3	548	409	0.03%	0.005%
94	10.971	3072	3073	3076	rVB	999	394	0.03%	0.004%
95	10.997	3076	3081	3083	rBV2	488	400	0.03%	0.004%
96	11.289	3160	3172	3198	rBV	588434	926723	78.63%	10.220%
97	11.666	3277	3289	3306	rBV	571914	908574	77.09%	10.020%
98	12.138	3432	3436	3440	rBV4	732	625	0.05%	0.007%
99	12.489	3541	3545	3546	rBV3	649	531	0.05%	0.006%
100	12.691	3605	3608	3611	rBV2	878	686	0.06%	0.008%


Sum of corrected areas: 9067761

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV020820\
Data File : VV014534.D
Acq On : 07 Feb 2020 13:21
Operator : SY/MD
Sample : VV0208MBL02
Misc : 5.0µ/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK206

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

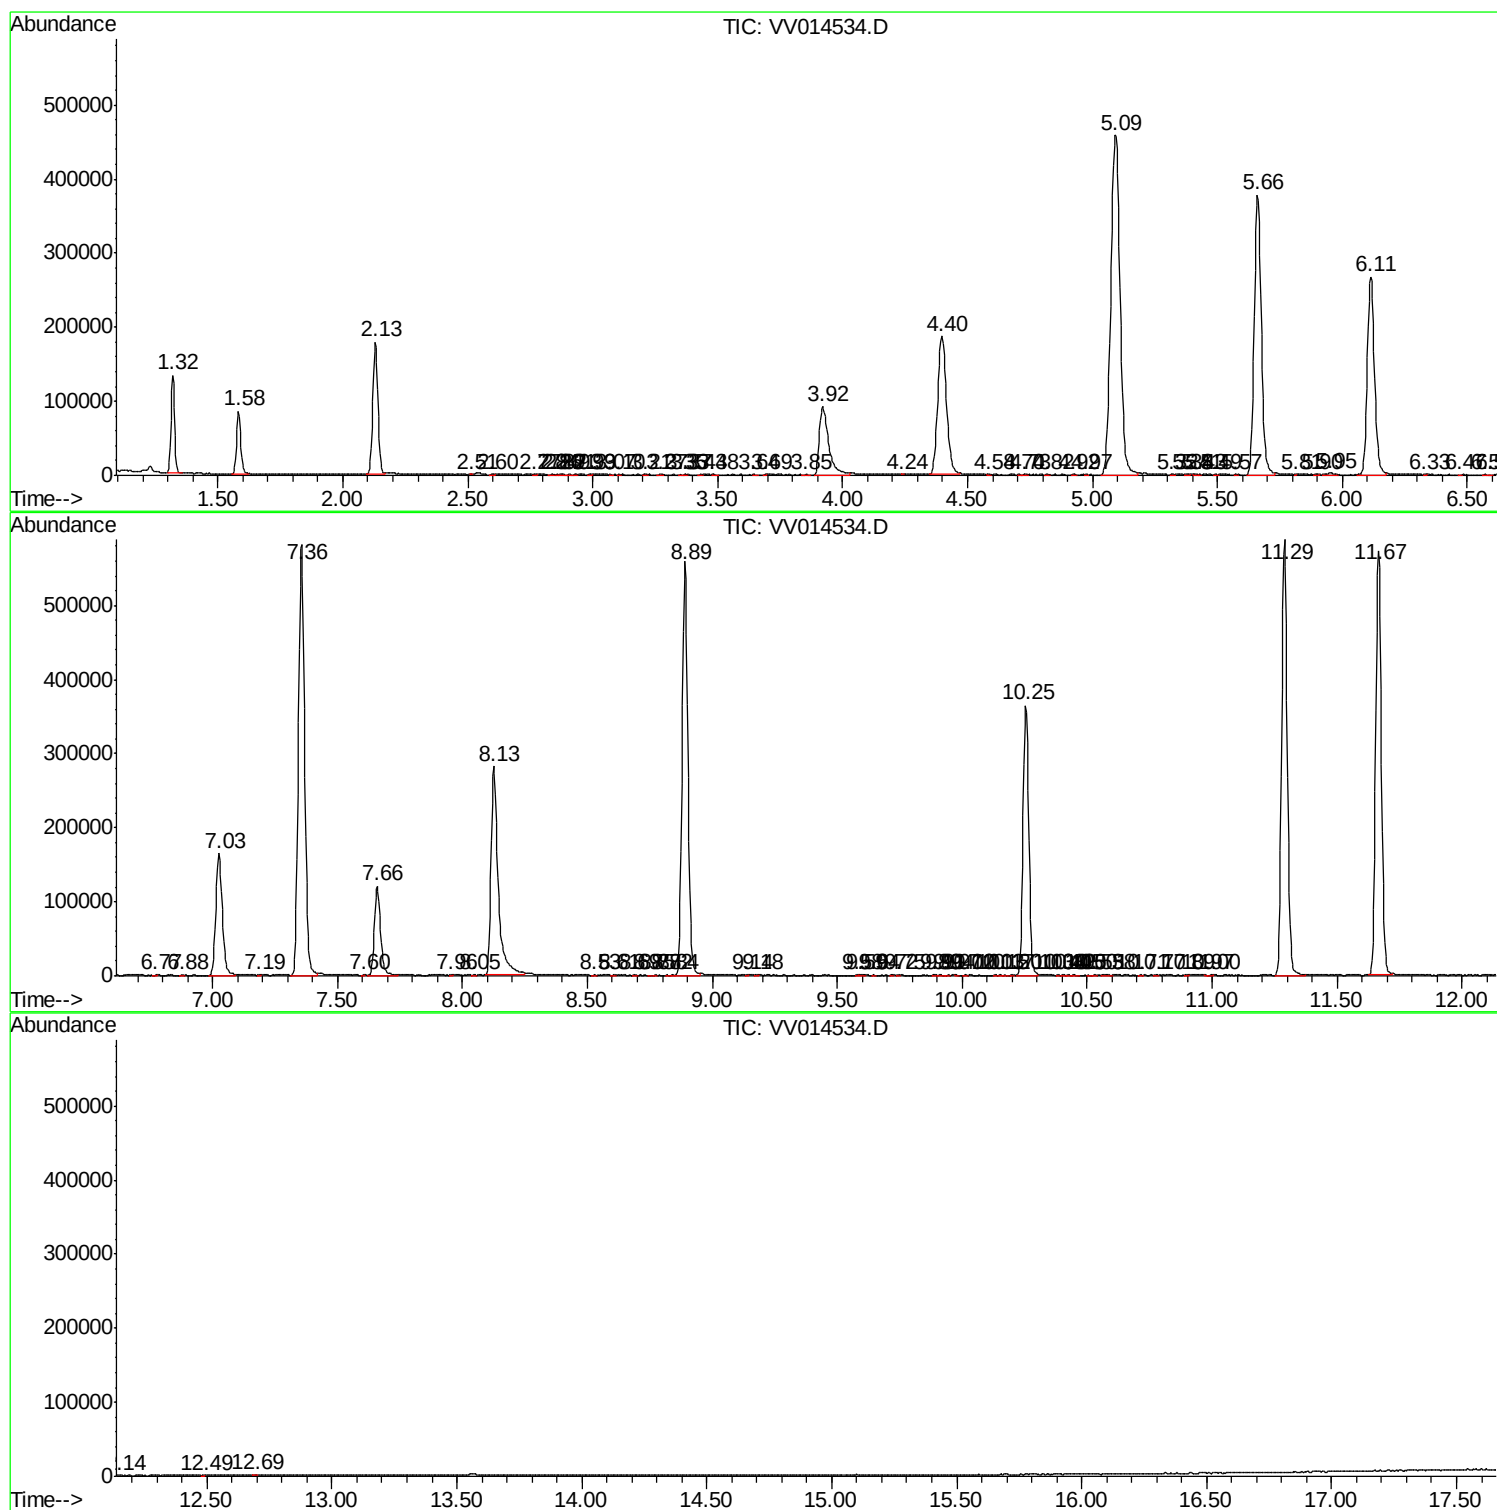

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV020820\
Data File : VV014534.D
Acq On : 07 Feb 2020 13:21
Operator : SY/MD
Sample : VV0208MBL02
Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK206

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV020820\
Data File : VV014534.D
Acq On : 07 Feb 2020 13:21
Operator : SY/MD
Sample : VV0208MBL02
Misc : 5.0g/5.0mL/100uL/5.0mL/MSV0A_V/MEOH
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK206

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc