


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV020820\
 Data File : VV014529.D
 Acq On : 07 Feb 2020 10:48
 Operator : SY/MD
 Sample : BFB89
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB202

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis
 Last Update : Sat Feb 08 00:03:07 2020

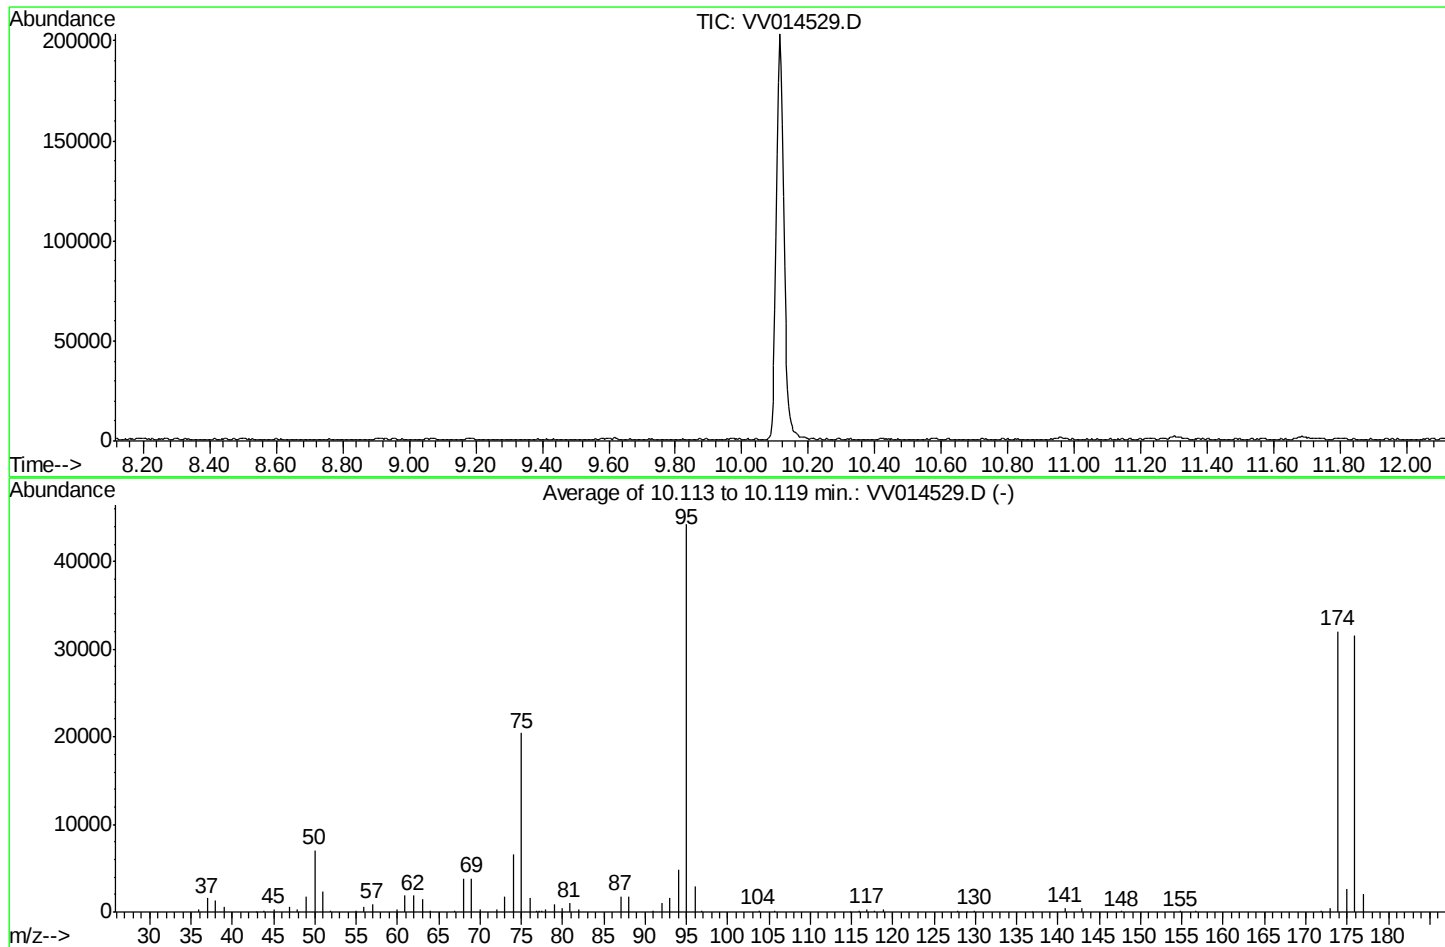

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	7021	PASS
75	95	30	80	46.1	20384	PASS
95	95	100	100	100.0	44242	PASS
96	95	5	9	6.8	2995	PASS
173	174	0.00	2	1.4	448	PASS
174	95	50	120	72.4	32016	PASS
175	174	5	9	8.3	2667	PASS
176	174	95	101	98.5	31525	PASS
177	176	5	9	6.7	2123	PASS

m/z	Abundance
35.90	331.0
37.00	1405.0
38.00	1205.0
38.90	565.0
39.90	336.0
42.90	106.0
44.00	465.0
45.00	291.0
46.90	585.0
48.00	221.0
49.00	1681.0
50.00	6594.0
51.00	2046.0
51.90	160.0
55.10	145.0
55.90	531.0
57.00	917.0
59.90	321.0
60.90	1687.0
61.90	1675.0
63.00	1245.0
63.90	171.0
66.90	164.0
68.00	3413.0
69.00	3683.0
69.90	289.0
72.10	269.0
73.00	1822.0
74.00	6115.0
75.00	18984.0
76.00	1641.0
77.20	179.0
77.50	177.0
77.90	201.0
79.00	788.0
79.90	364.0
80.80	930.0
81.90	307.0
87.00	1778.0
88.00	1759.0
91.00	150.0
92.00	1042.0
93.00	1523.0
94.00	4451.0
95.00	42104.0
96.00	2783.0
96.90	158.0
103.80	232.0
105.70	154.0
115.80	162.0
116.90	302.0
117.80	165.0
118.80	221.0
127.90	130.0
128.90	107.0
129.80	136.0
136.90	103.0
140.90	423.0
142.80	398.0
147.80	103.0
154.90	118.0
156.70	172.0
171.90	174.0
172.90	412.0
173.90	31208.0
174.90	2415.0
175.90	30384.0
176.90	1928.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
35.90	380.0
37.00	1601.0
38.00	1343.0
38.90	608.0
39.90	302.0
43.90	509.0
45.00	344.0
47.00	659.0
47.90	249.0
49.00	1747.0
50.00	7277.0
51.00	2361.0
51.90	140.0
55.00	134.0
55.90	608.0
57.00	881.0
60.00	343.0
61.00	1932.0
62.00	1940.0
63.00	1578.0
63.90	167.0
66.90	185.0
68.00	3939.0
69.00	3963.0
70.00	331.0
72.00	254.0
73.00	1842.0
74.00	6772.0
75.00	20968.0
76.00	1652.0
76.80	213.0
77.20	210.0
77.40	212.0
77.90	250.0
78.90	894.0
79.90	396.0
80.90	1075.0
81.90	351.0
87.00	1861.0
88.00	1783.0
91.00	179.0
92.00	1131.0
93.00	1710.0
94.00	5002.0
95.00	45600.0
96.00	3095.0
96.90	152.0
103.80	234.0
105.80	155.0
114.80	117.0
115.90	167.0
116.90	324.0
117.80	201.0
118.80	244.0
127.80	135.0
129.80	136.0
130.00	136.0
136.90	113.0
140.90	495.0
142.90	444.0
147.70	131.0
154.80	106.0
156.70	147.0
171.90	189.0
172.90	457.0
173.90	32856.0
174.90	2764.0
175.90	32584.0
176.90	2216.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
35.90	372.0
37.00	1697.0
38.00	1450.0
39.00	622.0
40.00	263.0
43.90	562.0
45.00	420.0
47.00	668.0
47.80	282.0
49.00	1645.0
50.00	7193.0
51.00	2419.0
52.00	115.0
54.90	114.0
56.00	582.0
57.00	836.0
60.00	371.0
61.00	1982.0
62.00	2000.0
63.00	1717.0
63.90	165.0
66.90	178.0
68.00	4077.0
69.00	3961.0
69.90	376.0
71.90	187.0
73.00	1698.0
74.00	7003.0
75.00	21200.0
76.00	1661.0
76.90	252.0
77.90	242.0
78.90	1014.0
79.90	355.0
80.90	1129.0
81.90	334.0
87.00	1794.0
88.00	1746.0
91.00	172.0
92.00	1082.0
93.00	1705.0
94.00	5006.0
95.00	45024.0
96.00	3107.0
96.90	133.0
103.80	205.0
105.80	163.0
115.90	189.0
116.80	299.0
117.80	188.0
118.90	243.0
127.80	156.0
130.00	139.0
140.90	481.0
142.90	410.0
147.70	127.0
154.80	105.0
171.90	158.0
173.00	476.0
173.90	31984.0
175.00	2822.0
175.90	31608.0
176.90	2227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

Scan 2794 (10.074 min): VV014529.D
BFB89

m/z	Abundance
39.80	315.0
40.70	101.0
43.90	378.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202