

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
 Data File : VV020820.D
 Acq On : 08 Feb 2021 11:22
 Operator : SY/MD
 Sample : VV0208WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	99	rVB	338283	333463	15.63%	1.988%
2	1.568	157	164	178	rVB	277305	301923	14.16%	1.800%
3	2.108	322	332	367	rVB	562991	864787	40.55%	5.157%
4	2.458	438	441	445	rVB2	758	522	0.02%	0.003%
5	2.507	451	456	466	rVB6	2303	3213	0.15%	0.019%
6	2.687	509	512	518	rVB2	627	511	0.02%	0.003%
7	2.892	575	576	577	rVB	535	103	0.00%	0.001%
8	2.915	578	583	587	rBV3	424	472	0.02%	0.003%
9	3.034	618	620	624	rVV2	463	283	0.01%	0.002%
10	3.153	653	657	661	rBV4	667	591	0.03%	0.004%
11	3.182	661	666	673	rBV2	557	618	0.03%	0.004%
12	3.214	674	676	678	rBV2	201	105	0.00%	0.001%
13	3.259	688	690	693	rBV2	221	173	0.01%	0.001%
14	3.320	705	709	710	rBV2	224	176	0.01%	0.001%
15	3.429	740	743	747	rVB2	382	278	0.01%	0.002%
16	3.474	754	757	759	rBV	352	189	0.01%	0.001%
17	3.487	759	761	764	rVB	493	207	0.01%	0.001%
18	3.510	764	768	772	rBV	394	383	0.02%	0.002%
19	3.561	779	784	788	rBV	486	387	0.02%	0.002%
20	3.580	788	790	793	rVV2	266	131	0.01%	0.001%
21	3.674	815	819	820	rBV2	208	145	0.01%	0.001%
22	3.722	831	834	835	rBV2	293	127	0.01%	0.001%
23	3.799	854	858	859	rBV2	319	156	0.01%	0.001%
24	3.892	874	887	927	rBV	140473	433429	20.32%	2.584%
25	4.352	1013	1030	1060	rBV	346100	848082	39.76%	5.057%
26	4.664	1125	1127	1128	rBV	389	100	0.00%	0.001%
27	4.687	1128	1134	1136	rBV4	681	506	0.02%	0.003%
28	4.780	1161	1163	1165	rVB2	430	135	0.01%	0.001%
29	4.834	1178	1180	1184	rVB3	440	258	0.01%	0.002%
30	4.873	1189	1192	1196	rBV4	502	342	0.02%	0.002%
31	4.924	1206	1208	1211	rBV3	336	213	0.01%	0.001%
32	4.963	1218	1220	1224	rVB3	418	205	0.01%	0.001%
33	5.050	1229	1247	1285	rBV2	833440	2132812	100.00%	12.718%
34	5.339	1333	1337	1340	rBV4	561	474	0.02%	0.003%
35	5.394	1353	1354	1356	rBV2	480	161	0.01%	0.001%
36	5.574	1406	1410	1411	rBV2	311	228	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
 Data File : VV020820.D
 Acq On : 08 Feb 2021 11:22
 Operator : SY/MD
 Sample : VV0208WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

37	5.619	1411	1424	1459	rVV	674153	1359257	63.73%	8.105%
38	5.908	1503	1514	1529	rBV2	21644	45757	2.15%	0.273%
39	5.995	1539	1541	1544	rVB2	640	296	0.01%	0.002%
40	6.072	1550	1565	1595	rBV	464257	952241	44.65%	5.678%
41	6.349	1649	1651	1652	rBV	244	99	0.00%	0.001%
42	6.362	1652	1655	1656	rBV3	420	280	0.01%	0.002%
43	6.539	1707	1710	1713	rBV3	296	201	0.01%	0.001%
44	6.577	1719	1722	1724	rBV2	430	250	0.01%	0.001%
45	6.651	1741	1745	1748	rBV4	751	670	0.03%	0.004%
46	6.703	1758	1761	1763	rBV	207	133	0.01%	0.001%
47	6.715	1763	1765	1768	rVB3	250	151	0.01%	0.001%
48	6.731	1768	1770	1772	rBV	339	131	0.01%	0.001%
49	6.760	1776	1779	1783	rBV2	372	302	0.01%	0.002%
50	6.780	1783	1785	1789	rVB2	297	130	0.01%	0.001%
51	6.796	1789	1790	1796	rVB	195	126	0.01%	0.001%
52	6.821	1796	1798	1802	rBV3	412	347	0.02%	0.002%
53	6.921	1825	1829	1833	rVB2	303	204	0.01%	0.001%
54	6.947	1833	1837	1839	rBV	291	233	0.01%	0.001%
55	6.989	1839	1850	1881	rBV	254176	467999	21.94%	2.791%
56	7.320	1938	1953	1978	rBV	1002284	1732512	81.23%	10.331%
57	7.574	2030	2032	2037	rBV3	548	418	0.02%	0.002%
58	7.625	2037	2048	2076	rBV	178699	311723	14.62%	1.859%
59	7.889	2126	2130	2134	rBV3	387	295	0.01%	0.002%
60	7.982	2154	2159	2160	rBV3	1261	1058	0.05%	0.006%
61	8.040	2175	2177	2181	rBV3	359	263	0.01%	0.002%
62	8.092	2182	2193	2234	rBV	505281	949981	44.54%	5.665%
63	8.477	2309	2313	2315	rBV4	537	414	0.02%	0.002%
64	8.651	2365	2367	2370	rVB2	434	213	0.01%	0.001%
65	8.693	2376	2380	2381	rBV	316	172	0.01%	0.001%
66	8.725	2387	2390	2391	rBV2	343	141	0.01%	0.001%
67	8.764	2399	2402	2404	rBV2	331	199	0.01%	0.001%
68	8.792	2409	2411	2413	rBV	600	374	0.02%	0.002%
69	8.857	2419	2431	2452	rBV	1042667	1670332	78.32%	9.960%
70	9.201	2535	2538	2541	rBV2	387	274	0.01%	0.002%
71	9.426	2606	2608	2610	rBV	281	188	0.01%	0.001%
72	9.555	2643	2648	2650	rBV2	433	363	0.02%	0.002%
73	9.686	2687	2689	2694	rBV2	412	264	0.01%	0.002%
74	9.712	2694	2697	2700	rBV2	361	304	0.01%	0.002%
75	9.786	2718	2720	2723	rBV	284	166	0.01%	0.001%
76	9.805	2723	2726	2729	rVV2	335	228	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
 Data File : VV02080.D
 Acq On : 08 Feb 2021 11:22
 Operator : SY/MD
 Sample : VV0208WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK94

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

77	9.847	2736	2739	2740	rBV2	292	174	0.01%	0.001%
78	9.931	2762	2765	2766	rBV2	486	240	0.01%	0.001%
79	9.982	2778	2781	2786	rBV	340	288	0.01%	0.002%
80	10.143	2829	2831	2832	rBV	287	111	0.01%	0.001%
81	10.223	2840	2856	2879	rBV	641935	1006335	47.18%	6.001%
82	10.506	2942	2944	2948	rVB2	294	156	0.01%	0.001%
83	10.532	2950	2952	2953	rBV	319	141	0.01%	0.001%
84	10.622	2978	2980	2981	rBV	311	134	0.01%	0.001%
85	10.799	3033	3035	3040	rVB3	430	286	0.01%	0.002%
86	10.821	3040	3042	3044	rBV	234	136	0.01%	0.001%
87	10.834	3044	3046	3049	rVB2	450	230	0.01%	0.001%
88	10.857	3049	3053	3054	rBV	462	309	0.01%	0.002%
89	10.927	3069	3075	3080	rBV5	660	752	0.04%	0.004%
90	11.005	3093	3099	3105	rBV3	381	513	0.02%	0.003%
91	11.255	3165	3177	3203	rBV	1080164	1677069	78.63%	10.000%
92	11.474	3243	3245	3247	rVB2	356	131	0.01%	0.001%
93	11.487	3247	3249	3251	rBV	500	241	0.01%	0.001%
94	11.632	3281	3294	3314	rBV	1059118	1653219	77.51%	9.858%
95	11.908	3378	3380	3382	rBV2	269	141	0.01%	0.001%
96	12.390	3526	3530	3533	rBV2	474	375	0.02%	0.002%
97	12.657	3608	3613	3615	rBV2	1530	1419	0.07%	0.008%
98	12.886	3682	3684	3687	rBV2	479	338	0.02%	0.002%
99	13.101	3749	3751	3754	rBV2	477	289	0.01%	0.002%
100	13.271	3798	3804	3815	rVB7	1776	2785	0.13%	0.017%




Sum of corrected areas: 16770389

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
Data File : VV020280.D
Acq On : 08 Feb 2021 11:22
Operator : SY/MD
Sample : VV0208WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

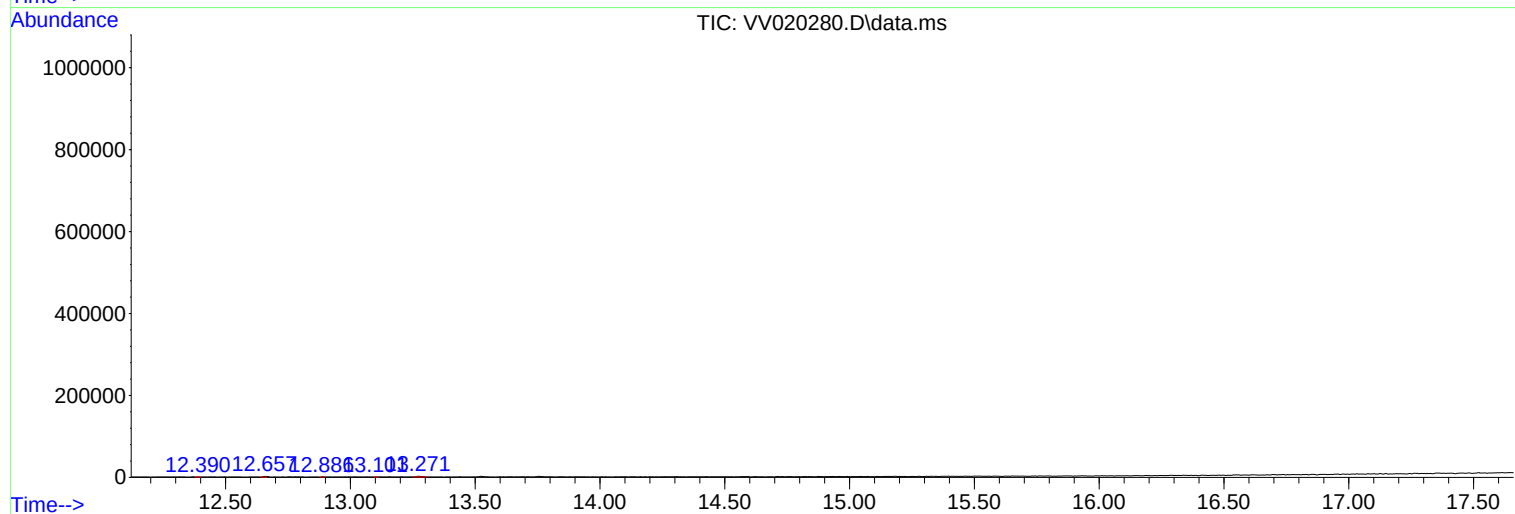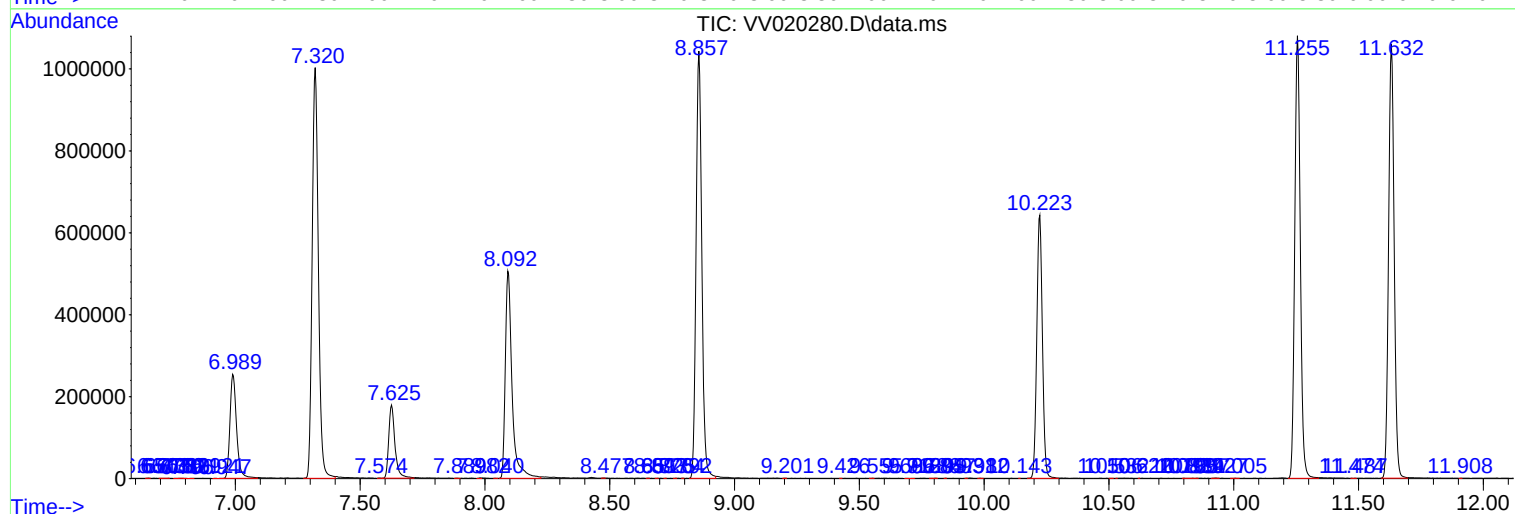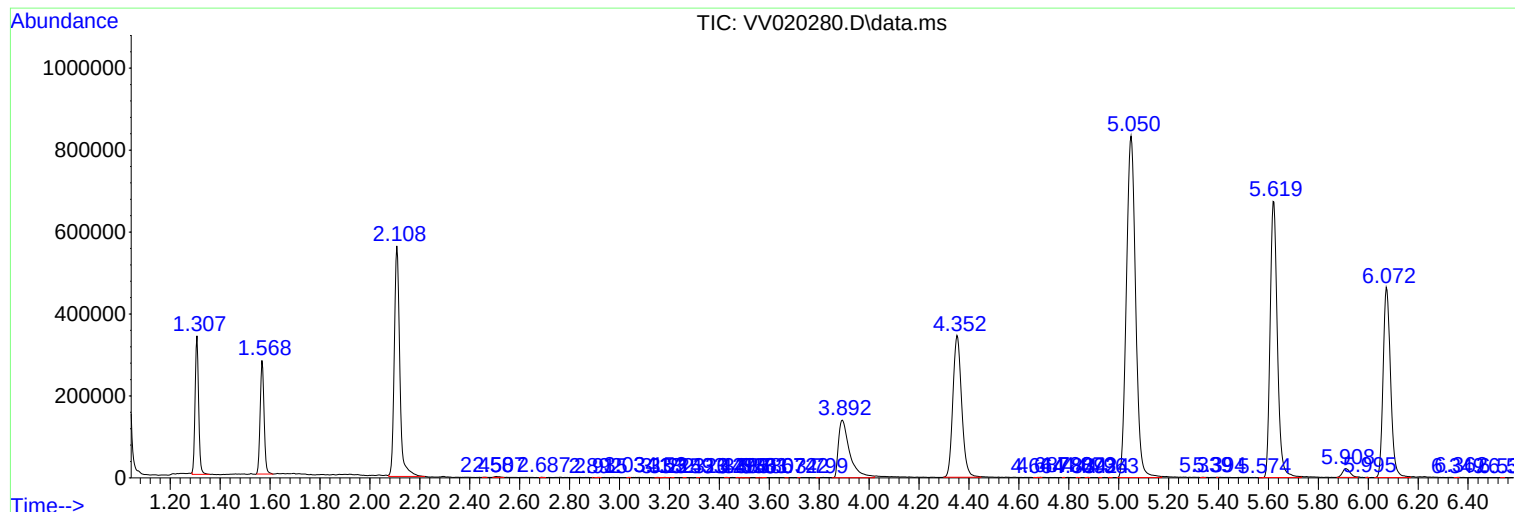

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
Data File : VV020820.D
Acq On : 08 Feb 2021 11:22
Operator : SY/MD
Sample : VV0208WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
Data File : VV020280.D
Acq On : 08 Feb 2021 11:22
Operator : SY/MD
Sample : VV0208WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK94

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
