

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
 Data File : VV020824.D
 Acq On : 08 Feb 2021 13:26
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020824.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	98	rVB	292758	292634	14.07%	1.822%
2	1.568	157	164	174	rBV	245637	276467	13.29%	1.721%
3	2.108	323	332	363	rVB	503311	769581	37.00%	4.790%
4	2.510	453	457	464	rVB6	1881	2272	0.11%	0.014%
5	2.641	495	498	502	rVB3	587	416	0.02%	0.003%
6	2.789	541	544	547	rBV2	618	324	0.02%	0.002%
7	2.834	555	558	559	rBV2	267	142	0.01%	0.001%
8	2.892	574	576	581	rBV3	317	232	0.01%	0.001%
9	2.998	605	609	614	rBV4	541	555	0.03%	0.003%
10	3.117	641	646	649	rBV2	490	474	0.02%	0.003%
11	3.156	655	658	661	rBV2	314	149	0.01%	0.001%
12	3.178	661	665	669	rBV2	243	195	0.01%	0.001%
13	3.227	678	680	681	rBV2	211	77	0.00%	0.000%
14	3.355	716	720	724	rBV3	429	323	0.02%	0.002%
15	3.397	731	733	734	rBV3	218	100	0.00%	0.001%
16	3.494	761	763	769	rVV3	523	284	0.01%	0.002%
17	3.529	772	774	778	rVB2	262	187	0.01%	0.001%
18	3.577	787	789	791	rBV2	105	63	0.00%	0.000%
19	3.603	791	797	801	rBV2	537	630	0.03%	0.004%
20	3.654	811	813	816	rBV	239	151	0.01%	0.001%
21	3.709	827	830	832	rBV	225	151	0.01%	0.001%
22	3.735	836	838	840	rVB	499	216	0.01%	0.001%
23	3.776	847	851	854	rBV2	629	387	0.02%	0.002%
24	3.799	857	858	860	rVB	307	88	0.00%	0.001%
25	3.812	860	862	863	rBV	191	85	0.00%	0.001%
26	3.895	877	888	926	rBV	130471	429646	20.66%	2.674%
27	4.352	1013	1030	1056	rBV	333304	819464	39.40%	5.101%
28	4.493	1071	1074	1076	rBV2	1001	719	0.03%	0.004%
29	4.764	1154	1158	1162	rVB4	512	422	0.02%	0.003%
30	4.802	1168	1170	1172	rBV2	292	145	0.01%	0.001%
31	4.873	1189	1192	1194	rBV	276	165	0.01%	0.001%
32	4.892	1194	1198	1200	rVV2	281	214	0.01%	0.001%
33	5.050	1229	1247	1275	rBV2	811429	2079843	100.00%	12.946%
34	5.500	1384	1387	1390	rBV3	669	501	0.02%	0.003%
35	5.535	1396	1398	1400	rBV2	415	224	0.01%	0.001%
36	5.564	1405	1407	1408	rBV2	213	75	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
 Data File : VV020824.D
 Acq On : 08 Feb 2021 13:26
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

37	5.619	1411	1424	1456	rBV	641341	1291951	62.12%	8.042%
38	5.908	1503	1514	1532	rBV4	20805	45029	2.17%	0.280%
39	6.008	1543	1545	1547	rVB	442	137	0.01%	0.001%
40	6.021	1548	1549	1551	rBV	194	84	0.00%	0.001%
41	6.072	1551	1565	1593	rBV	460226	935074	44.96%	5.820%
42	6.384	1660	1662	1667	rVB2	554	364	0.02%	0.002%
43	6.413	1669	1671	1674	rBV	296	184	0.01%	0.001%
44	6.461	1684	1686	1692	rVB3	481	371	0.02%	0.002%
45	6.497	1694	1697	1700	rBV2	210	129	0.01%	0.001%
46	6.509	1700	1701	1703	rBV	298	96	0.00%	0.001%
47	6.529	1705	1707	1709	rBV2	310	123	0.01%	0.001%
48	6.590	1724	1726	1728	rBV	203	91	0.00%	0.001%
49	6.599	1728	1729	1731	rBV	565	238	0.01%	0.001%
50	6.690	1754	1757	1760	rBV4	331	237	0.01%	0.001%
51	6.757	1775	1778	1780	rBV2	386	212	0.01%	0.001%
52	6.802	1790	1792	1795	rBV	151	84	0.00%	0.001%
53	6.841	1802	1804	1806	rVB	212	84	0.00%	0.001%
54	6.857	1806	1809	1812	rBV2	271	192	0.01%	0.001%
55	6.889	1817	1819	1822	rVV3	299	161	0.01%	0.001%
56	6.905	1822	1824	1826	rVV	320	135	0.01%	0.001%
57	6.918	1826	1828	1830	rVB	393	174	0.01%	0.001%
58	6.947	1835	1837	1838	rBV	294	102	0.00%	0.001%
59	6.989	1839	1850	1880	rBV	245568	445450	21.42%	2.773%
60	7.320	1941	1953	1987	rBV	946264	1636575	78.69%	10.187%
61	7.625	2037	2048	2069	rBV	172956	300015	14.42%	1.867%
62	7.863	2120	2122	2124	rBV2	357	143	0.01%	0.001%
63	7.921	2138	2140	2141	rBV	400	159	0.01%	0.001%
64	7.985	2153	2160	2168	rBV5	1723	2577	0.12%	0.016%
65	8.091	2178	2193	2231	rBV	486298	930072	44.72%	5.789%
66	8.580	2342	2345	2347	rBV2	549	462	0.02%	0.003%
67	8.609	2352	2354	2355	rBV2	387	190	0.01%	0.001%
68	8.857	2419	2431	2458	rBV	992470	1614997	77.65%	10.053%
69	9.152	2522	2523	2529	rVB3	653	370	0.02%	0.002%
70	9.194	2534	2536	2540	rBV4	368	317	0.02%	0.002%
71	9.307	2569	2571	2573	rVB	438	172	0.01%	0.001%
72	9.333	2573	2579	2580	rBV2	424	357	0.02%	0.002%
73	9.779	2716	2718	2722	rBV3	297	241	0.01%	0.002%
74	9.860	2739	2743	2745	rBB2	300	157	0.01%	0.001%
75	9.876	2746	2748	2750	rBV	254	157	0.01%	0.001%
76	9.905	2754	2757	2760	rBV2	342	201	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
 Data File : VV020824.D
 Acq On : 08 Feb 2021 13:26
 Operator : SY/MD
 Sample : VIBLK80
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

77	10.056	2802	2804	2807	rBV2	358	199	0.01%	0.001%
78	10.104	2815	2819	2823	rVB2	457	427	0.02%	0.003%
79	10.223	2843	2856	2873	rBV	633793	986655	47.44%	6.141%
80	10.413	2913	2915	2919	rVB3	480	167	0.01%	0.001%
81	10.577	2964	2966	2970	rBV4	670	496	0.02%	0.003%
82	10.680	2995	2998	3000	rBV	300	227	0.01%	0.001%
83	10.934	3073	3077	3082	rBV4	483	572	0.03%	0.004%
84	11.001	3095	3098	3100	rBV2	577	346	0.02%	0.002%
85	11.046	3110	3112	3114	rVB	445	193	0.01%	0.001%
86	11.059	3114	3116	3119	rBV2	367	201	0.01%	0.001%
87	11.136	3138	3140	3141	rBV	287	83	0.00%	0.001%
88	11.255	3165	3177	3203	rBV	1020389	1598952	76.88%	9.953%
89	11.631	3281	3294	3315	rBV	1019270	1590866	76.49%	9.902%
90	12.689	3620	3623	3625	rBV2	547	299	0.01%	0.002%
91	12.818	3661	3663	3665	rBV2	516	235	0.01%	0.001%




Sum of corrected areas: 16065383

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
Data File : VV02084.D
Acq On : 08 Feb 2021 13:26
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

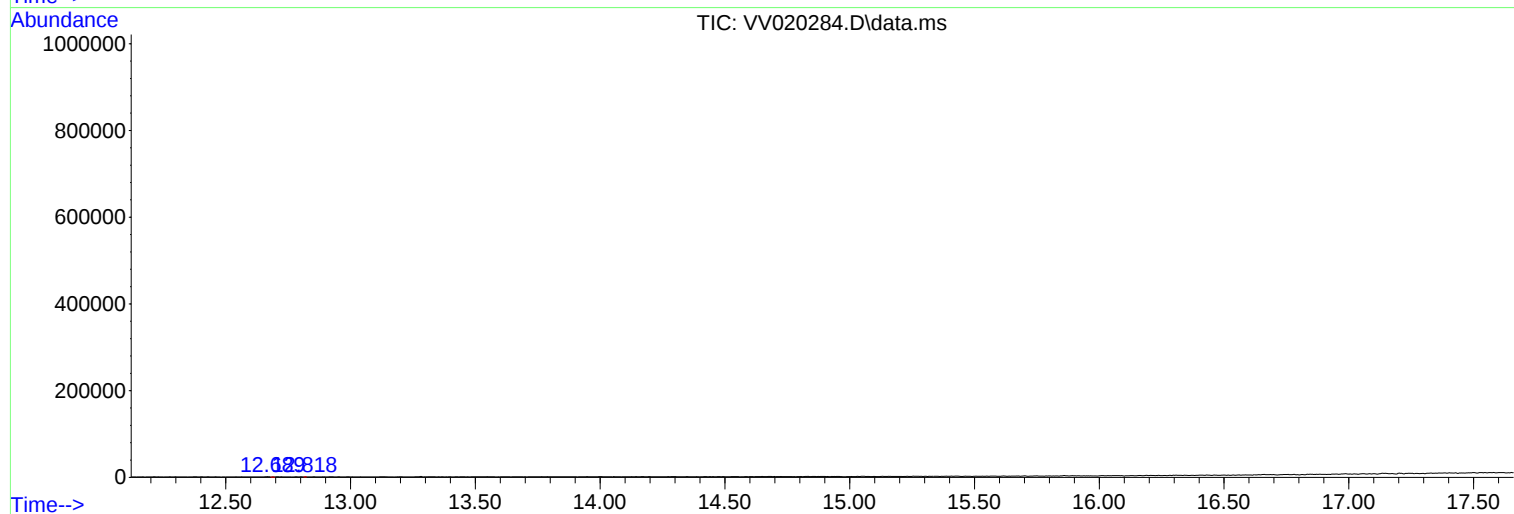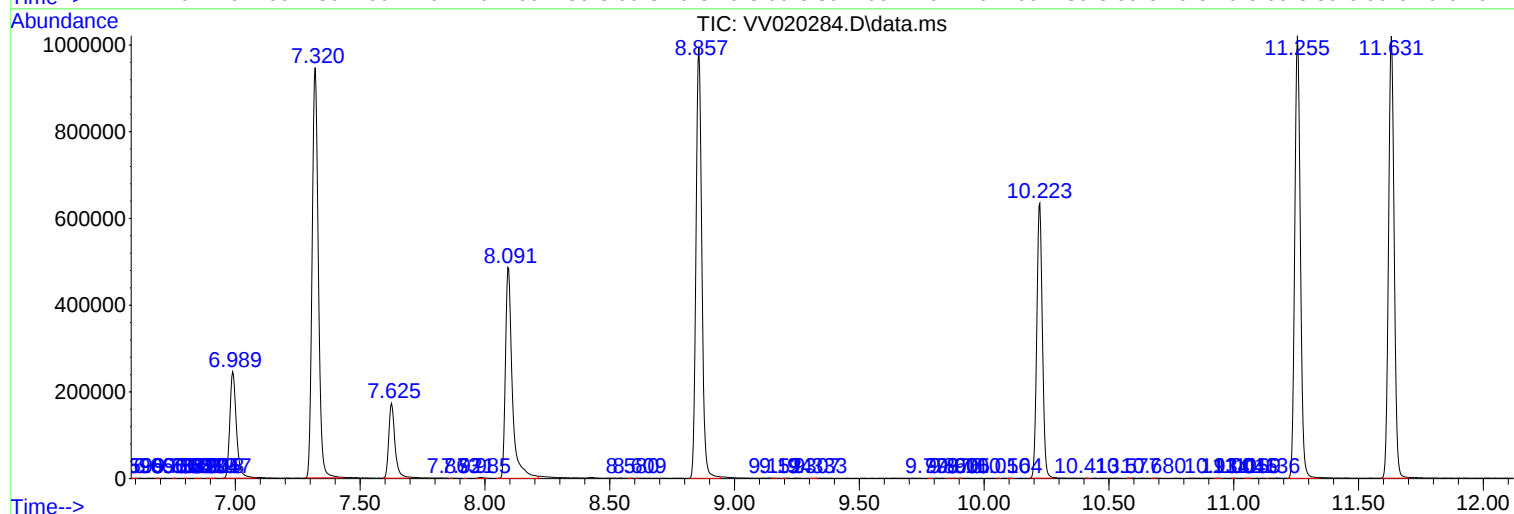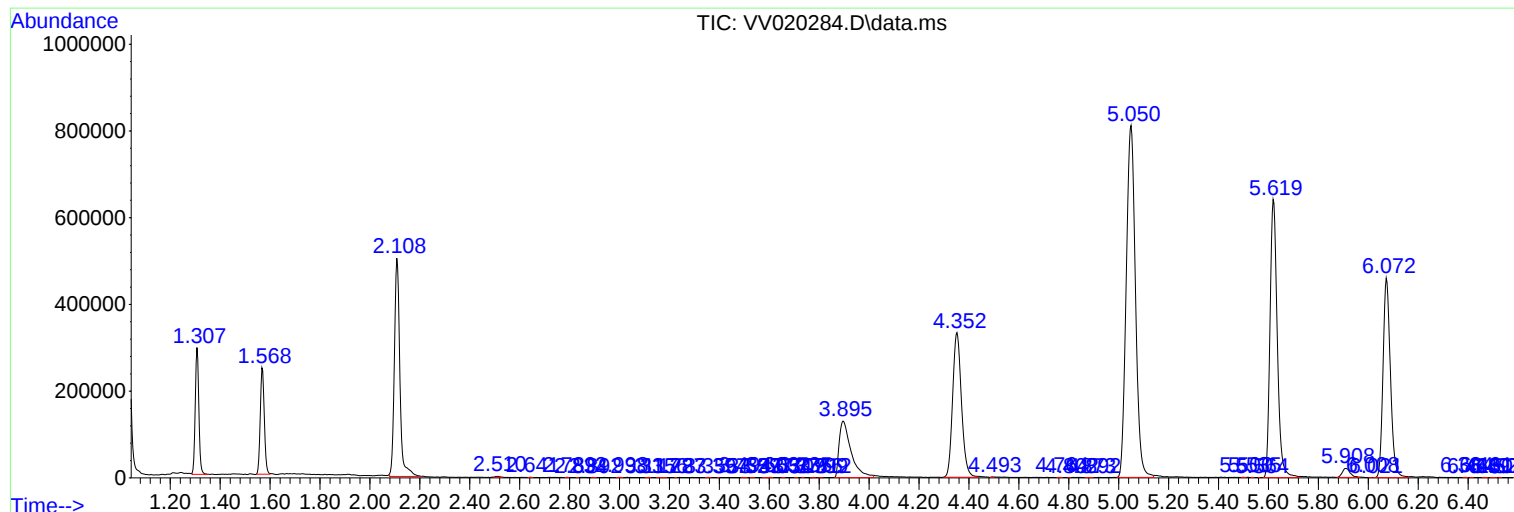

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
Data File : VV020284.D
Acq On : 08 Feb 2021 13:26
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
Data File : VV020824.D
Acq On : 08 Feb 2021 13:26
Operator : SY/MD
Sample : VIBLK80
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
