
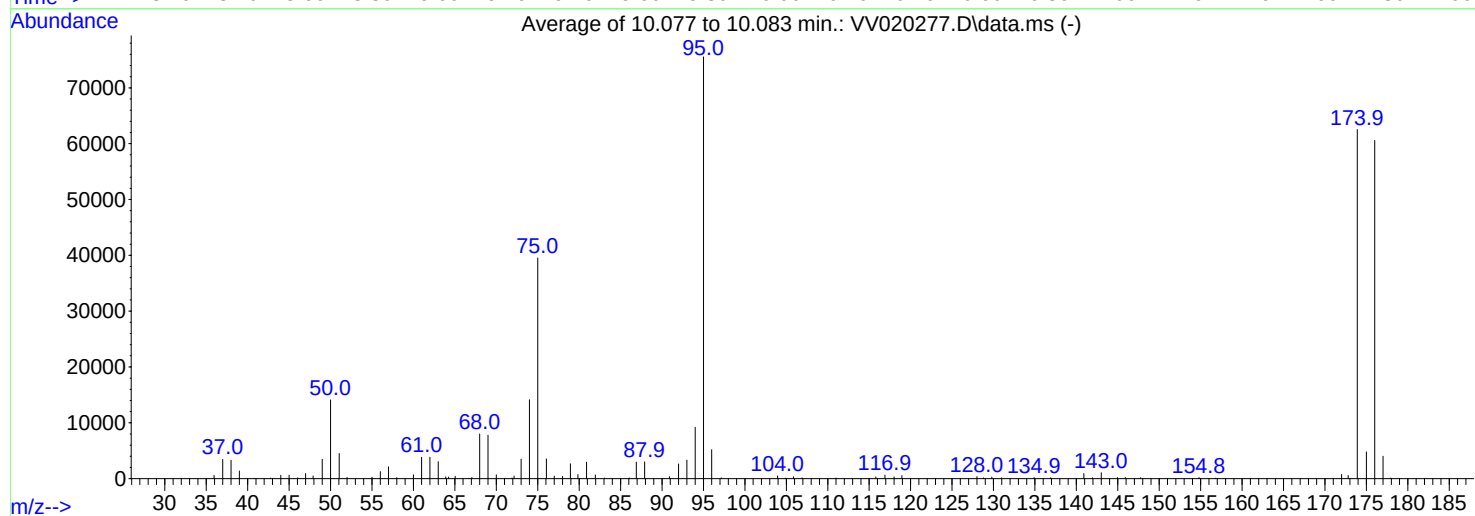


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020821\
 Data File : VV020277.D
 Acq On : 08 Feb 2021 09:13
 Operator : SY/MD
 Sample : BFB87
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB87

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 09 01:47:10 2021

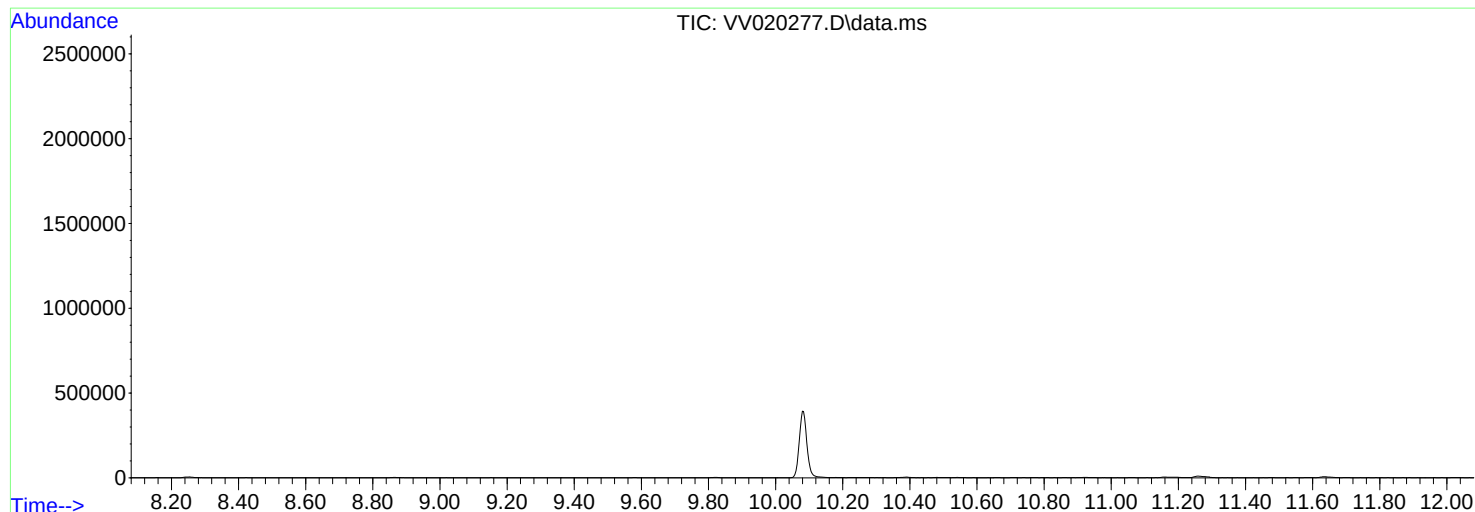

AutoFind: Scans 2826, 2827, 2828; Background Corrected with Scan 2815

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	14096	PASS
75	95	30	80	52.3	39509	PASS
95	95	100	100	100.0	75552	PASS
96	95	5	9	6.9	5193	PASS
173	174	0.00	2	0.9	571	PASS
174	95	50	120	82.8	62533	PASS
175	174	5	9	7.7	4784	PASS
176	174	95	101	96.9	60589	PASS
177	176	5	9	6.6	4020	PASS

m/z	Abundance
36.00	858.0
37.00	3365.0
38.00	3270.0
39.00	1466.0
40.00	257.0
40.80	117.0
42.80	101.0
44.00	991.0
45.00	582.0
46.00	174.0
47.00	906.0
47.90	440.0
49.00	3283.0
50.00	13513.0
51.10	4385.0
52.00	265.0
55.00	243.0
56.00	1058.0
57.00	2105.0
57.90	205.0
60.00	632.0
61.00	3456.0
62.00	3903.0
63.00	2951.0
63.90	337.0
64.20	304.0
65.10	390.0
67.10	204.0
68.00	7784.0
69.00	7450.0
70.00	629.0
71.90	372.0
72.20	412.0
73.00	3496.0
74.00	13772.0
75.00	37000.0
76.00	3406.0
77.00	427.0
78.00	415.0
78.90	2512.0
79.80	802.0
80.90	2747.0
82.00	707.0
83.10	111.0
86.00	119.0
86.90	2927.0
87.90	2755.0
90.90	346.0
92.00	2457.0
93.00	3270.0
94.00	8586.0
95.00	70736.0
96.00	5007.0
97.20	127.0
103.90	542.0
105.90	320.0
106.90	136.0
111.00	108.0
115.00	120.0
115.80	283.0
116.90	653.0
118.00	245.0
118.90	604.0
128.00	332.0
128.80	159.0
129.80	243.0
130.90	119.0
134.90	214.0
136.90	153.0
140.90	800.0
141.90	139.0
143.00	1021.0
144.90	179.0
145.90	134.0
147.80	147.0
154.90	182.0
172.00	738.0
172.80	583.0
173.90	57072.0
175.00	4362.0
176.00	55440.0
177.00	3733.0
178.00	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
36.00	930.0
37.00	3598.0
38.00	3511.0
39.00	1411.0
40.00	241.0
40.80	104.0
42.70	113.0
44.00	1060.0
45.00	659.0
46.00	167.0
47.00	943.0
47.90	491.0
49.00	3583.0
50.00	14507.0
51.00	4685.0
52.00	254.0
55.00	275.0
56.00	1319.0
57.00	2200.0
58.00	159.0
60.00	700.0
61.00	3968.0
62.00	3972.0
63.00	3132.0
63.90	326.0
64.30	315.0
65.00	434.0
67.10	219.0
68.00	8167.0
69.00	8091.0
70.00	715.0
72.10	484.0
73.00	3651.0
74.00	14635.0
75.00	40816.0
76.00	3642.0
77.00	483.0
78.00	446.0
79.00	2747.0
79.90	785.0
80.90	3070.0
81.90	658.0
83.10	146.0
86.00	133.0
86.90	3016.0
87.90	3131.0
90.90	354.0
92.00	2783.0
93.00	3406.0
94.00	9494.0
95.00	78104.0
96.00	5367.0
97.10	141.0
104.00	522.0
104.90	115.0
105.90	340.0
106.90	142.0
111.00	131.0
115.00	109.0
115.80	316.0
116.90	645.0
118.00	315.0
119.00	564.0
128.00	397.0
128.80	167.0
129.80	285.0
130.90	134.0
134.90	208.0
136.90	181.0
140.90	921.0
141.90	144.0
143.00	1126.0
145.00	219.0
145.90	208.0
147.70	195.0
154.80	179.0
156.80	121.0
172.00	782.0
172.80	596.0
173.90	64672.0
175.00	4985.0
176.00	62464.0
177.00	4183.0
178.00	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
36.00	930.0
37.00	3358.0
38.00	3453.0
39.00	1251.0
40.00	241.0
42.70	104.0
44.00	950.0
45.00	663.0
46.10	136.0
47.00	889.0
47.90	539.0
49.00	3562.0
50.00	14267.0
51.00	4469.0
52.00	201.0
55.00	285.0
56.00	1454.0
57.00	2043.0
58.10	119.0
60.00	704.0
61.00	4054.0
62.00	3636.0
63.00	3039.0
63.90	291.0
64.20	260.0
65.00	473.0
66.70	226.0
67.00	216.0
68.00	8043.0
69.00	7746.0
70.00	710.0
72.10	487.0
73.00	3324.0
74.00	13978.0
75.00	40712.0
76.10	3505.0
77.00	482.0
78.00	387.0
79.00	2762.0
79.80	673.0
80.90	3024.0
81.90	616.0
83.00	114.0
86.10	107.0
86.90	2899.0
87.90	3146.0
90.90	326.0
92.00	2708.0
93.00	3259.0
94.00	9493.0
95.00	77816.0
96.00	5206.0
97.10	149.0
103.90	423.0
104.90	148.0
105.80	372.0
106.90	150.0
111.00	130.0
115.80	347.0
116.90	568.0
118.00	364.0
119.00	439.0
128.00	387.0
128.80	150.0
129.80	307.0
131.00	150.0
134.90	155.0
136.90	152.0
140.90	1010.0
142.00	147.0
143.00	1067.0
145.00	230.0
145.90	228.0
147.70	213.0
154.70	202.0
156.80	136.0
161.00	109.0
172.00	728.0
172.80	533.0
173.90	65856.0
175.00	5004.0
176.00	63864.0
177.00	4144.0
177.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.80	293.0
38.20	105.0
39.90	283.0
44.00	384.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87