




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034101.D
Acq On : 09 Feb 2024 10:49
Operator : SY/MD
Sample : P1401-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/09/2024
Supervised By :Mahesh Dadoda 02/09/2024

Quant Time: Feb 09 13:40:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 09 03:48:51 2024
Response via : Initial Calibration

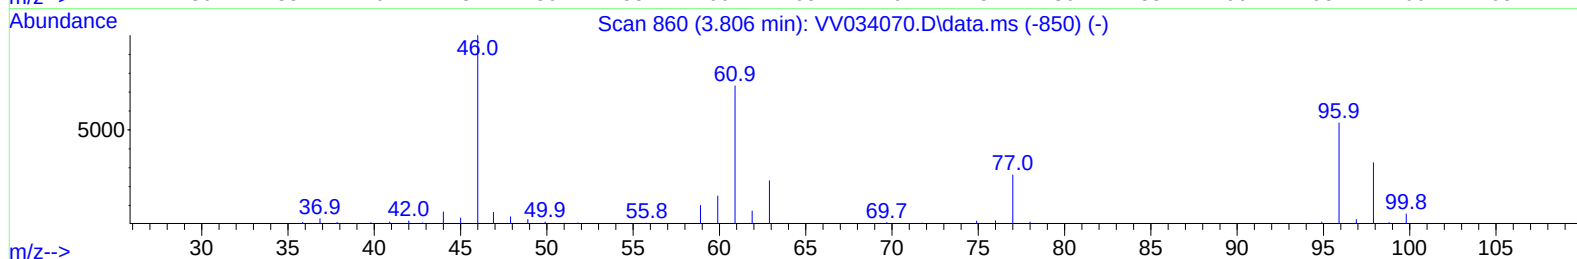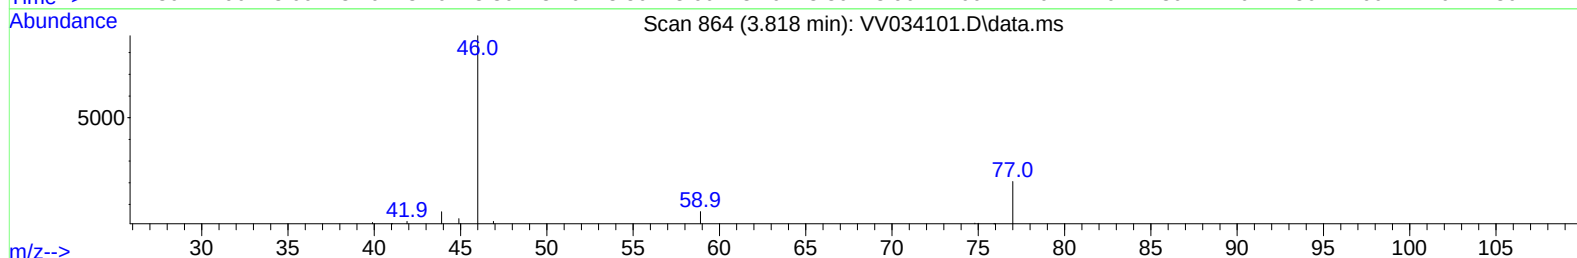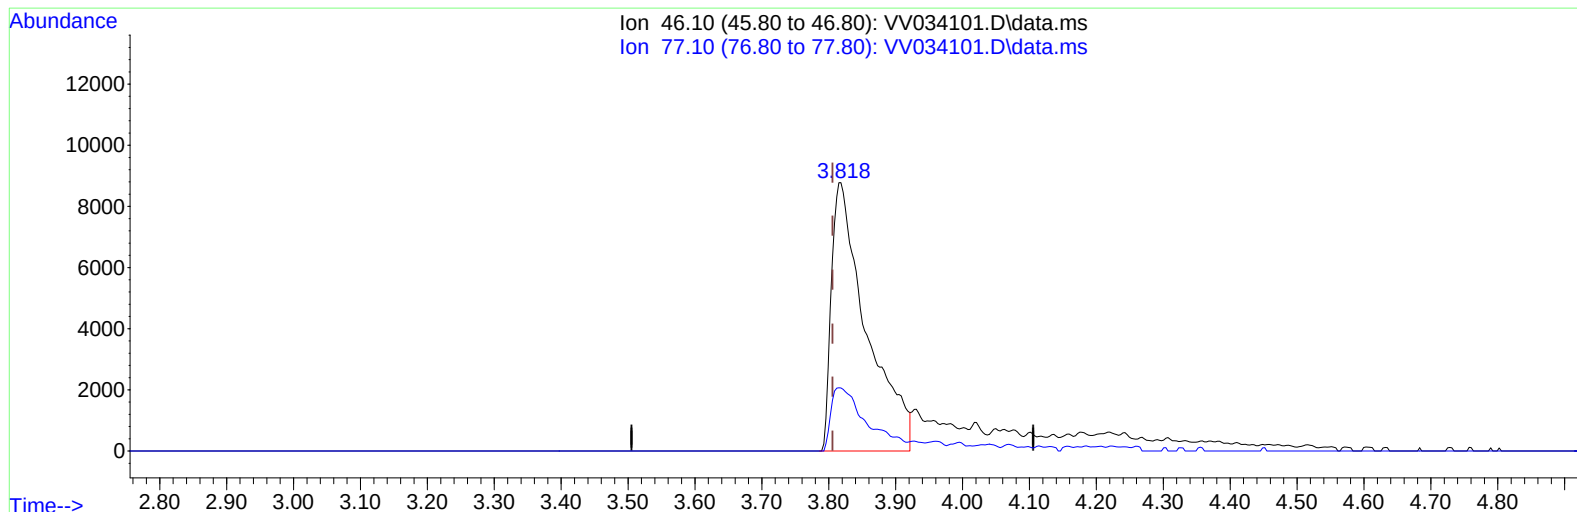

TIC: VV034101.D\data.ms

(20) 2-Butanone-d5 (S)**3.818min (+ 0.013) 32.27 ug/L****response 31927**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	24.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034101.D
Acq On : 09 Feb 2024 10:49
Operator : SY/MD
Sample : P1401-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/09/2024
Supervised By :Mahesh Dadoda 02/09/2024

Quant Time: Feb 09 13:40:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 09 03:48:51 2024
Response via : Initial Calibration

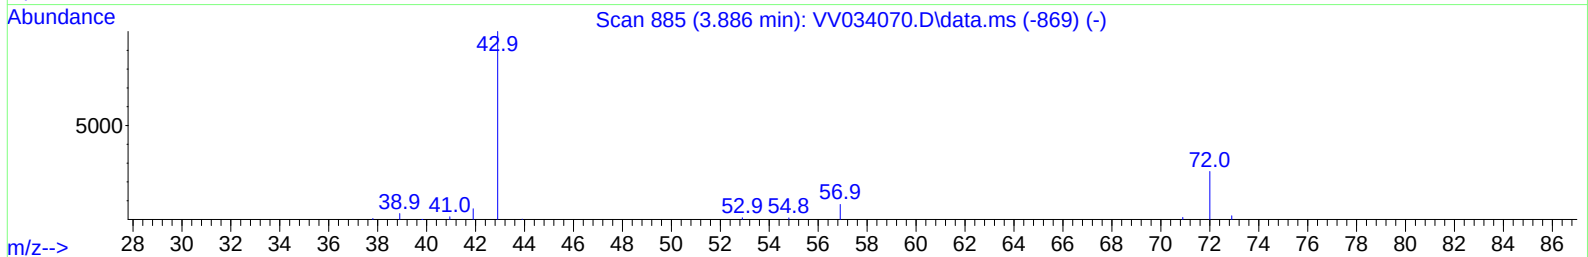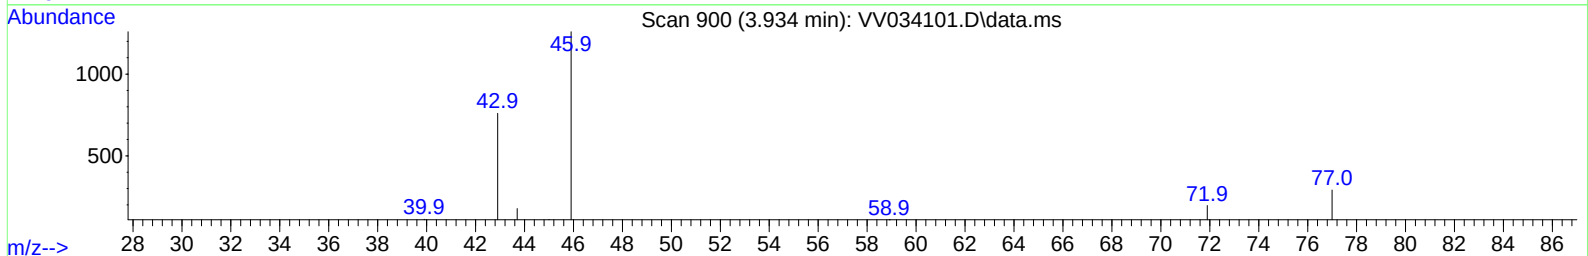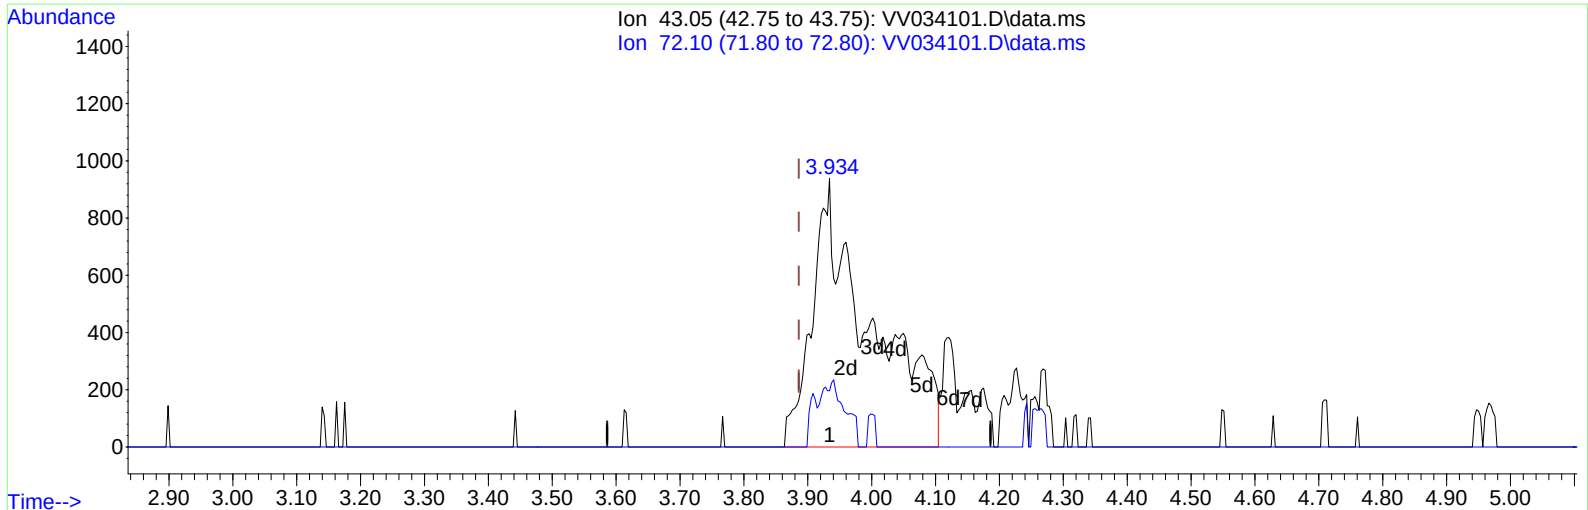

TIC: VV034101.D\data.ms

(21) 2-Butanone (T)

3.934min (+ 0.048) 5.99 ug/L m

response 5937

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	7.90	3.67#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034101.D
Acq On : 09 Feb 2024 10:49
Operator : SY/MD
Sample : P1401-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/09/2024
Supervised By :Mahesh Dadoda 02/09/2024

Quant Time: Feb 09 13:40:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 09 03:48:51 2024
Response via : Initial Calibration

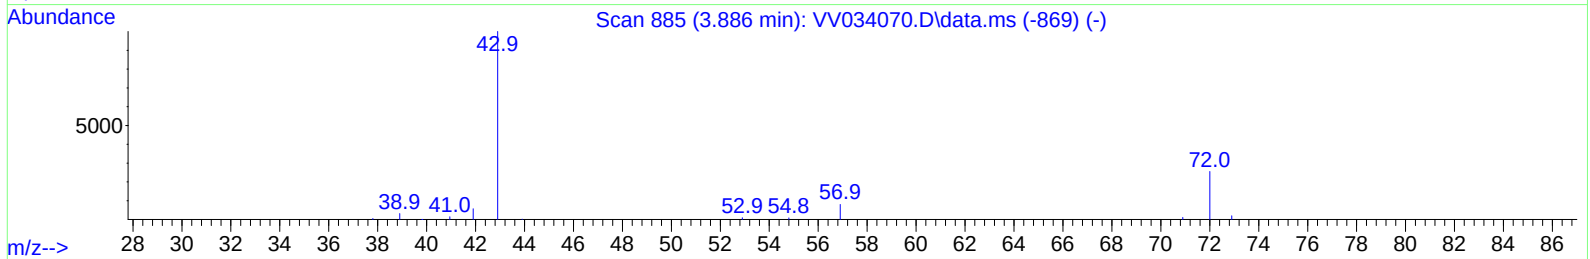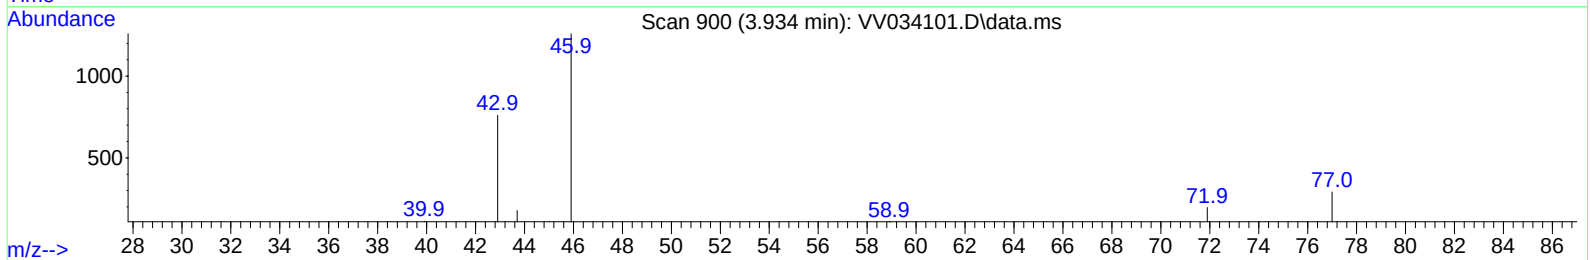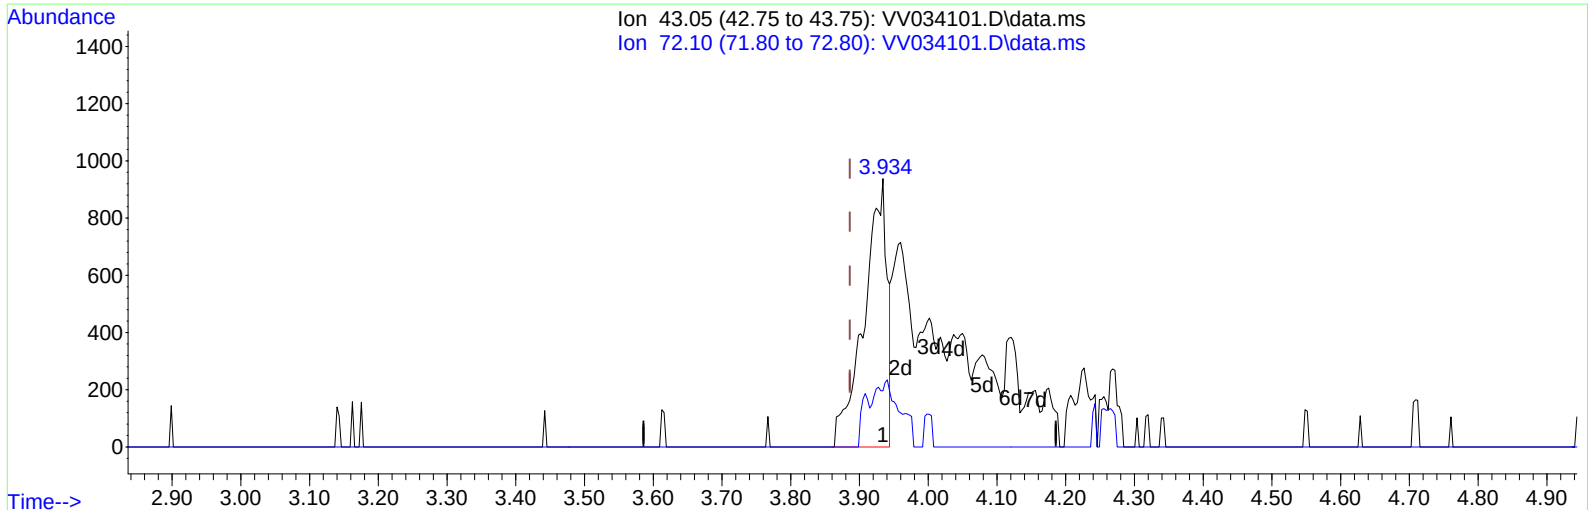

TIC: VV034101.D\data.ms

(21) 2-Butanone (T)

3.934min (+ 0.048) 2.18 ug/L

response 2166

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	7.90	10.06
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034101.D
Acq On : 09 Feb 2024 10:49
Operator : SY/MD
Sample : P1401-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/09/2024
Supervised By :Mahesh Dadoda 02/09/2024

Quant Time: Feb 09 13:40:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 09 03:48:51 2024
Response via : Initial Calibration

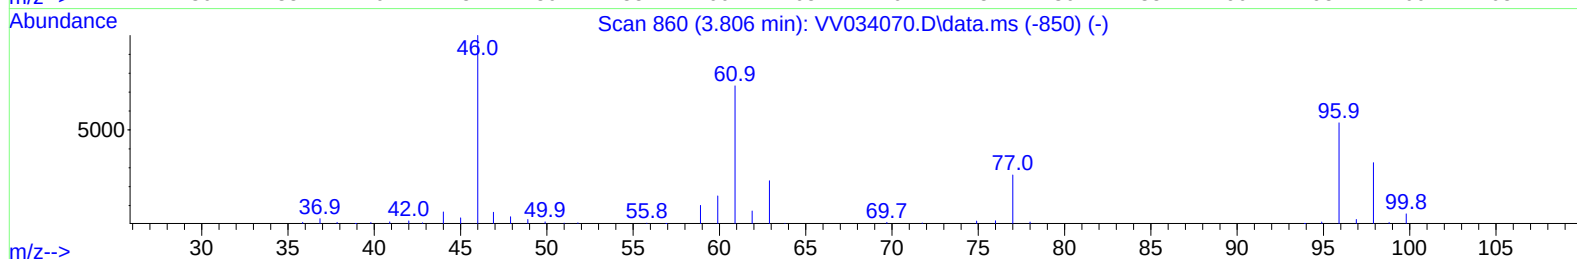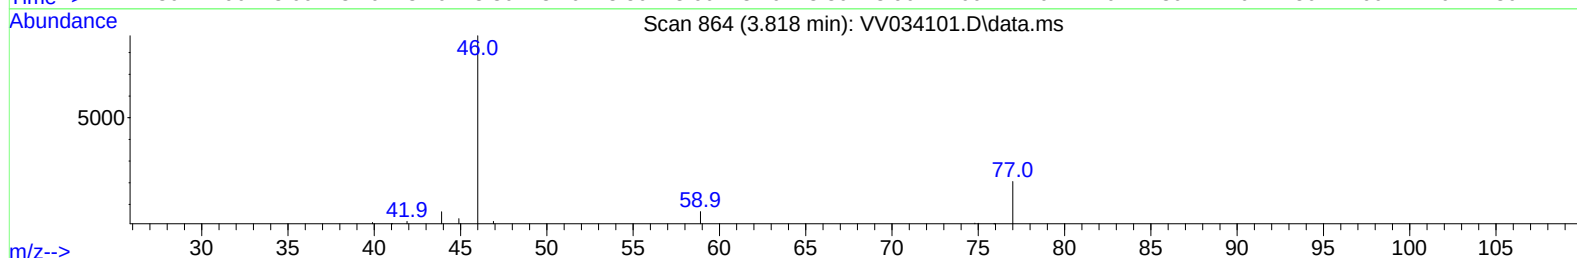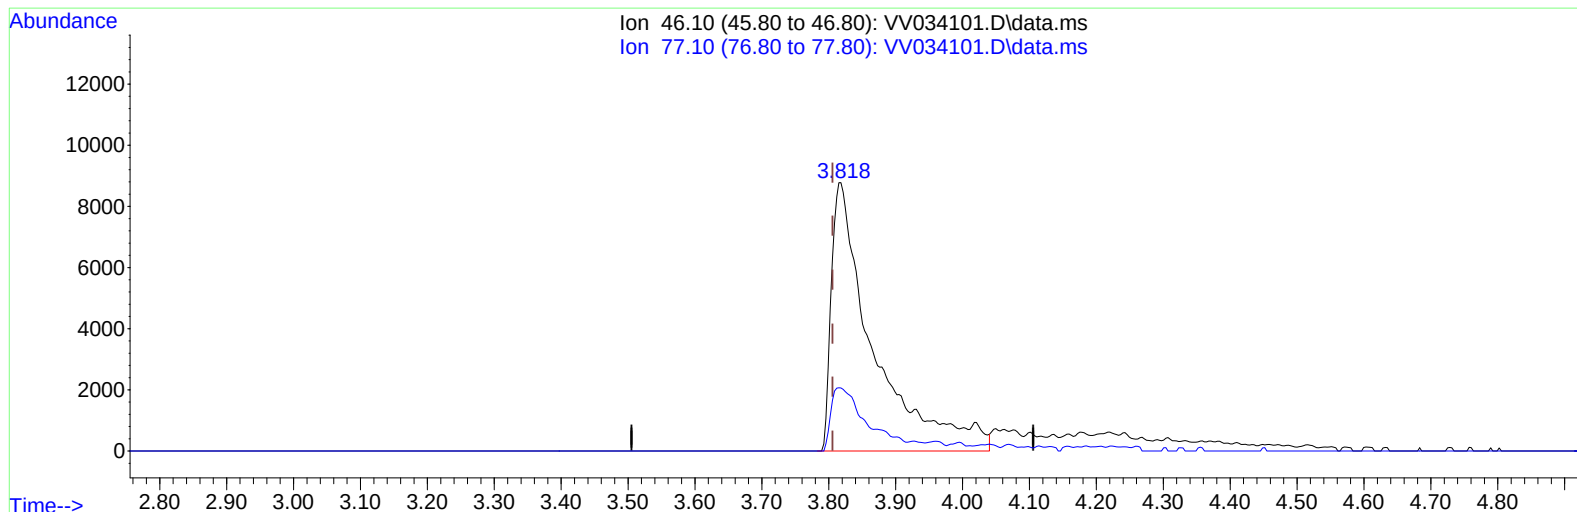

TIC: VV034101.D\data.ms

(20) 2-Butanone-d5 (S)

3.818min (+ 0.013) 38.63 ug/L m

response 38223

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.80	20.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW020924\
 Data File : VW034101.D
 Acq On : 09 Feb 2024 10:49
 Operator : SY/MD
 Sample : P1401-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AH8

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 02/09/2024
 Supervised By :Mahesh Dadoda 02/09/2024

Quant Time: Feb 09 13:40:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 09 03:48:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.538	114	76071	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	72105	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	37285	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	28553	4.846	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.000%
7) Chloroethane-d5	1.535	69	23251	4.506	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.200%
11) 1,1-Dichloroethene-d2	2.059	65	13444	4.732	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.600%
20) 2-Butanone-d5	3.818	46	38223m	38.630	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	77.260%
24) Chloroform-d	4.256	84	48901	4.568	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.400%
26) 1,2-Dichloroethane-d4	4.947	65	24584	4.914	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%
32) Benzene-d6	4.963	84	96789	4.474	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.400%
36) 1,2-Dichloropropane-d6	5.992	67	26450	4.374	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.400%
41) Toluene-d8	7.246	98	88378	4.445	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.000%
43) trans-1,3-Dichloroprop...	7.561	79	10294	4.508	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.200%
46) 2-Hexanone-d5	8.027	63	32355	39.693	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.380%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	16826	4.590	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.800%
66) 1,2-Dichlorobenzene-d4	11.561	152	32436	4.783	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.600%
Target Compounds					Qvalue	
21) 2-Butanone	3.934	43	5937m	5.985	ug/L	
53) m,p-Xylene	9.082	106	1583	0.157	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034101.D
Acq On : 09 Feb 2024 10:49
Operator : SY/MD
Sample : P1401-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AH8

Manual IntegrationsAPPROVED

Quant Time: Feb 09 13:40:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 09 03:48:51 2024
Response via : Initial Calibration

Reviewed By :John Carlone 02/09/2024
Supervised By :Mahesh Dadoda 02/09/2024

