

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
 Data File : VV034102.D
 Acq On : 09 Feb 2024 11:13
 Operator : SY/MD
 Sample : P1401-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AJ9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034102.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	45615	48888	17.35%	2.117%
2	1.532	146	153	166	rBV	38707	45336	16.09%	1.963%
3	1.973	281	290	300	rVB4	3987	6095	2.16%	0.264%
4	2.060	307	317	332	rBV	84925	121301	43.04%	5.253%
5	2.455	431	440	447	rVB5	2322	3911	1.39%	0.169%
6	3.831	855	868	893	rBV3	16104	69109	24.52%	2.993%
7	4.252	984	999	1025	rBV	48278	123492	43.82%	5.348%
8	4.960	1205	1219	1250	rBV3	112132	281830	100.00%	12.206%
9	5.535	1385	1398	1421	rBV	91075	188178	66.77%	8.150%
10	5.992	1528	1540	1564	rBV2	58901	124811	44.29%	5.406%
11	6.918	1819	1828	1850	rBV	30734	59466	21.10%	2.575%
12	7.246	1919	1930	1956	rBV	139833	249580	88.56%	10.809%
13	7.561	2020	2028	2044	rBV	16939	30759	10.91%	1.332%
14	7.876	2118	2126	2137	rVB4	1907	3246	1.15%	0.141%
15	8.030	2165	2174	2205	rBV	101583	216853	76.94%	9.392%
16	8.786	2399	2409	2439	rBV	137043	231180	82.03%	10.012%
17	10.156	2825	2835	2854	rVB	37908	60804	21.57%	2.633%
18	10.329	2879	2889	2899	rBV	4230	6495	2.30%	0.281%
19	11.188	3143	3156	3178	rBV	147162	230356	81.74%	9.977%
20	11.561	3262	3272	3291	rBV	131854	207269	73.54%	8.977%




Sum of corrected areas: 2308959

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034102.D
Acq On : 09 Feb 2024 11:13
Operator : SY/MD
Sample : P1401-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

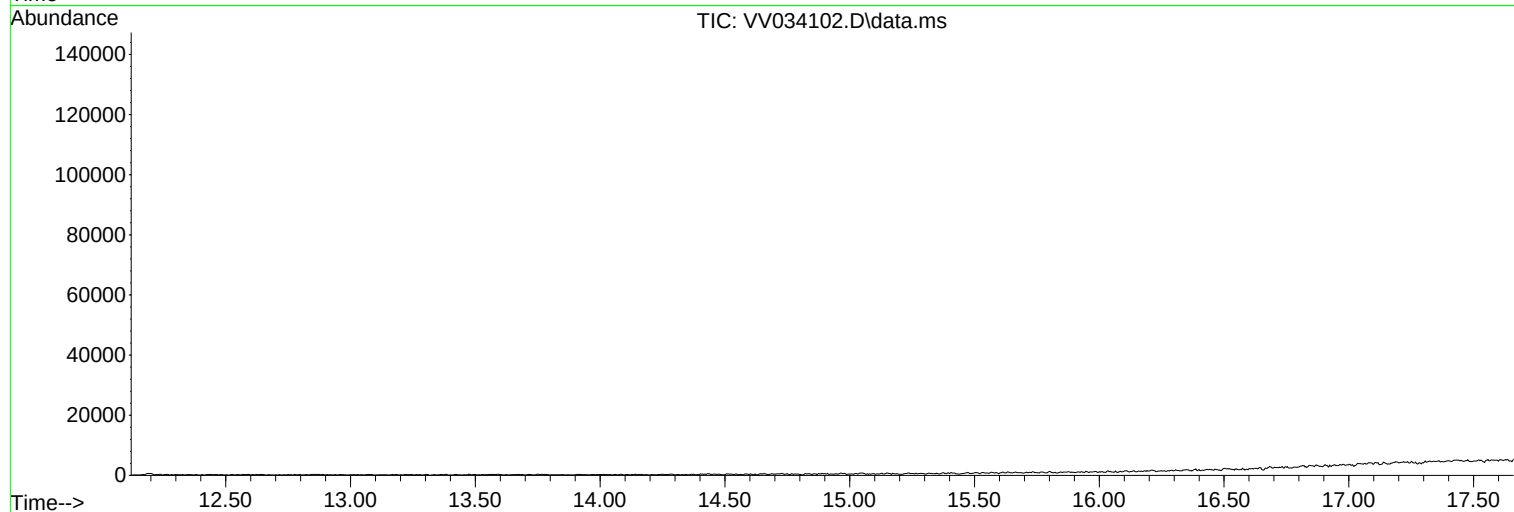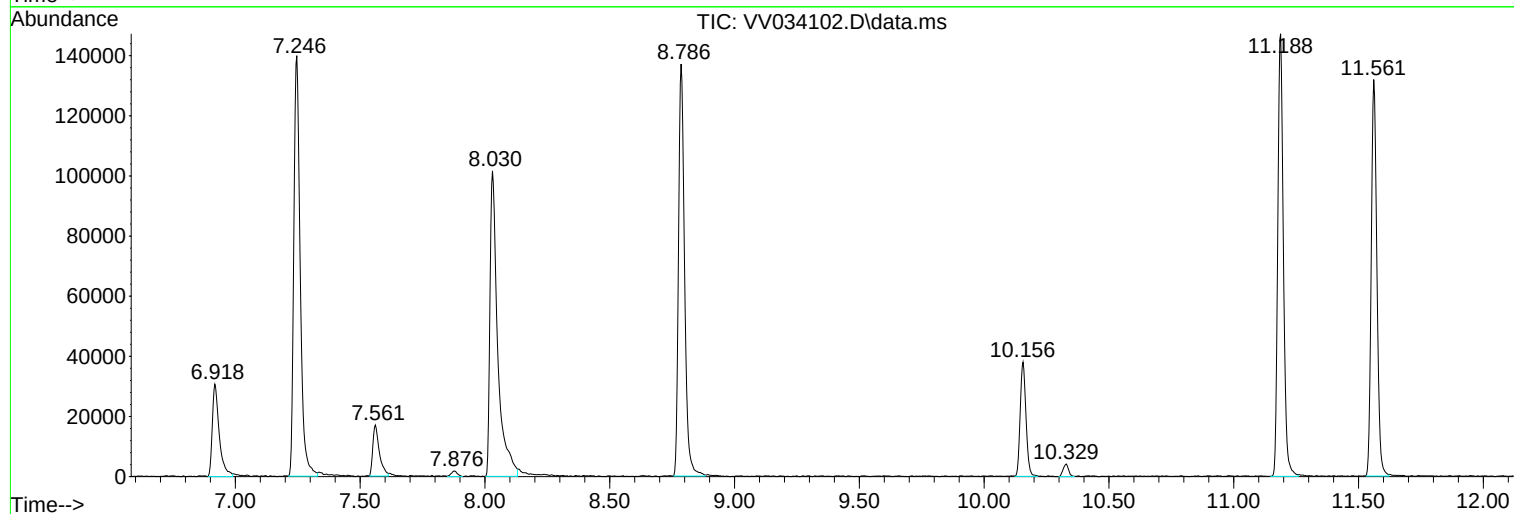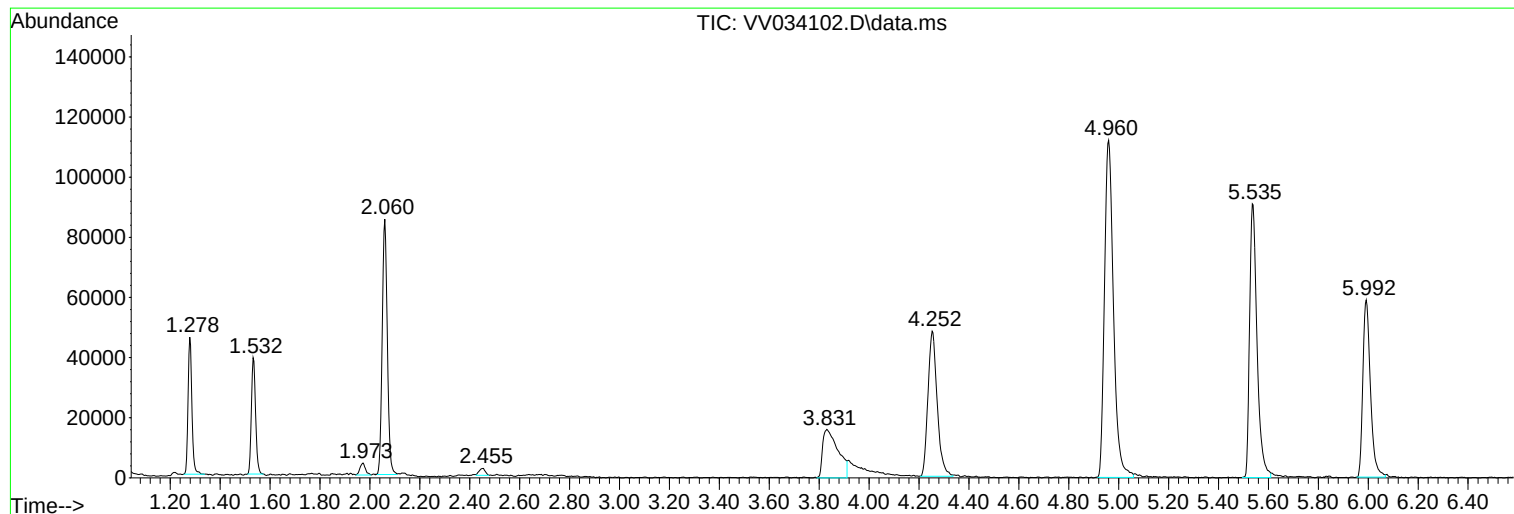

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034102.D
Acq On : 09 Feb 2024 11:13
Operator : SY/MD
Sample : P1401-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034102.D
Acq On : 09 Feb 2024 11:13
Operator : SY/MD
Sample : P1401-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
