

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
 Data File : VV034118.D
 Acq On : 09 Feb 2024 17:39
 Operator : SY/MD
 Sample : P1402-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV034118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.166	34	39	46	rBV2	1897	2167	1.26%	0.161%
2	1.281	66	75	87	rBV	23830	26007	15.14%	1.931%
3	1.532	146	153	169	rVB	20591	23635	13.76%	1.755%
4	2.060	307	317	328	rBV	44714	65938	38.38%	4.895%
5	2.114	329	334	344	rVB3	3428	5133	2.99%	0.381%
6	2.452	430	439	450	rBV2	7022	11390	6.63%	0.846%
7	3.796	848	857	886	rBV2	19854	55317	32.20%	4.107%
8	4.252	985	999	1020	rBV2	24625	63321	36.86%	4.701%
9	4.522	1073	1083	1093	rBV4	1009	2461	1.43%	0.183%
10	4.960	1202	1219	1243	rBV3	59432	148644	86.52%	11.035%
11	5.539	1387	1399	1418	rBV2	49578	102301	59.54%	7.595%
12	5.995	1529	1541	1564	rBV2	31887	66868	38.92%	4.964%
13	6.921	1820	1829	1852	rBV2	15605	30189	17.57%	2.241%
14	7.246	1920	1930	1958	rBV	71316	127534	74.23%	9.468%
15	7.564	2021	2029	2044	rBV2	8850	17413	10.13%	1.293%
16	8.027	2164	2173	2206	rBV	87495	171811	100.00%	12.755%
17	8.786	2399	2409	2432	rBV	76897	129487	75.37%	9.613%
18	10.156	2824	2835	2851	rBV2	27042	43513	25.33%	3.230%
19	11.188	3146	3156	3176	rBV	85336	134080	78.04%	9.954%
20	11.564	3262	3273	3291	rBV	74757	117886	68.61%	8.752%
21	17.098	4989	4994	4999	rBV7	1375	1888	1.10%	0.140%




Sum of corrected areas: 1346983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034118.D
Acq On : 09 Feb 2024 17:39
Operator : SY/MD
Sample : P1402-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

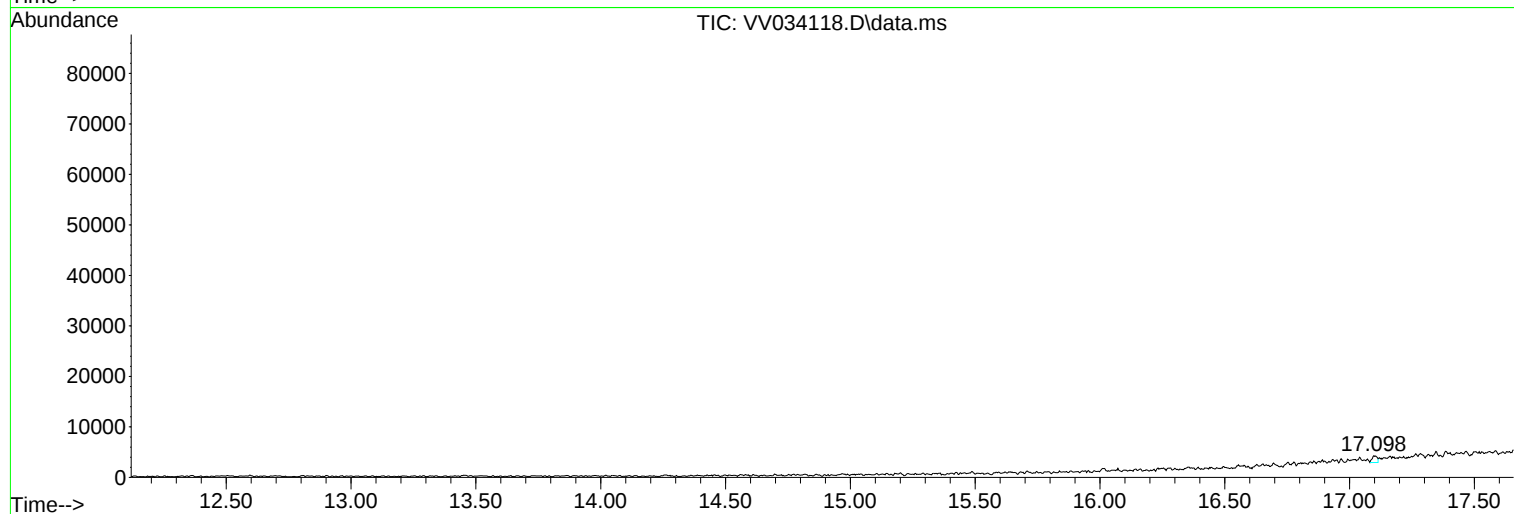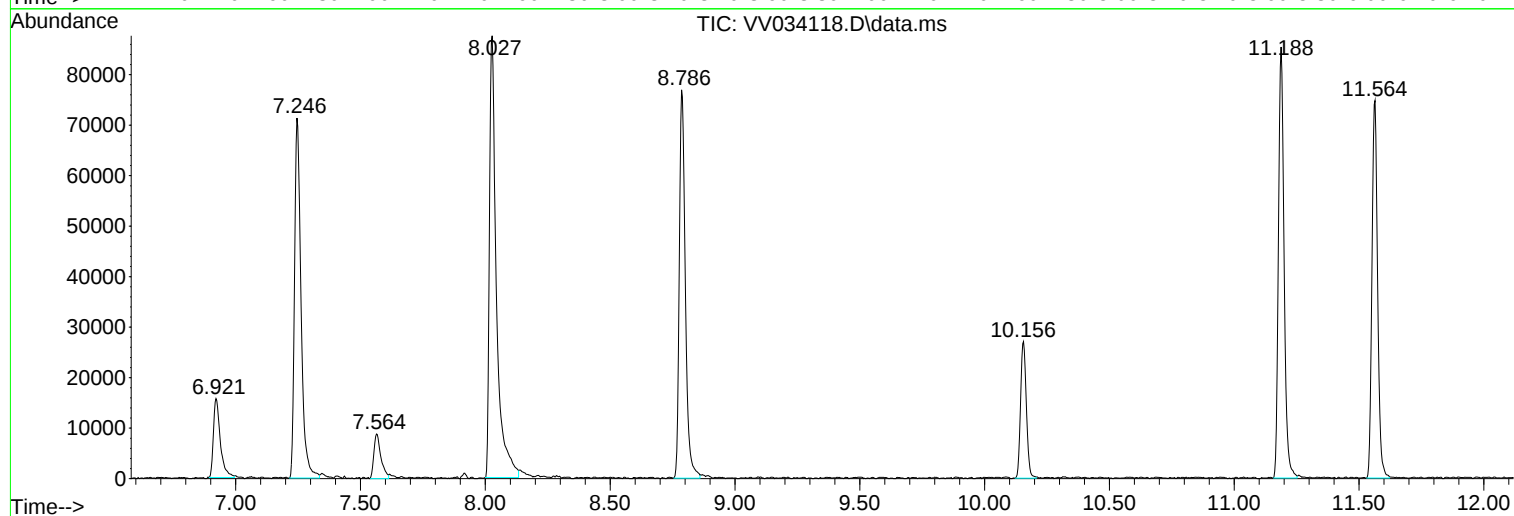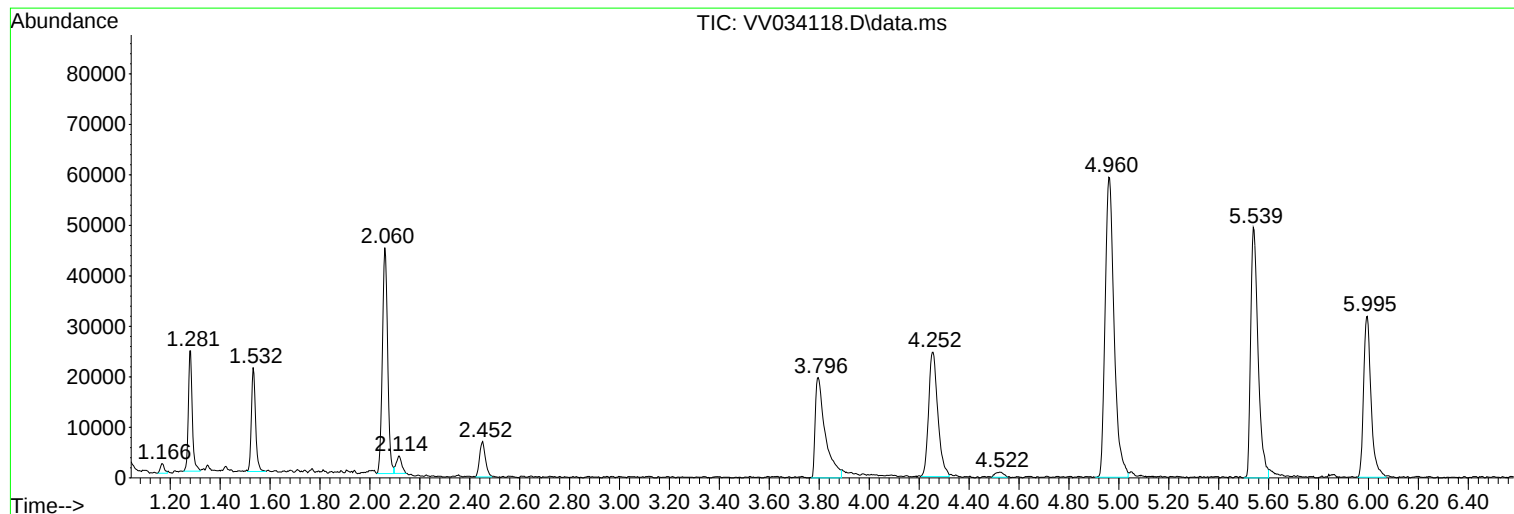

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034118.D
Acq On : 09 Feb 2024 17:39
Operator : SY/MD
Sample : P1402-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034118.D
Acq On : 09 Feb 2024 17:39
Operator : SY/MD
Sample : P1402-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
