

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
 Data File : VV034120.D
 Acq On : 09 Feb 2024 18:28
 Operator : SY/MD
 Sample : P1402-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV034120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	65	74	87	rBV	39267	45557	17.86%	1.849%
2	1.536	146	154	176	rVB	35107	43720	17.14%	1.774%
3	2.063	307	318	333	rBV2	77360	120646	47.30%	4.895%
4	3.796	847	857	884	rBV	24231	72336	28.36%	2.935%
5	4.256	984	1000	1035	rVB5	46467	137583	53.94%	5.583%
6	4.738	1132	1150	1174	rBV	50732	125880	49.35%	5.108%
7	4.960	1205	1219	1251	rBV2	99454	255067	100.00%	10.350%
8	5.539	1388	1399	1420	rBV	83740	173933	68.19%	7.058%
9	5.841	1483	1493	1516	rBV3	24868	54206	21.25%	2.200%
10	5.992	1529	1540	1567	rBV	54300	115920	45.45%	4.704%
11	6.918	1819	1828	1856	rBV2	26141	52793	20.70%	2.142%
12	7.246	1920	1930	1960	rBV	127192	228622	89.63%	9.277%
13	7.561	2017	2028	2051	rBV2	14799	29193	11.45%	1.185%
14	7.908	2125	2136	2154	rVB	67502	116605	45.72%	4.732%
15	8.027	2164	2173	2212	rBV	102851	206492	80.96%	8.379%
16	8.786	2396	2409	2433	rBV	127203	216720	84.97%	8.794%
17	10.156	2825	2835	2853	rBV	36172	56656	22.21%	2.299%
18	11.188	3144	3156	3178	rBV	138863	219031	85.87%	8.888%
19	11.561	3261	3272	3290	rBV	123274	193479	75.85%	7.851%




Sum of corrected areas: 2464439

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034120.D
Acq On : 09 Feb 2024 18:28
Operator : SY/MD
Sample : P1402-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

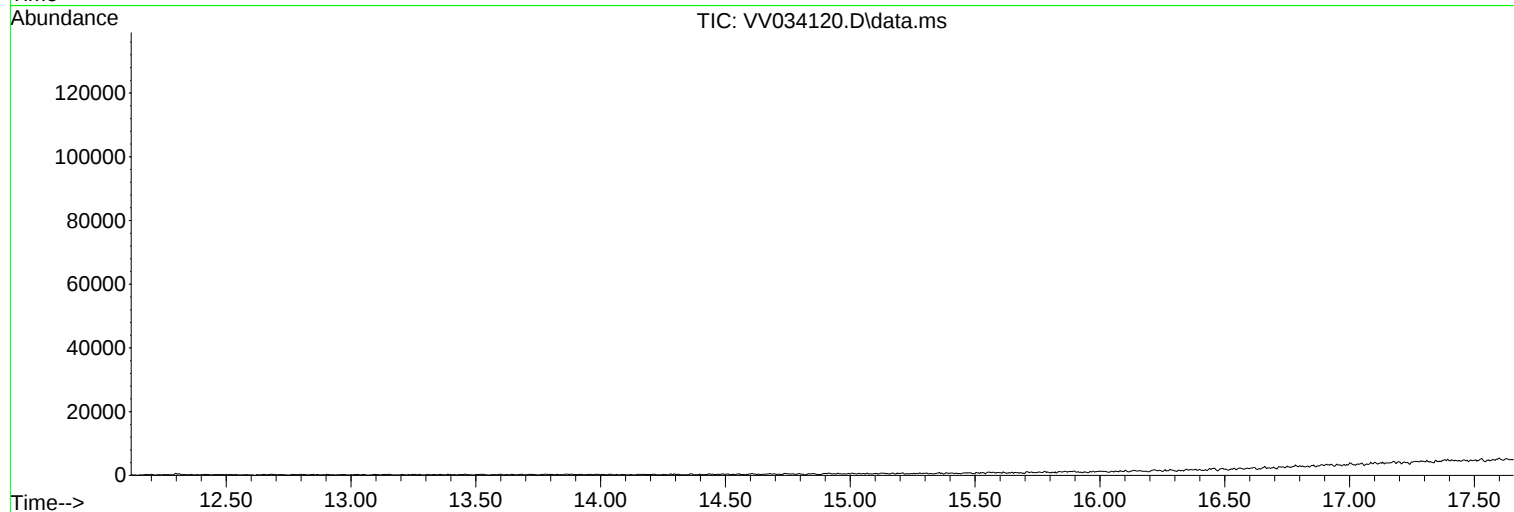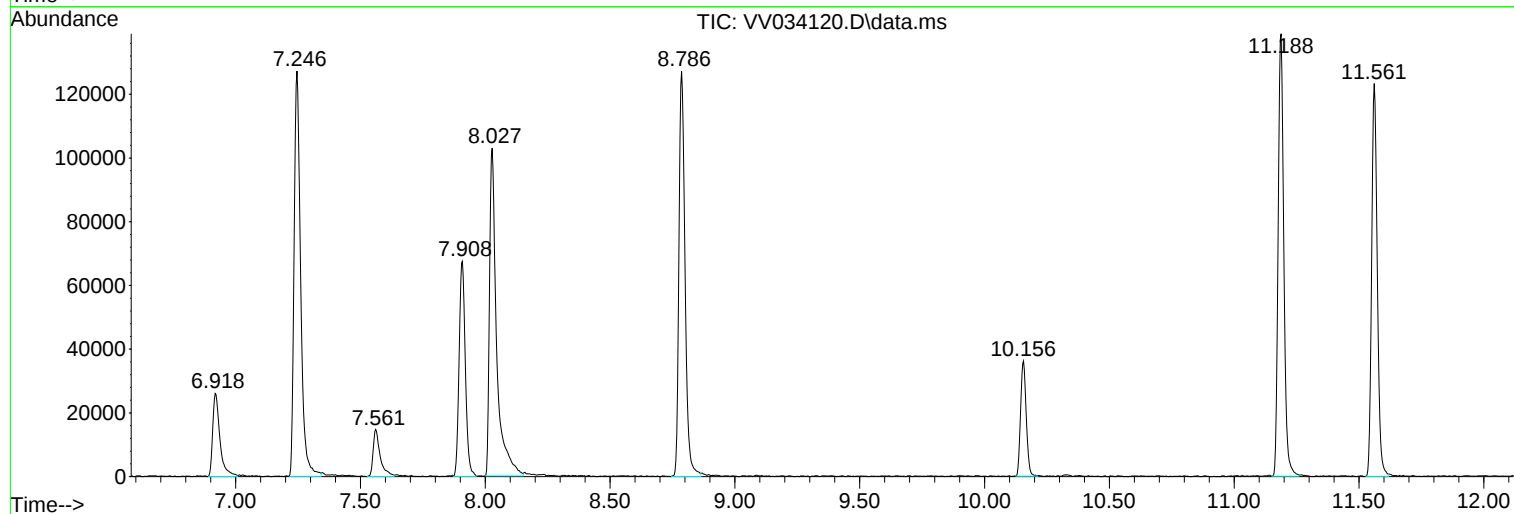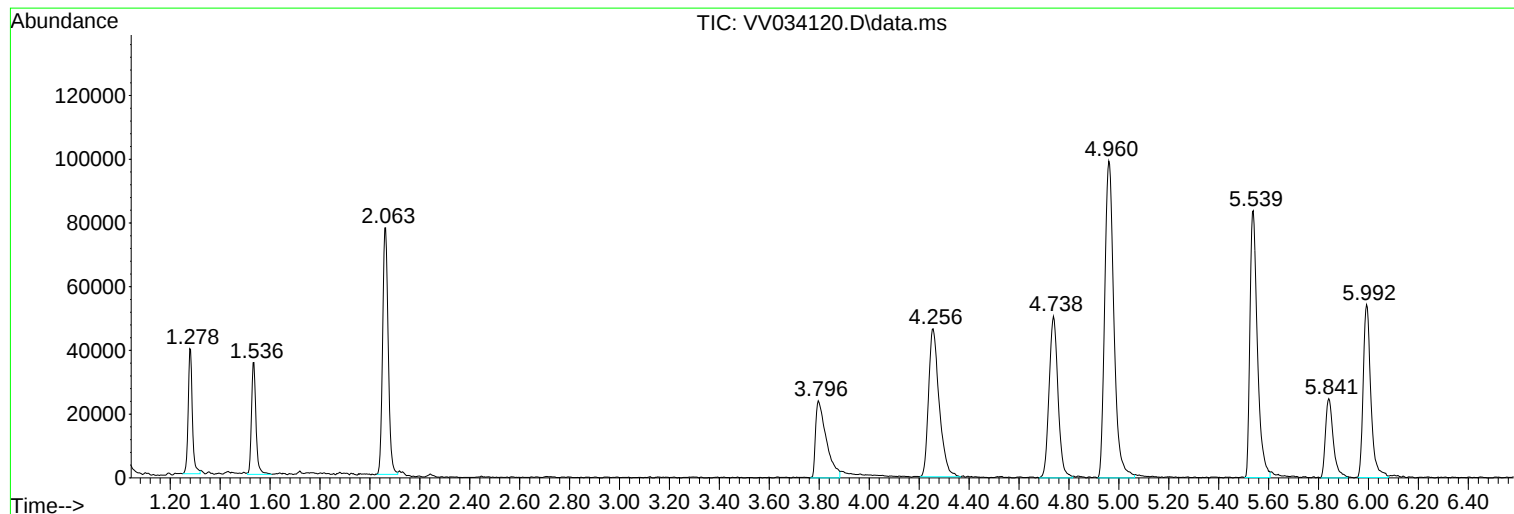

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034120.D
Acq On : 09 Feb 2024 18:28
Operator : SY/MD
Sample : P1402-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV020924\
Data File : VV034120.D
Acq On : 09 Feb 2024 18:28
Operator : SY/MD
Sample : P1402-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR012524WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc