

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014542.D
 Acq On : 10 Feb 2020 11:21
 Operator : SY/MD
 Sample : VV0210MBL03
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	83	rVB	138365	133862	10.99%	1.427%
2	1.586	146	154	169	rVB	85096	103459	8.50%	1.103%
3	2.000	279	283	285	rBV3	726	459	0.04%	0.005%
4	2.132	313	324	335	rBV	184589	265386	21.80%	2.830%
5	2.405	407	409	412	rBV	751	381	0.03%	0.004%
6	2.537	443	450	461	rBV6	2987	5042	0.41%	0.054%
7	2.579	461	463	469	rVB3	763	554	0.05%	0.006%
8	2.637	478	481	482	rBV2	956	539	0.04%	0.006%
9	2.724	506	508	512	rVB3	551	324	0.03%	0.003%
10	2.888	557	559	561	rVV3	506	240	0.02%	0.003%
11	2.907	563	565	567	rVV2	676	337	0.03%	0.004%
12	2.936	570	574	577	rVV2	331	308	0.03%	0.003%
13	3.158	641	643	646	rBV2	453	282	0.02%	0.003%
14	3.174	646	648	651	rBV	404	226	0.02%	0.002%
15	3.245	668	670	674	rVB	623	379	0.03%	0.004%
16	3.341	697	700	701	rBV2	358	223	0.02%	0.002%
17	3.380	710	712	715	rBV2	593	322	0.03%	0.003%
18	3.434	726	729	732	rBV3	387	328	0.03%	0.003%
19	3.450	732	734	738	rVB	647	418	0.03%	0.004%
20	3.495	743	748	752	rBV2	467	506	0.04%	0.005%
21	3.544	761	763	766	rVB2	388	211	0.02%	0.002%
22	3.762	828	831	834	rVB	633	404	0.03%	0.004%
23	3.788	834	839	842	rBV3	418	466	0.04%	0.005%
24	3.807	842	845	847	rBV3	524	310	0.03%	0.003%
25	3.862	860	862	866	rBV2	324	271	0.02%	0.003%
26	3.920	870	880	911	rBV	83638	221418	18.18%	2.361%
27	4.319	1000	1004	1006	rBV2	513	356	0.03%	0.004%
28	4.399	1012	1029	1056	rBV	193986	477594	39.22%	5.093%
29	4.618	1094	1097	1099	rBV2	511	267	0.02%	0.003%
30	4.666	1110	1112	1117	rVB	404	240	0.02%	0.003%
31	4.688	1117	1119	1122	rBV3	410	303	0.02%	0.003%
32	4.897	1181	1184	1187	rBV3	477	321	0.03%	0.003%
33	4.952	1199	1201	1205	rVB2	508	249	0.02%	0.003%
34	4.984	1208	1211	1214	rBV3	558	457	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014542.D
 Acq On : 10 Feb 2020 11:21
 Operator : SY/MD
 Sample : VV0210MBL03
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

35	5.093	1226	1245	1272	rBV3	478121	1217604	100.00%	12.983%
36	5.438	1349	1352	1355	rBV4	584	391	0.03%	0.004%
37	5.521	1376	1378	1381	rVB2	706	302	0.02%	0.003%
38	5.598	1400	1402	1404	rBV3	618	325	0.03%	0.003%
39	5.659	1407	1421	1442	rBV	401189	791192	64.98%	8.436%
40	5.859	1480	1483	1485	rBV3	551	350	0.03%	0.004%
41	5.920	1498	1502	1503	rBV2	342	212	0.02%	0.002%
42	5.991	1522	1524	1528	rBV2	479	239	0.02%	0.003%
43	6.061	1543	1546	1548	rBV2	500	351	0.03%	0.004%
44	6.113	1548	1562	1590	rBV	274480	550935	45.25%	5.875%
45	6.396	1648	1650	1652	rBV2	532	345	0.03%	0.004%
46	6.508	1683	1685	1690	rVB2	580	385	0.03%	0.004%
47	6.553	1695	1699	1701	rVB	423	273	0.02%	0.003%
48	6.708	1744	1747	1755	rVB5	596	563	0.05%	0.006%
49	7.026	1834	1846	1864	rBV	171088	304414	25.00%	3.246%
50	7.164	1887	1889	1892	rBV	467	251	0.02%	0.003%
51	7.280	1916	1925	1932	rBV8	1331	2453	0.20%	0.026%
52	7.357	1936	1949	1967	rBV	600168	1046075	85.91%	11.154%
53	7.659	2032	2043	2063	rBV	126817	213547	17.54%	2.277%
54	8.023	2152	2156	2159	rVB2	599	451	0.04%	0.005%
55	8.081	2172	2174	2177	rBV	434	246	0.02%	0.003%
56	8.129	2177	2189	2223	rBV	248213	534053	43.86%	5.695%
57	8.515	2305	2309	2310	rBV	430	294	0.02%	0.003%
58	8.553	2319	2321	2323	rBV2	381	231	0.02%	0.002%
59	8.724	2367	2374	2377	rBV2	371	392	0.03%	0.004%
60	8.798	2394	2397	2400	rVB2	500	344	0.03%	0.004%
61	8.823	2401	2405	2408	rBV4	550	393	0.03%	0.004%
62	8.891	2414	2426	2454	rBV	584292	957357	78.63%	10.208%
63	9.029	2467	2469	2472	rVB3	661	326	0.03%	0.003%
64	9.148	2502	2506	2507	rBV2	629	393	0.03%	0.004%
65	9.228	2526	2531	2535	rVB4	591	513	0.04%	0.005%
66	9.289	2548	2550	2555	rVV2	505	327	0.03%	0.003%
67	9.315	2555	2558	2560	rVB3	409	260	0.02%	0.003%
68	9.447	2597	2599	2602	rVV	438	223	0.02%	0.002%
69	9.482	2608	2610	2614	rVB2	381	217	0.02%	0.002%
70	9.508	2614	2618	2619	rBV	371	276	0.02%	0.003%
71	9.582	2638	2641	2642	rBV3	546	334	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV021020\
 Data File : VV014542.D
 Acq On : 10 Feb 2020 11:21
 Operator : SY/MD
 Sample : VV0210MBL03
 Misc : 5.0µL/5.0mL/100µL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

72	9.736	2685	2689	2691	rBV2	649	339	0.03%	0.004%
73	9.781	2701	2703	2705	rBV	557	256	0.02%	0.003%
74	10.013	2772	2775	2780	rVB2	308	220	0.02%	0.002%
75	10.061	2786	2790	2794	rVB2	571	422	0.03%	0.004%
76	10.254	2837	2850	2872	rBV	362085	572902	47.05%	6.109%
77	10.424	2902	2903	2906	rBV3	504	295	0.02%	0.003%
78	10.450	2909	2911	2917	rVB3	463	343	0.03%	0.004%
79	10.524	2931	2934	2936	rBV2	414	285	0.02%	0.003%
80	10.585	2947	2953	2957	rBV6	1169	1309	0.11%	0.014%
81	10.640	2967	2970	2971	rBV	352	214	0.02%	0.002%
82	10.672	2978	2980	2982	rBV	413	244	0.02%	0.003%
83	10.839	3028	3032	3035	rBV2	569	393	0.03%	0.004%
84	10.891	3045	3048	3052	rBV3	615	520	0.04%	0.006%
85	11.289	3159	3172	3193	rBV	630885	988246	81.16%	10.538%
86	11.489	3231	3234	3236	rBV	532	329	0.03%	0.004%
87	11.563	3251	3257	3260	rBV3	467	436	0.04%	0.005%
88	11.666	3276	3289	3308	rBV	598804	961797	78.99%	10.256%
89	11.830	3337	3340	3344	rBV	560	399	0.03%	0.004%
90	12.106	3423	3426	3429	rVB2	512	382	0.03%	0.004%
91	12.125	3429	3432	3436	rBV2	306	282	0.02%	0.003%
92	12.534	3557	3559	3562	rBV2	488	265	0.02%	0.003%
93	12.582	3572	3574	3578	rBV2	392	259	0.02%	0.003%
94	12.662	3595	3599	3602	rBV	353	281	0.02%	0.003%
95	12.694	3605	3609	3612	rVV3	1052	994	0.08%	0.011%
96	12.723	3615	3618	3626	rBV2	626	652	0.05%	0.007%
97	12.794	3638	3640	3647	rVB4	456	430	0.04%	0.005%
98	12.862	3658	3661	3664	rVV2	749	398	0.03%	0.004%
99	12.907	3672	3675	3680	rVB2	651	484	0.04%	0.005%
100	13.791	3947	3950	3957	rVB3	1652	1565	0.13%	0.017%


Sum of corrected areas: 9378220

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV021020\
Data File : VV014542.D
Acq On : 10 Feb 2020 11:21
Operator : SY/MD
Sample : VV0210MBL03
Misc : 5.0µ/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

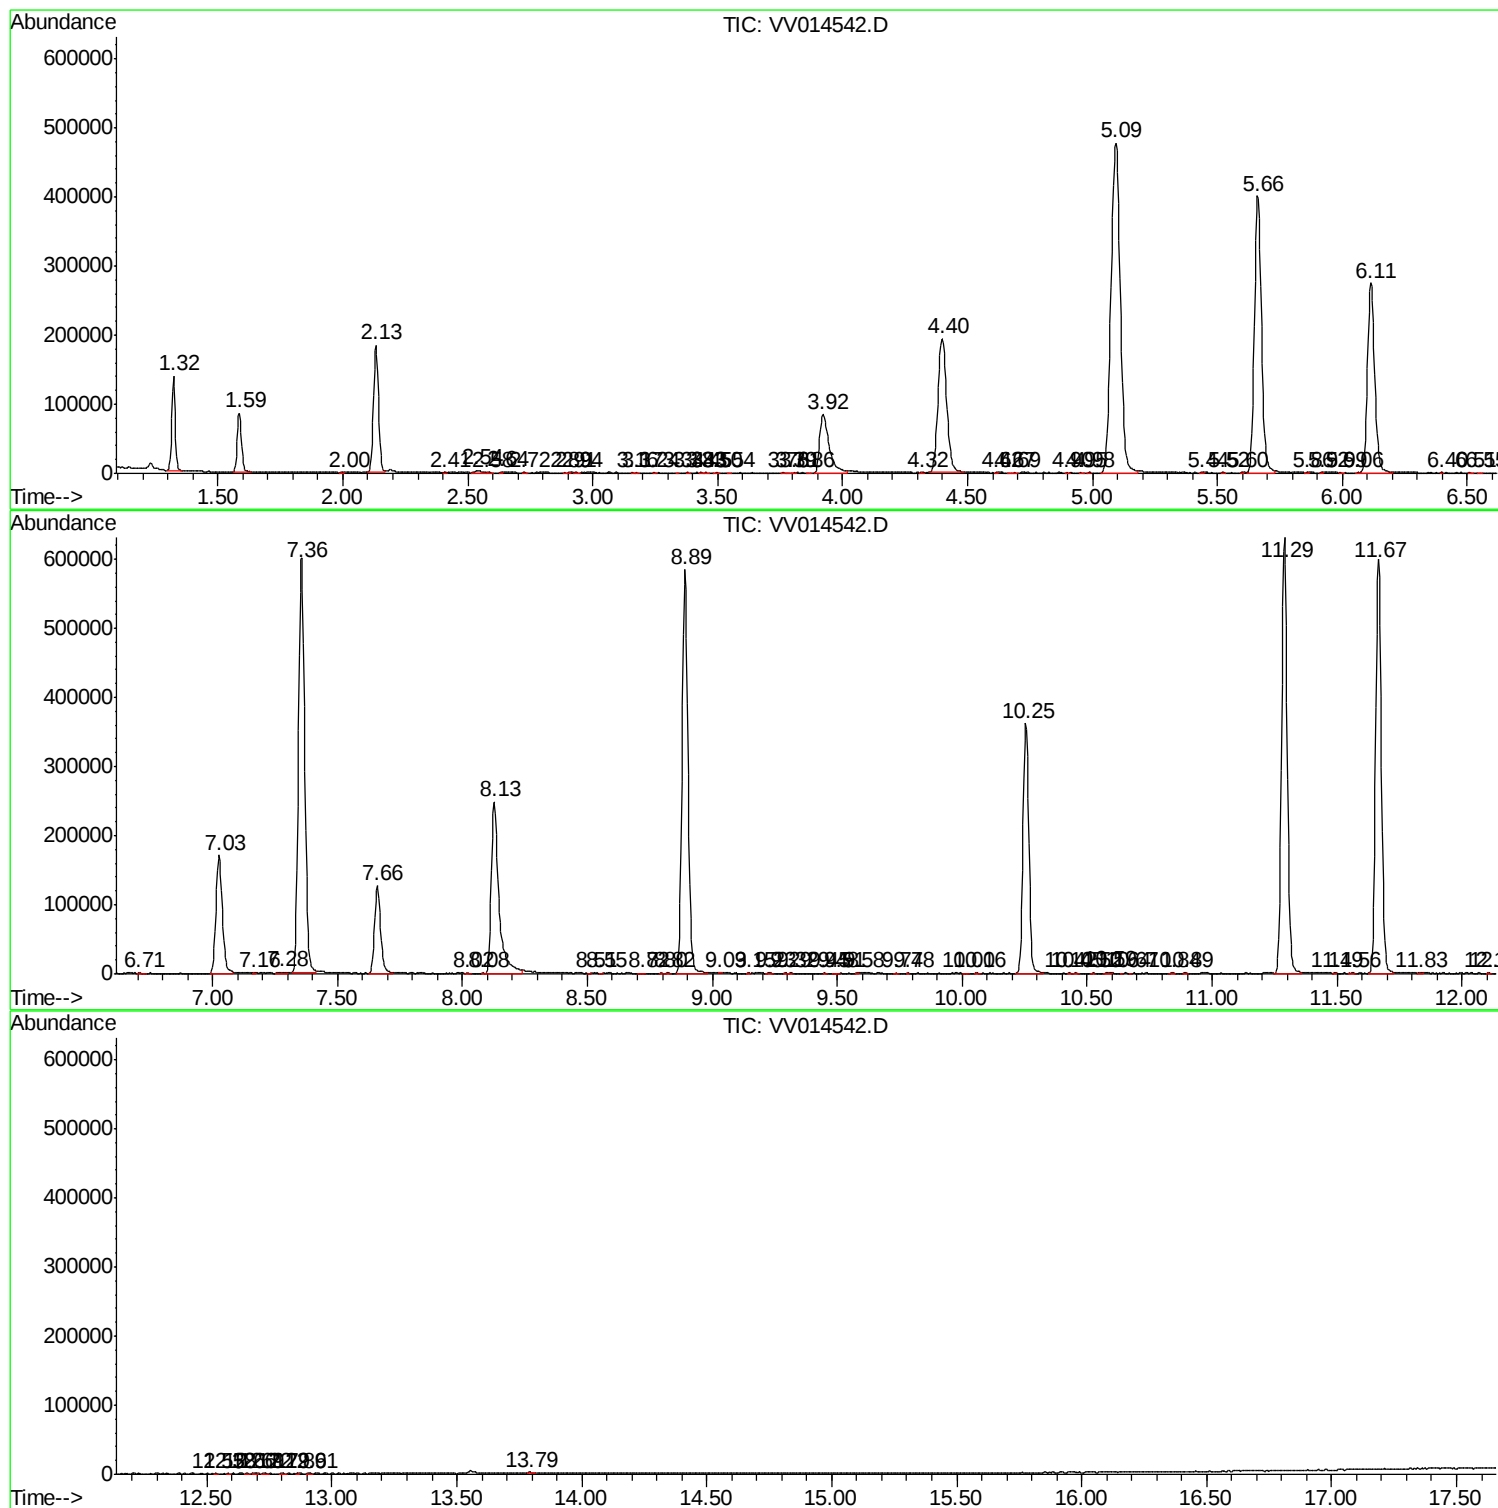

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV021020\
Data File : VV014542.D
Acq On : 10 Feb 2020 11:21
Operator : SY/MD
Sample : VV0210MBL03
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV021020\
Data File : VV014542.D
Acq On : 10 Feb 2020 11:21
Operator : SY/MD
Sample : VV0210MBL03
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc