

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014545.D
 Acq On : 10 Feb 2020 12:35
 Operator : SY/MD
 Sample : VV0210WBL06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	80	rVB	122321	120044	10.16%	1.332%
2	1.586	146	154	169	rVB	80372	96082	8.13%	1.066%
3	2.036	292	294	299	rBV4	856	606	0.05%	0.007%
4	2.132	313	324	336	rBV	174907	253175	21.43%	2.809%
5	2.541	443	451	459	rBV6	2533	4287	0.36%	0.048%
6	2.795	528	530	533	rVB3	672	306	0.03%	0.003%
7	2.859	544	550	552	rBV3	441	482	0.04%	0.005%
8	2.917	564	568	570	rBV	558	313	0.03%	0.003%
9	3.142	635	638	640	rBV	470	255	0.02%	0.003%
10	3.184	647	651	652	rBV2	396	260	0.02%	0.003%
11	3.348	699	702	704	rBV2	468	252	0.02%	0.003%
12	3.389	712	715	718	rBV3	465	338	0.03%	0.004%
13	3.450	731	734	738	rVB2	416	309	0.03%	0.003%
14	3.505	749	751	754	rVV3	429	224	0.02%	0.002%
15	3.563	766	769	772	rBV2	451	325	0.03%	0.004%
16	3.576	772	773	777	rVB2	642	288	0.02%	0.003%
17	3.637	787	792	794	rBV2	442	371	0.03%	0.004%
18	3.711	809	815	818	rVB3	490	473	0.04%	0.005%
19	3.769	830	833	837	rVB3	487	364	0.03%	0.004%
20	3.795	837	841	843	rBV	413	264	0.02%	0.003%
21	3.852	854	859	860	rBV2	276	229	0.02%	0.003%
22	3.920	869	880	910	rBV	86028	231021	19.55%	2.563%
23	4.129	942	945	951	rBV6	655	662	0.06%	0.007%
24	4.322	1002	1005	1008	rBV3	484	321	0.03%	0.004%
25	4.399	1011	1029	1053	rBV	190339	465115	39.36%	5.160%
26	4.634	1097	1102	1104	rBV4	573	461	0.04%	0.005%
27	4.711	1123	1126	1129	rBV2	593	383	0.03%	0.004%
28	4.814	1153	1158	1161	rBV4	420	425	0.04%	0.005%
29	4.865	1172	1174	1178	rVB	516	294	0.02%	0.003%
30	4.997	1210	1215	1217	rBV2	291	267	0.02%	0.003%
31	5.094	1224	1245	1272	rBV2	463292	1181676	100.00%	13.109%
32	5.447	1352	1355	1360	rBV4	684	599	0.05%	0.007%
33	5.585	1396	1398	1401	rBV2	488	336	0.03%	0.004%
34	5.659	1408	1421	1445	rBV	379120	743047	62.88%	8.243%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014545.D
 Acq On : 10 Feb 2020 12:35
 Operator : SY/MD
 Sample : VV0210WBL06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

35	5.817	1469	1470	1474	rVB3	683	411	0.03%	0.005%
36	5.936	1504	1507	1508	rBV	845	414	0.04%	0.005%
37	6.000	1525	1527	1531	rVB3	719	442	0.04%	0.005%
38	6.026	1531	1535	1537	rBV2	399	290	0.02%	0.003%
39	6.113	1546	1562	1587	rBV	264399	534559	45.24%	5.930%
40	6.425	1655	1659	1663	rVB4	555	457	0.04%	0.005%
41	6.486	1676	1678	1682	rVB3	781	431	0.04%	0.005%
42	6.521	1685	1689	1694	rVB2	419	358	0.03%	0.004%
43	6.547	1694	1697	1701	rVB2	475	375	0.03%	0.004%
44	6.579	1701	1707	1711	rBV2	436	397	0.03%	0.004%
45	6.666	1728	1734	1737	rBV3	771	654	0.06%	0.007%
46	6.688	1737	1741	1743	rVB2	971	565	0.05%	0.006%
47	6.708	1743	1747	1749	rBV3	732	429	0.04%	0.005%
48	6.833	1779	1786	1787	rVV2	296	246	0.02%	0.003%
49	6.968	1827	1828	1832	rVB2	531	240	0.02%	0.003%
50	7.026	1832	1846	1868	rBV	166953	299450	25.34%	3.322%
51	7.270	1920	1922	1923	rBV	665	247	0.02%	0.003%
52	7.357	1934	1949	1967	rBV	579445	1012910	85.72%	11.237%
53	7.601	2022	2025	2026	rBV	656	314	0.03%	0.003%
54	7.659	2032	2043	2064	rBV	121800	204975	17.35%	2.274%
55	7.801	2085	2087	2089	rVB	634	272	0.02%	0.003%
56	7.820	2089	2093	2096	rVB3	605	427	0.04%	0.005%
57	7.942	2129	2131	2135	rBV2	360	269	0.02%	0.003%
58	7.958	2135	2136	2139	rVB	590	231	0.02%	0.003%
59	8.126	2176	2188	2222	rBV	253751	541583	45.83%	6.008%
60	8.466	2289	2294	2296	rBV4	618	366	0.03%	0.004%
61	8.499	2300	2304	2307	rBV3	523	480	0.04%	0.005%
62	8.585	2327	2331	2335	rBV3	520	503	0.04%	0.006%
63	8.698	2362	2366	2367	rBV2	507	364	0.03%	0.004%
64	8.785	2390	2393	2396	rVB3	563	309	0.03%	0.003%
65	8.891	2413	2426	2450	rBV	556964	897585	75.96%	9.957%
66	9.055	2473	2477	2479	rBV4	890	644	0.05%	0.007%
67	9.161	2508	2510	2515	rBV2	322	247	0.02%	0.003%
68	9.183	2515	2517	2521	rVV3	652	429	0.04%	0.005%
69	9.254	2537	2539	2543	rVB2	547	283	0.02%	0.003%
70	9.286	2546	2549	2552	rBV	362	241	0.02%	0.003%
71	9.579	2637	2640	2642	rVV	354	240	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014545.D
 Acq On : 10 Feb 2020 12:35
 Operator : SY/MD
 Sample : VV0210WBL06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK210

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

72	9.608	2647	2649	2652	rVV3	773	500	0.04%	0.006%
73	9.637	2656	2658	2660	rVV2	565	305	0.03%	0.003%
74	9.650	2660	2662	2665	rVB	521	243	0.02%	0.003%
75	9.666	2665	2667	2672	rVB	426	282	0.02%	0.003%
76	9.695	2672	2676	2680	rBV2	398	302	0.03%	0.003%
77	9.730	2682	2687	2690	rBV4	470	439	0.04%	0.005%
78	10.080	2794	2796	2799	rBV2	569	282	0.02%	0.003%
79	10.154	2817	2819	2823	rBV2	292	243	0.02%	0.003%
80	10.254	2837	2850	2871	rBV	359109	568222	48.09%	6.304%
81	10.675	2978	2981	2984	rBV2	511	359	0.03%	0.004%
82	10.695	2985	2987	2991	rVB3	469	238	0.02%	0.003%
83	10.785	3011	3015	3017	rBV3	774	401	0.03%	0.004%
84	10.842	3030	3033	3036	rBV	630	402	0.03%	0.004%
85	11.055	3096	3099	3103	rVB2	453	303	0.03%	0.003%
86	11.148	3126	3128	3131	rBV2	379	257	0.02%	0.003%
87	11.225	3149	3152	3154	rBV3	558	337	0.03%	0.004%
88	11.289	3160	3172	3191	rBV	585837	915341	77.46%	10.154%
89	11.666	3277	3289	3309	rBV	567052	914994	77.43%	10.150%
90	11.897	3358	3361	3362	rBV2	526	257	0.02%	0.003%
91	11.936	3370	3373	3378	rBV3	485	338	0.03%	0.004%
92	11.974	3381	3385	3388	rVB2	539	467	0.04%	0.005%
93	12.003	3392	3394	3401	rVB3	692	504	0.04%	0.006%
94	12.196	3452	3454	3458	rBV4	334	263	0.02%	0.003%
95	12.460	3534	3536	3542	rVV2	415	275	0.02%	0.003%
96	12.524	3553	3556	3557	rBV3	418	243	0.02%	0.003%
97	12.643	3590	3593	3597	rBV	487	362	0.03%	0.004%
98	12.691	3604	3608	3613	rBV3	659	782	0.07%	0.009%
99	12.768	3628	3632	3636	rBV3	544	582	0.05%	0.006%
100	13.283	3790	3792	3796	rBV3	575	306	0.03%	0.003%


Sum of corrected areas: 9014320

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV021020\
Data File : VV014545.D
Acq On : 10 Feb 2020 12:35
Operator : SY/MD
Sample : VV0210WBL06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

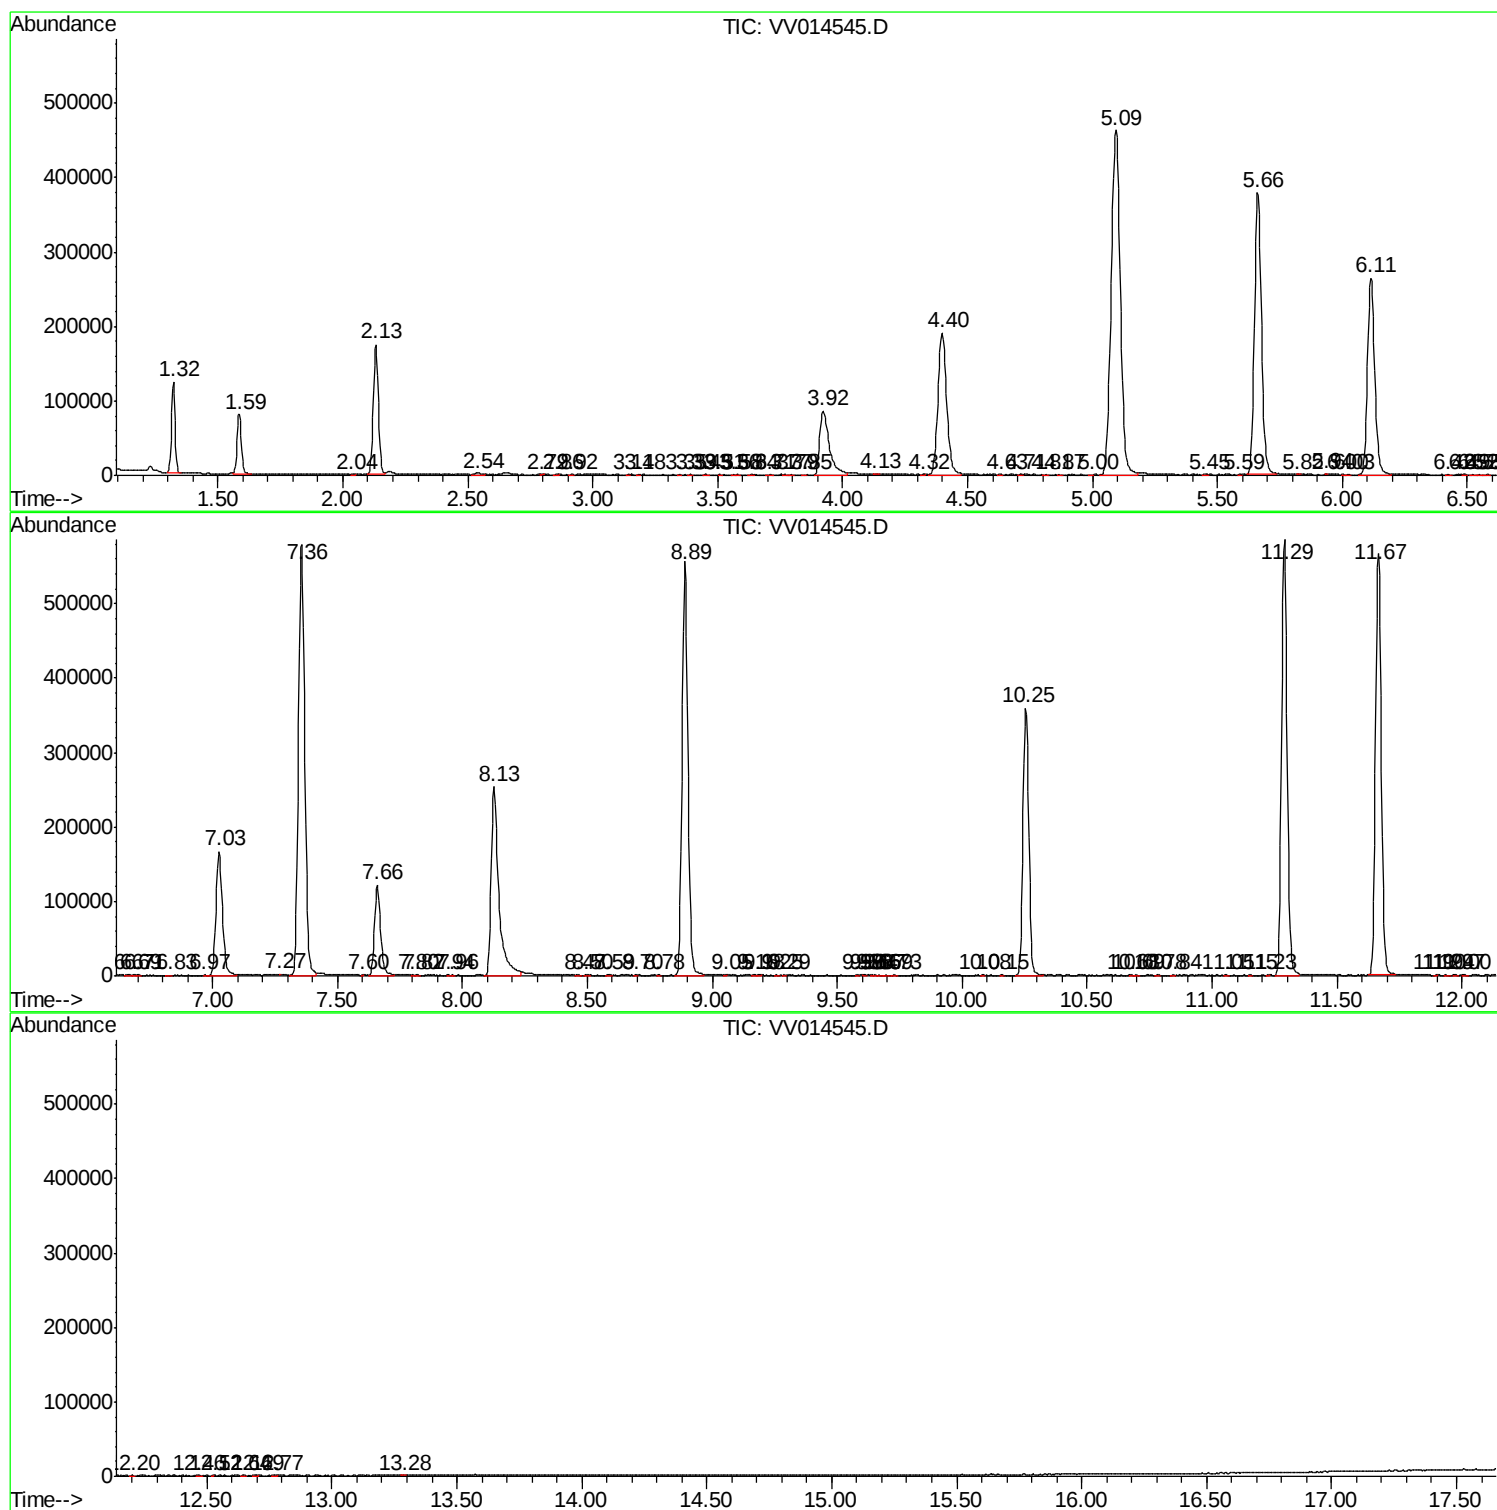

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV021020\
Data File : VV014545.D
Acq On : 10 Feb 2020 12:35
Operator : SY/MD
Sample : VV0210WBL06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV021020\
Data File : VV014545.D
Acq On : 10 Feb 2020 12:35
Operator : SY/MD
Sample : VV0210WBL06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK210

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc