

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014546.D
 Acq On : 10 Feb 2020 12:58
 Operator : SY/MD
 Sample : VV0210WBL07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.322	65	72	85	rVB	131360	127367	10.75%	1.394%
2	1.582	146	153	165	rVB	82493	98180	8.28%	1.074%
3	1.971	272	274	278	rVB2	567	353	0.03%	0.004%
4	1.994	278	281	282	rBV3	610	311	0.03%	0.003%
5	2.032	290	293	294	rBV2	493	276	0.02%	0.003%
6	2.077	304	307	311	rBV3	710	507	0.04%	0.006%
7	2.129	312	323	335	rBV	178505	255494	21.56%	2.796%
8	2.457	422	425	427	rBV3	457	309	0.03%	0.003%
9	2.762	518	520	524	rVB2	487	324	0.03%	0.004%
10	2.862	548	551	556	rBV4	469	494	0.04%	0.005%
11	2.949	573	578	579	rBV3	638	492	0.04%	0.005%
12	3.064	610	614	615	rVV3	426	264	0.02%	0.003%
13	3.090	619	622	625	rBV	781	511	0.04%	0.006%
14	3.193	651	654	658	rBV	349	264	0.02%	0.003%
15	3.219	660	662	668	rVB3	549	376	0.03%	0.004%
16	3.318	691	693	696	rBV2	473	351	0.03%	0.004%
17	3.457	733	736	740	rBV2	621	401	0.03%	0.004%
18	3.486	740	745	748	rBV4	678	517	0.04%	0.006%
19	3.595	777	779	786	rVV2	676	572	0.05%	0.006%
20	3.717	812	817	821	rVB3	531	421	0.04%	0.005%
21	3.769	831	833	837	rVB3	482	242	0.02%	0.003%
22	3.839	853	855	858	rVB2	590	242	0.02%	0.003%
23	3.920	870	880	907	rBV	85761	223235	18.84%	2.443%
24	4.399	1012	1029	1057	rBV	191482	472593	39.88%	5.172%
25	4.617	1094	1097	1100	rVB2	581	362	0.03%	0.004%
26	4.634	1100	1102	1104	rBV	729	354	0.03%	0.004%
27	4.695	1118	1121	1126	rBV4	666	594	0.05%	0.007%
28	4.778	1142	1147	1148	rBV2	622	461	0.04%	0.005%
29	4.878	1173	1178	1180	rBV3	584	411	0.03%	0.004%
30	5.093	1227	1245	1276	rBV2	462182	1185137	100.00%	12.970%
31	5.428	1344	1349	1352	rBV3	621	655	0.06%	0.007%
32	5.563	1387	1391	1394	rBV2	390	259	0.02%	0.003%
33	5.579	1394	1396	1400	rBV2	458	321	0.03%	0.004%
34	5.659	1407	1421	1445	rBV	391256	773448	65.26%	8.465%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014546.D
 Acq On : 10 Feb 2020 12:58
 Operator : SY/MD
 Sample : VV0210WBL07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

35	5.839	1474	1477	1482	rBV4	723	690	0.06%	0.008%
36	5.862	1482	1484	1488	rVB3	617	365	0.03%	0.004%
37	5.945	1504	1510	1511	rBV3	1879	1630	0.14%	0.018%
38	6.019	1530	1533	1534	rBV	582	320	0.03%	0.004%
39	6.058	1542	1545	1549	rBV	449	386	0.03%	0.004%
40	6.113	1549	1562	1581	rBV	266053	534387	45.09%	5.848%
41	6.283	1613	1615	1619	rVB2	648	326	0.03%	0.004%
42	6.396	1645	1650	1651	rBV2	471	327	0.03%	0.004%
43	6.437	1660	1663	1666	rVB2	594	393	0.03%	0.004%
44	6.460	1666	1670	1671	rBV	433	254	0.02%	0.003%
45	6.495	1677	1681	1683	rBV2	338	248	0.02%	0.003%
46	6.588	1707	1710	1713	rBV2	379	242	0.02%	0.003%
47	6.656	1729	1731	1734	rBV3	687	491	0.04%	0.005%
48	6.961	1823	1826	1830	rVB2	558	356	0.03%	0.004%
49	7.026	1834	1846	1868	rBV	165440	296163	24.99%	3.241%
50	7.260	1917	1919	1921	rBV	456	253	0.02%	0.003%
51	7.270	1921	1922	1924	rBV2	630	269	0.02%	0.003%
52	7.357	1935	1949	1968	rBV	583721	1018799	85.96%	11.150%
53	7.553	2008	2010	2012	rBV2	441	258	0.02%	0.003%
54	7.659	2031	2043	2067	rBV	121454	206336	17.41%	2.258%
55	7.920	2120	2124	2127	rBV2	444	347	0.03%	0.004%
56	7.968	2132	2139	2141	rBV3	411	346	0.03%	0.004%
57	8.125	2177	2188	2222	rBV	254531	543205	45.83%	5.945%
58	8.469	2293	2295	2299	rBV2	713	451	0.04%	0.005%
59	8.543	2316	2318	2322	rVB2	556	342	0.03%	0.004%
60	8.810	2395	2401	2403	rBV2	491	368	0.03%	0.004%
61	8.891	2414	2426	2449	rBV	566112	927026	78.22%	10.145%
62	9.045	2472	2474	2478	rVB3	531	337	0.03%	0.004%
63	9.370	2571	2575	2578	rBV4	617	446	0.04%	0.005%
64	9.453	2597	2601	2605	rBV3	386	332	0.03%	0.004%
65	9.556	2631	2633	2636	rVB2	418	244	0.02%	0.003%
66	9.579	2636	2640	2641	rBV2	491	306	0.03%	0.003%
67	9.592	2641	2644	2647	rBV4	699	447	0.04%	0.005%
68	9.633	2655	2657	2661	rVB2	541	345	0.03%	0.004%
69	9.710	2675	2681	2683	rBV4	572	373	0.03%	0.004%
70	9.807	2707	2711	2715	rBV4	382	425	0.04%	0.005%
71	9.894	2734	2738	2740	rBV4	477	287	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV021020\
 Data File : VV014546.D
 Acq On : 10 Feb 2020 12:58
 Operator : SY/MD
 Sample : VV0210WBL07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK211

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis

72	9.961	2756	2759	2763	rBV3	693	405	0.03%	0.004%
73	9.981	2763	2765	2769	rVB3	491	341	0.03%	0.004%
74	10.170	2821	2824	2828	rBV2	601	379	0.03%	0.004%
75	10.254	2838	2850	2866	rBV	360216	568057	47.93%	6.217%
76	10.341	2874	2877	2881	rBV3	557	422	0.04%	0.005%
77	10.386	2887	2891	2895	rVB3	565	481	0.04%	0.005%
78	10.408	2895	2898	2901	rBV	574	354	0.03%	0.004%
79	10.428	2901	2904	2908	rVB	607	401	0.03%	0.004%
80	10.447	2908	2910	2912	rBV	585	293	0.02%	0.003%
81	10.495	2923	2925	2929	rBV	394	248	0.02%	0.003%
82	10.550	2937	2942	2944	rBV2	424	386	0.03%	0.004%
83	10.572	2947	2949	2952	rBV2	625	447	0.04%	0.005%
84	10.592	2952	2955	2960	rVB3	568	397	0.03%	0.004%
85	10.691	2982	2986	2989	rBV2	375	340	0.03%	0.004%
86	10.849	3031	3035	3038	rBV2	430	291	0.02%	0.003%
87	10.891	3044	3048	3050	rBV3	623	367	0.03%	0.004%
88	11.016	3084	3087	3091	rBV	437	386	0.03%	0.004%
89	11.218	3146	3150	3156	rVB5	642	640	0.05%	0.007%
90	11.289	3160	3172	3194	rBV	606560	947672	79.96%	10.371%
91	11.543	3249	3251	3255	rBV2	515	249	0.02%	0.003%
92	11.665	3276	3289	3310	rBV	581565	927468	78.26%	10.150%
93	11.845	3343	3345	3348	rVB2	590	309	0.03%	0.003%
94	12.103	3423	3425	3429	rBV2	422	269	0.02%	0.003%
95	12.302	3484	3487	3493	rVV4	513	475	0.04%	0.005%
96	12.357	3500	3504	3506	rBV3	368	304	0.03%	0.003%
97	12.405	3517	3519	3522	rBV3	445	263	0.02%	0.003%
98	12.646	3589	3594	3597	rBV2	365	415	0.04%	0.005%
99	12.961	3689	3692	3696	rBV2	336	265	0.02%	0.003%
100	15.450	4464	4466	4470	rBV	918	771	0.07%	0.008%




Sum of corrected areas: 9137313

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV021020\
Data File : VV014546.D
Acq On : 10 Feb 2020 12:58
Operator : SY/MD
Sample : VV0210WBL07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

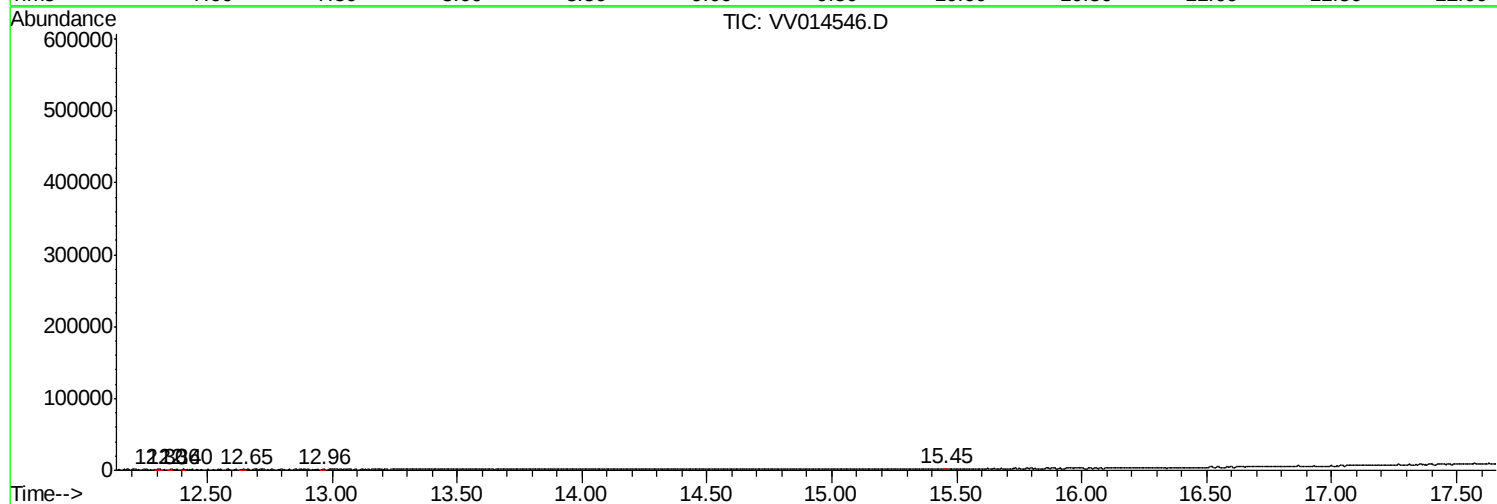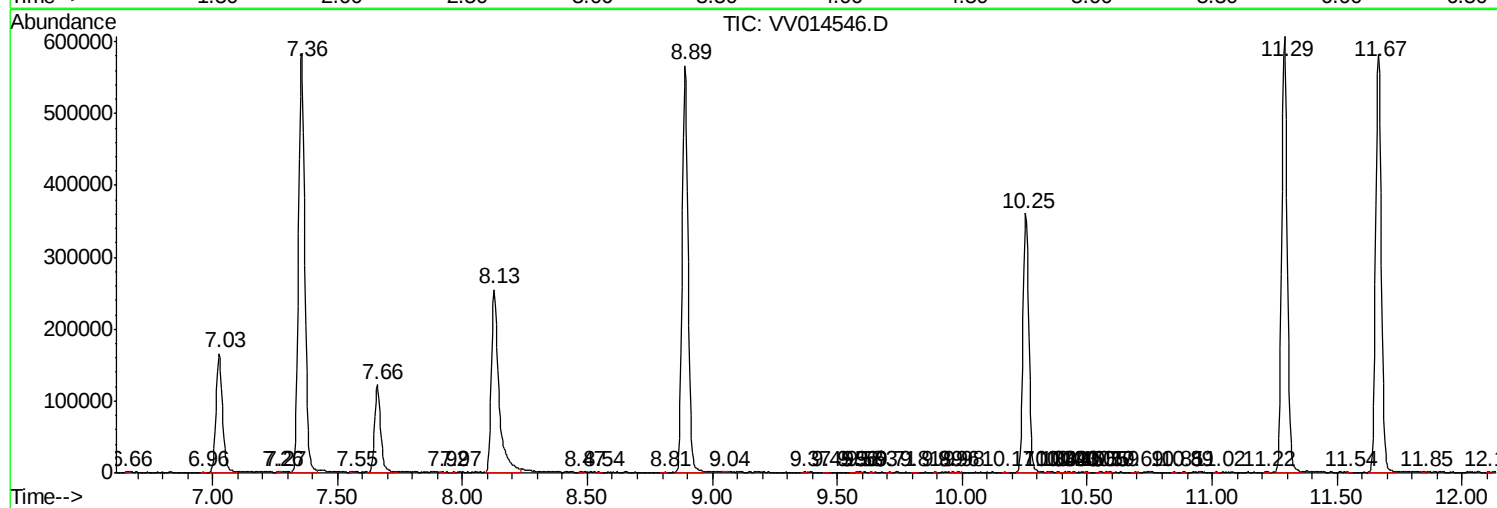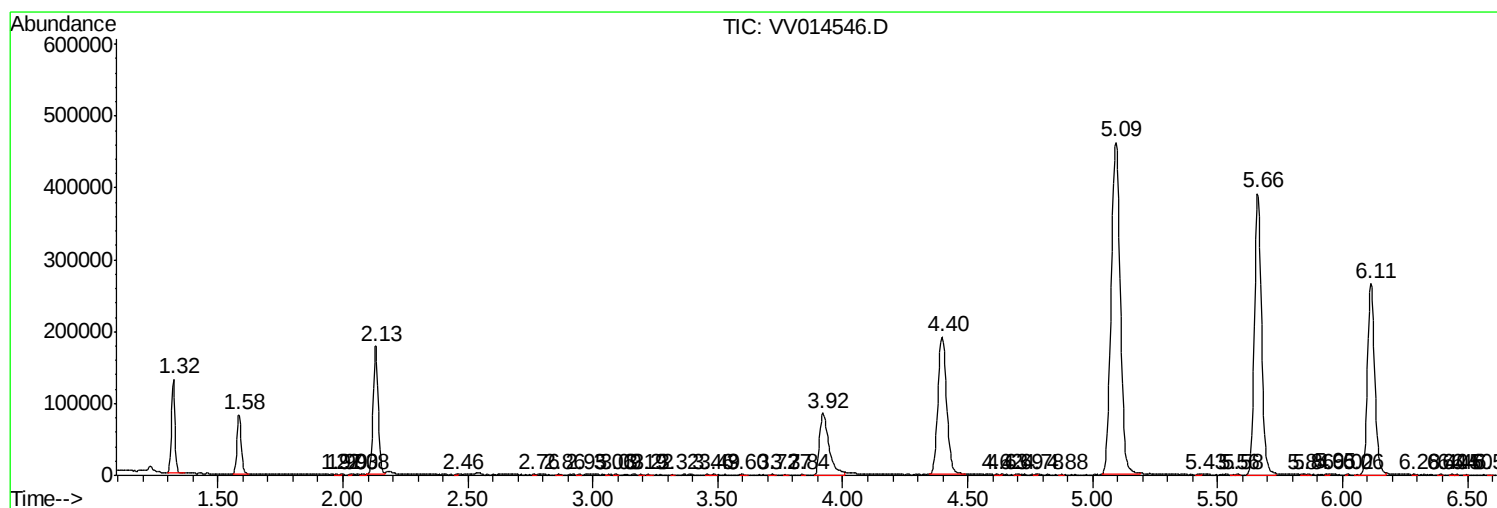

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV021020\
Data File : VV014546.D
Acq On : 10 Feb 2020 12:58
Operator : SY/MD
Sample : VV0210WBL07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV021020\
Data File : VV014546.D
Acq On : 10 Feb 2020 12:58
Operator : SY/MD
Sample : VV0210WBL07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK211

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc