


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV021020\
 Data File : VV014540.D
 Acq On : 10 Feb 2020 09:55
 Operator : SY/MD
 Sample : BFB90
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB203

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM020620W.M
 Title : VOC Analysis
 Last Update : Tue Feb 11 04:43:03 2020

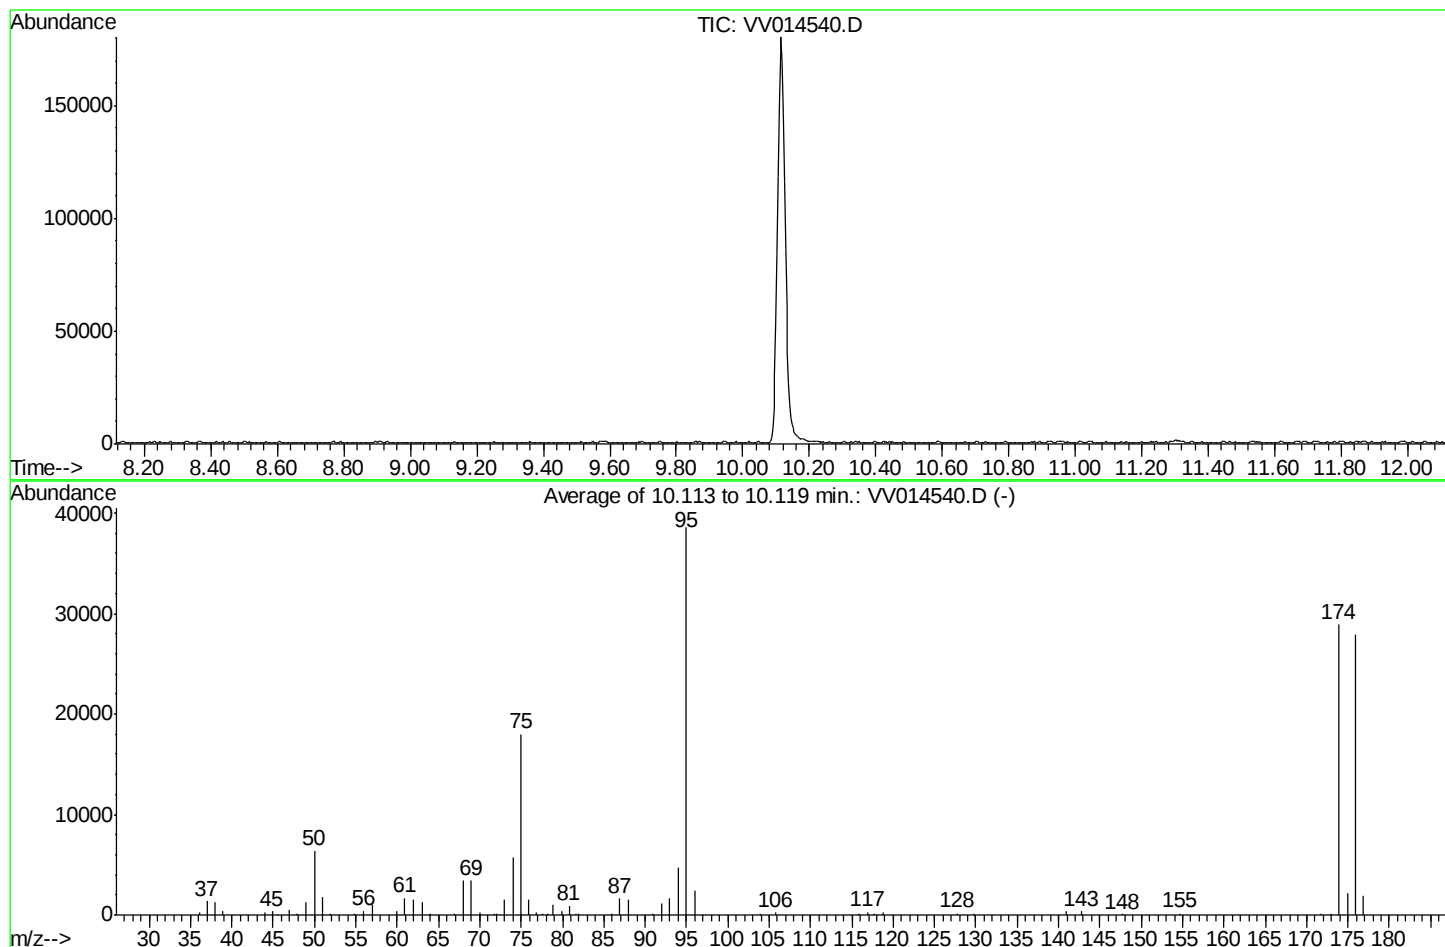

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	6372	PASS
75	95	30	80	46.6	17997	PASS
95	95	100	100	100.0	38584	PASS
96	95	5	9	6.2	2401	PASS
173	174	0.00	2	0.6	173	PASS
174	95	50	120	74.9	28898	PASS
175	174	5	9	7.5	2175	PASS
176	174	95	101	96.7	27949	PASS
177	176	5	9	7.0	1945	PASS

m/z	Abundance
36.10	271.0
37.00	1377.0
38.00	1268.0
39.00	483.0
40.00	227.0
44.00	557.0
44.90	291.0
45.60	121.0
47.00	514.0
47.90	202.0
48.90	1270.0
50.00	6439.0
51.00	1881.0
51.90	148.0
54.80	157.0
55.90	444.0
57.00	1016.0
59.90	365.0
60.90	1677.0
62.00	1696.0
63.00	1133.0
64.00	134.0
66.90	164.0
68.00	3481.0
69.00	3356.0
70.00	289.0
71.70	212.0
72.90	1551.0
74.00	5745.0
75.00	18376.0
76.00	1567.0
76.90	308.0
77.70	191.0
78.10	189.0
78.80	1001.0
80.00	259.0
80.90	946.0
81.90	216.0
86.00	129.0
86.90	1633.0
87.90	1497.0
91.00	151.0
92.00	1169.0
93.00	1608.0
94.00	4533.0
95.00	38600.0
96.00	2567.0
103.90	192.0
105.80	202.0
115.80	148.0
117.00	275.0
117.80	166.0
118.80	205.0
127.80	172.0
129.80	133.0
140.90	400.0
142.80	380.0
147.80	104.0
154.80	170.0
173.00	519.0
173.90	28368.0
174.90	2251.0
175.90	26760.0
176.90	1874.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	302.0
37.00	1426.0
38.00	1291.0
38.90	439.0
40.00	255.0
44.00	577.0
44.90	357.0
47.00	492.0
47.90	189.0
48.90	1304.0
50.00	6570.0
51.00	1906.0
51.90	135.0
54.80	134.0
55.90	455.0
57.00	1005.0
59.90	358.0
60.90	1754.0
62.00	1671.0
63.00	1272.0
63.90	168.0
66.90	181.0
68.00	3447.0
69.00	3531.0
70.10	252.0
71.90	191.0
73.00	1585.0
74.00	5861.0
75.00	18584.0
75.90	1640.0
76.90	337.0
77.70	185.0
78.20	176.0
78.80	1041.0
79.90	236.0
80.00	234.0
80.80	957.0
81.60	197.0
81.90	197.0
85.90	148.0
86.90	1688.0
88.00	1603.0
90.90	140.0
92.00	1189.0
93.00	1703.0
94.00	4921.0
95.00	39888.0
96.00	2435.0
97.00	109.0
103.90	188.0
105.80	209.0
115.80	130.0
117.00	285.0
117.80	175.0
118.80	262.0
127.80	182.0
129.80	147.0
140.90	381.0
142.80	396.0
147.80	114.0
154.70	176.0
171.80	108.0
173.90	29856.0
175.00	2207.0
175.90	28936.0
176.90	2017.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

m/z	Abundance
36.00	318.0
37.00	1394.0
38.00	1269.0
38.90	413.0
39.90	288.0
44.00	550.0
44.90	326.0
47.00	418.0
47.80	187.0
48.90	1255.0
50.00	6108.0
51.00	1670.0
51.80	127.0
56.00	415.0
57.00	879.0
59.90	333.0
60.90	1693.0
62.00	1423.0
63.00	1249.0
63.90	176.0
66.90	162.0
68.00	3236.0
69.00	3317.0
70.00	194.0
72.00	184.0
73.00	1381.0
74.00	5630.0
75.00	17032.0
76.00	1578.0
76.90	320.0
77.60	169.0
78.20	151.0
78.80	967.0
79.80	244.0
80.80	948.0
81.70	188.0
85.90	148.0
87.00	1562.0
88.00	1487.0
90.90	133.0
92.00	1077.0
93.00	1641.0
94.00	4634.0
95.00	37264.0
96.00	2202.0
103.90	168.0
105.80	204.0
115.90	118.0
116.90	245.0
117.70	156.0
118.70	273.0
127.80	177.0
129.80	133.0
140.90	336.0
142.90	364.0
147.60	104.0
154.80	131.0
171.80	134.0
173.90	28472.0
175.00	2068.0
175.90	28152.0
176.90	1944.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203

Scan 2795 (10.077 min): VV014540.D
BFB90

m/z	Abundance
35.80	108.0
39.80	260.0
44.00	330.0

Instrument :
MSVOA_V
ClientSampleId :
BFB203