

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021021\
 Data File : VV020289.D
 Acq On : 10 Feb 2021 15:34
 Operator : SY/MD
 Sample : M1377-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M

Title : VOC Analysis

Signal : TIC: VV020289.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	98	rVB	297673	305025	14.33%	1.728%
2	1.571	158	165	178	rVB	246536	278888	13.10%	1.580%
3	2.108	322	332	371	rVB	523930	822001	38.62%	4.658%
4	2.941	586	591	594	rBV2	421	393	0.02%	0.002%
5	3.047	622	624	628	rBV2	378	318	0.01%	0.002%
6	3.085	632	636	642	rVB4	490	462	0.02%	0.003%
7	3.150	653	656	659	rVB3	411	226	0.01%	0.001%
8	3.166	659	661	665	rBV2	525	326	0.02%	0.002%
9	3.220	673	678	683	rBV2	579	455	0.02%	0.003%
10	3.243	683	685	687	rVV2	196	115	0.01%	0.001%
11	3.265	688	692	695	rVV3	370	325	0.02%	0.002%
12	3.278	695	696	700	rVV2	417	261	0.01%	0.001%
13	3.304	700	704	707	rVB2	428	319	0.01%	0.002%
14	3.317	707	708	710	rBV	212	92	0.00%	0.001%
15	3.336	712	714	717	rBV2	264	162	0.01%	0.001%
16	3.378	723	727	729	rBV2	294	169	0.01%	0.001%
17	3.400	732	734	736	rBV2	330	125	0.01%	0.001%
18	3.471	754	756	759	rVB2	589	265	0.01%	0.002%
19	3.503	763	766	770	rBV	297	218	0.01%	0.001%
20	3.532	773	775	779	rVB2	208	115	0.01%	0.001%
21	3.561	780	784	785	rBV	413	212	0.01%	0.001%
22	3.584	790	791	793	rBV	240	105	0.00%	0.001%
23	3.622	799	803	804	rBV2	209	143	0.01%	0.001%
24	3.658	811	814	815	rBV	432	194	0.01%	0.001%
25	3.754	841	844	847	rVB2	270	156	0.01%	0.001%
26	3.770	847	849	852	rVB2	245	136	0.01%	0.001%
27	3.831	866	868	871	rBV2	231	140	0.01%	0.001%
28	3.883	873	884	917	rBV	134150	392528	18.44%	2.224%
29	4.349	1012	1029	1056	rBV	337609	829060	38.95%	4.698%
30	4.635	1114	1118	1120	rBV2	621	475	0.02%	0.003%
31	4.731	1143	1148	1150	rBV3	757	595	0.03%	0.003%
32	4.838	1178	1181	1187	rVB3	557	419	0.02%	0.002%
33	4.876	1187	1193	1196	rBV4	537	632	0.03%	0.004%
34	4.915	1204	1205	1209	rVB3	255	151	0.01%	0.001%
35	4.934	1209	1211	1212	rBV	237	91	0.00%	0.001%
36	5.047	1227	1246	1279	rBV2	802879	2079583	97.70%	11.784%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021021\
 Data File : VW020289.D
 Acq On : 10 Feb 2021 15:34
 Operator : SY/MD
 Sample : M1377-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

37	5.391	1351	1353	1357	rBV3	679	396	0.02%	0.002%
38	5.413	1357	1360	1362	rBV2	782	499	0.02%	0.003%
39	5.545	1399	1401	1404	rBV2	573	354	0.02%	0.002%
40	5.616	1410	1423	1456	rBV	848041	1694966	79.63%	9.604%
41	5.905	1505	1513	1532	rVB2	25411	52883	2.48%	0.300%
42	6.069	1550	1564	1589	rBV	455550	929582	43.67%	5.267%
43	6.320	1639	1642	1643	rBV2	578	355	0.02%	0.002%
44	6.426	1673	1675	1676	rBV2	580	244	0.01%	0.001%
45	6.471	1685	1689	1690	rBV	411	270	0.01%	0.002%
46	6.516	1699	1703	1710	rVB6	1495	1878	0.09%	0.011%
47	6.574	1719	1721	1722	rVB2	376	130	0.01%	0.001%
48	6.600	1727	1729	1731	rBV	295	215	0.01%	0.001%
49	6.628	1736	1738	1744	rBV3	503	402	0.02%	0.002%
50	6.677	1751	1753	1760	rVB3	774	586	0.03%	0.003%
51	6.709	1761	1763	1768	rVV3	546	297	0.01%	0.002%
52	6.738	1770	1772	1775	rVB2	350	118	0.01%	0.001%
53	6.767	1778	1781	1786	rVB3	396	312	0.01%	0.002%
54	6.821	1794	1798	1802	rVB3	372	328	0.02%	0.002%
55	6.847	1802	1806	1807	rBV3	377	225	0.01%	0.001%
56	6.905	1820	1824	1825	rBV2	344	199	0.01%	0.001%
57	6.947	1831	1837	1838	rBV3	423	328	0.02%	0.002%
58	6.985	1838	1849	1872	rBV	250675	459110	21.57%	2.602%
59	7.317	1939	1952	1977	rBV	995029	1715976	80.62%	9.723%
60	7.622	2037	2047	2068	rBV	174841	306935	14.42%	1.739%
61	7.889	2127	2130	2133	rVB4	474	309	0.01%	0.002%
62	7.940	2136	2146	2156	rBV2	7034	12725	0.60%	0.072%
63	8.091	2182	2193	2232	rBV	453869	866753	40.72%	4.911%
64	8.571	2340	2342	2343	rBV2	506	211	0.01%	0.001%
65	8.609	2352	2354	2356	rBV2	381	234	0.01%	0.001%
66	8.699	2379	2382	2383	rBV	256	127	0.01%	0.001%
67	8.857	2418	2431	2468	rBV	1280989	2104710	98.88%	11.926%
68	9.226	2537	2546	2557	rBV8	2791	5200	0.24%	0.029%
69	9.304	2568	2570	2571	rBV	454	134	0.01%	0.001%
70	9.345	2581	2583	2587	rBV	689	277	0.01%	0.002%
71	9.519	2635	2637	2639	rBV2	372	159	0.01%	0.001%
72	9.635	2670	2673	2678	rBV4	508	415	0.02%	0.002%
73	9.680	2683	2687	2689	rBV3	544	300	0.01%	0.002%
74	9.738	2700	2705	2715	rVB6	1945	3231	0.15%	0.018%
75	9.789	2718	2721	2723	rBV2	399	183	0.01%	0.001%
76	9.837	2734	2736	2742	rBV4	795	550	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021021\
 Data File : VV020289.D
 Acq On : 10 Feb 2021 15:34
 Operator : SY/MD
 Sample : M1377-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis

77	9.918	2757	2761	2764	rVB3	420	284	0.01%	0.002%
78	9.934	2764	2766	2770	rBV2	452	345	0.02%	0.002%
79	9.982	2779	2781	2786	rVB	387	227	0.01%	0.001%
80	10.005	2786	2788	2790	rBV	311	171	0.01%	0.001%
81	10.072	2808	2809	2810	rBV	343	99	0.00%	0.001%
82	10.114	2819	2822	2826	rBV2	531	298	0.01%	0.002%
83	10.162	2835	2837	2839	rBV	285	137	0.01%	0.001%
84	10.220	2843	2855	2882	rVV	596943	948299	44.55%	5.373%
85	10.387	2898	2907	2921	rVB	14087	22638	1.06%	0.128%
86	10.477	2931	2935	2937	rBV2	367	271	0.01%	0.002%
87	10.516	2944	2947	2948	rBV2	430	216	0.01%	0.001%
88	10.596	2969	2972	2974	rBV2	453	236	0.01%	0.001%
89	10.644	2985	2987	2988	rBV2	353	142	0.01%	0.001%
90	10.683	2996	2999	3000	rBV2	537	240	0.01%	0.001%
91	10.744	3016	3018	3022	rBV2	268	218	0.01%	0.001%
92	11.030	3103	3107	3109	rBV2	374	273	0.01%	0.002%
93	11.056	3113	3115	3116	rBV	493	225	0.01%	0.001%
94	11.255	3165	3177	3201	rBV	1378646	2128513	100.00%	12.061%
95	11.632	3281	3294	3316	rBV	1048649	1645887	77.33%	9.326%
96	12.033	3417	3419	3422	rBV3	364	114	0.01%	0.001%
97	12.230	3478	3480	3481	rBV	543	190	0.01%	0.001%
98	12.262	3483	3490	3500	rVB2	7174	9973	0.47%	0.057%
99	13.275	3797	3805	3816	rVB5	5902	9720	0.46%	0.055%
100	13.455	3857	3861	3867	rVB7	2121	2149	0.10%	0.012%




Sum of corrected areas: 17647851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021021\
Data File : VV020289.D
Acq On : 10 Feb 2021 15:34
Operator : SY/MD
Sample : M1377-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

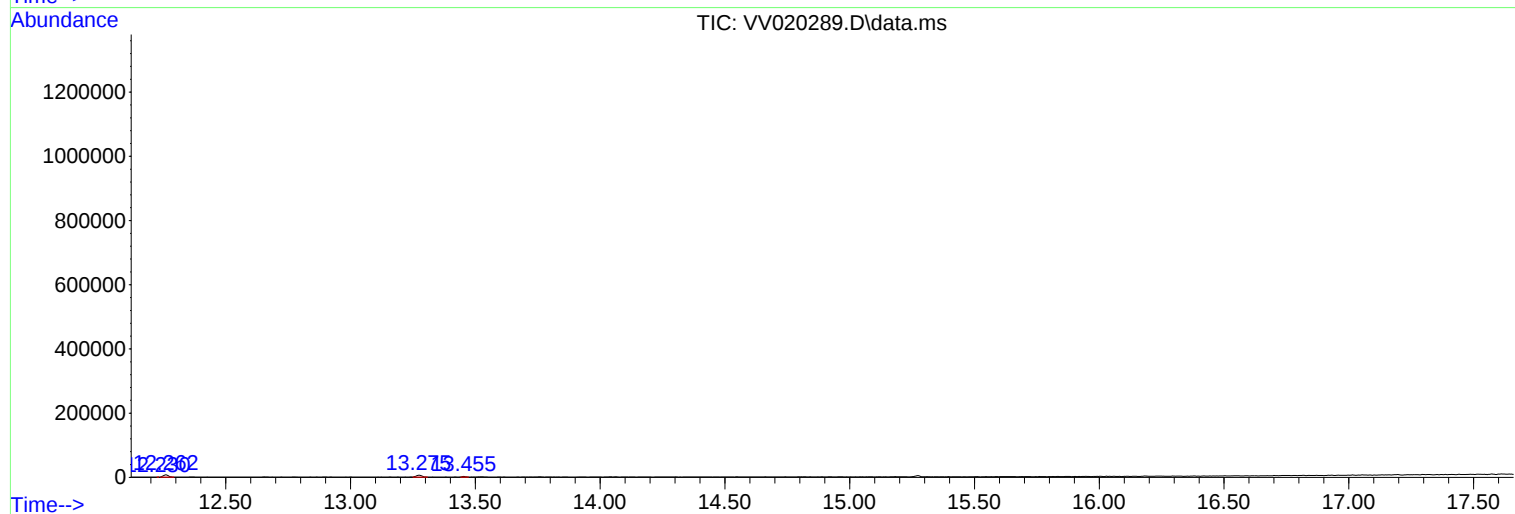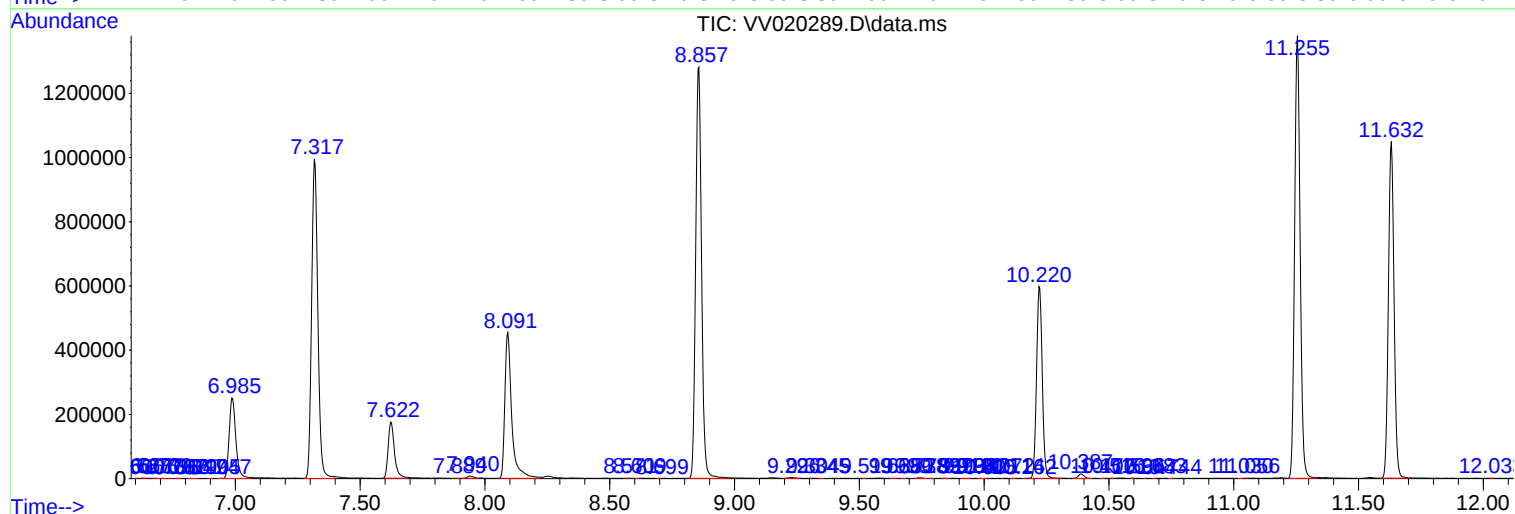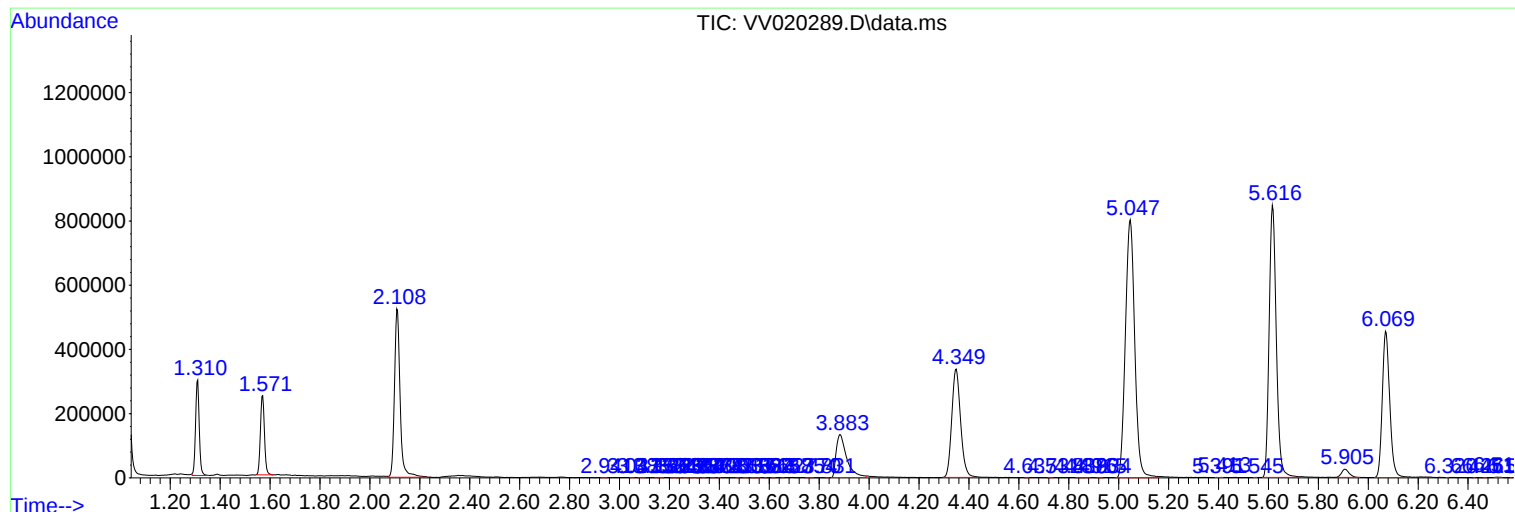

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021021\
Data File : VV020289.D
Acq On : 10 Feb 2021 15:34
Operator : SY/MD
Sample : M1377-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021021\
Data File : VV020289.D
Acq On : 10 Feb 2021 15:34
Operator : SY/MD
Sample : M1377-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COBJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
