
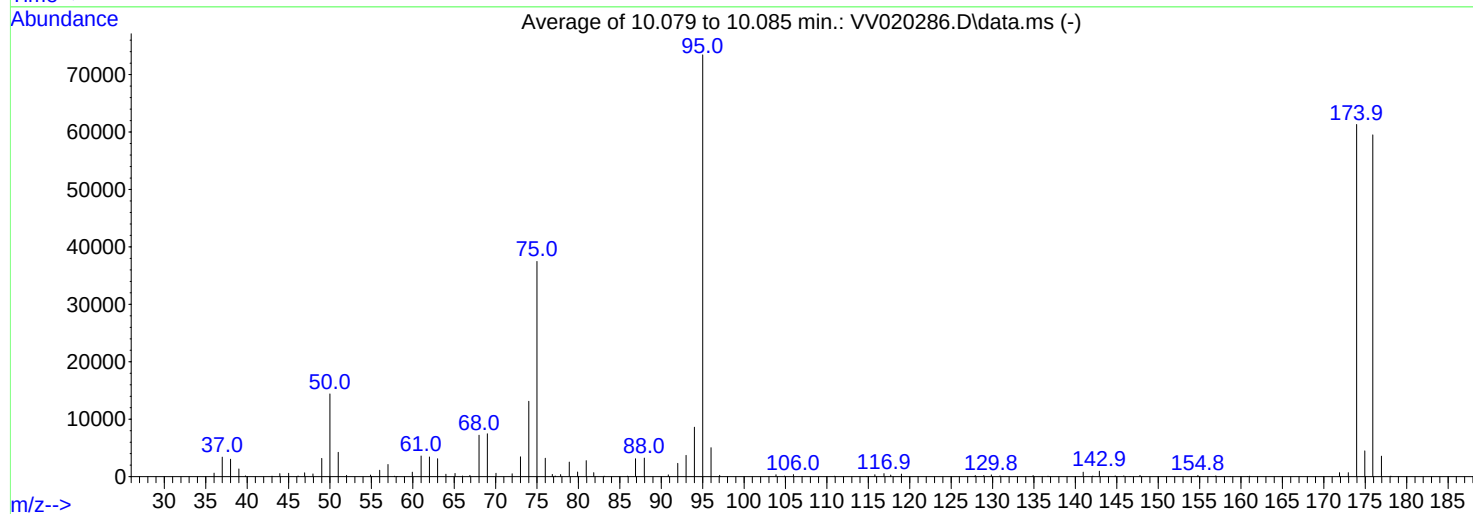


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021021\
 Data File : VV020286.D
 Acq On : 10 Feb 2021 09:12
 Operator : SY/MD
 Sample : BFB88
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB88

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM020521WMA.M
 Title : VOC Analysis
 Last Update : Tue Feb 09 01:47:10 2021

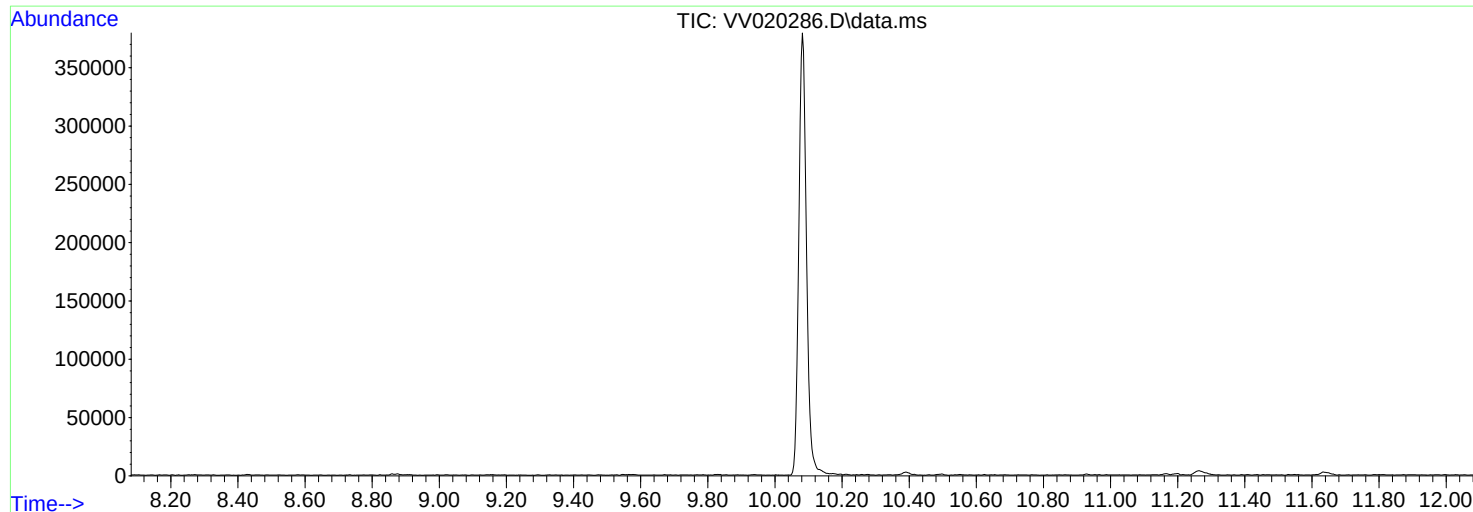

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	14409	PASS
75	95	30	80	51.0	37472	PASS
95	95	100	100	100.0	73445	PASS
96	95	5	9	6.9	5036	PASS
173	174	0.00	2	1.2	711	PASS
174	95	50	120	83.5	61315	PASS
175	174	5	9	7.3	4477	PASS
176	174	95	101	97.1	59515	PASS
177	176	5	9	6.0	3581	PASS

m/z	Abundance
36.00	632.0
37.00	3339.0
38.00	3075.0
39.00	1367.0
39.80	234.0
44.00	961.0
45.00	502.0
46.20	113.0
46.90	670.0
47.90	458.0
49.00	3099.0
50.00	14653.0
51.00	4313.0
52.00	199.0
54.90	227.0
56.00	1162.0
57.00	1960.0
58.10	122.0
60.00	724.0
61.00	3604.0
62.00	3600.0
63.00	2969.0
64.00	357.0
65.10	528.0
66.00	125.0
66.90	228.0
68.00	7631.0
69.00	7928.0
70.00	566.0
72.00	532.0
73.00	3472.0
74.00	12670.0
75.00	37184.0
76.00	3106.0
76.90	439.0
77.80	384.0
78.90	2435.0
79.90	788.0
80.90	2697.0
81.80	693.0
85.90	127.0
86.90	3303.0
88.00	3240.0
90.80	241.0
92.00	2402.0
93.00	3597.0
94.00	8314.0
95.00	71296.0
96.00	5087.0
97.10	190.0
103.80	363.0
105.00	125.0
105.90	299.0
107.00	106.0
110.90	122.0
115.80	361.0
116.90	455.0
117.70	295.0
119.00	448.0
127.80	266.0
128.90	124.0
129.80	253.0
130.90	108.0
135.00	210.0
136.70	133.0
141.00	782.0
142.10	126.0
142.90	875.0
144.80	139.0
145.80	129.0
146.60	107.0
147.80	206.0
154.80	241.0
156.90	156.0
160.80	102.0
171.90	625.0
172.90	771.0
174.00	58392.0
175.00	4368.0
175.90	56760.0
177.00	3538.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
36.00	635.0
37.00	3524.0
38.00	3145.0
39.00	1391.0
43.00	104.0
44.00	1057.0
45.00	606.0
46.20	126.0
47.00	690.0
47.90	478.0
49.00	3291.0
50.00	14895.0
51.00	4365.0
52.00	223.0
54.90	282.0
56.00	1172.0
57.00	2197.0
57.80	132.0
59.90	793.0
61.00	3738.0
62.00	3487.0
63.00	3169.0
64.00	445.0
65.10	587.0
66.00	123.0
66.90	240.0
68.00	7384.0
69.00	7632.0
70.10	591.0
72.00	540.0
73.00	3552.0
74.00	13699.0
75.00	38632.0
76.00	3315.0
76.80	415.0
77.90	335.0
78.90	2607.0
79.90	832.0
80.90	2865.0
81.80	705.0
83.10	124.0
86.00	120.0
86.90	3209.0
88.00	3308.0
90.80	303.0
92.00	2426.0
93.00	3879.0
94.00	8931.0
95.00	76376.0
96.00	5286.0
97.00	237.0
103.90	357.0
104.90	115.0
106.00	384.0
111.00	120.0
115.80	346.0
116.90	549.0
117.70	292.0
119.00	456.0
128.00	285.0
128.90	194.0
129.90	306.0
130.90	127.0
134.90	206.0
136.70	127.0
140.90	785.0
142.10	133.0
142.90	997.0
144.80	134.0
145.90	145.0
147.80	241.0
154.80	249.0
157.00	152.0
161.00	104.0
171.90	685.0
173.00	735.0
174.00	63336.0
175.00	4599.0
175.90	61600.0
176.90	3713.0
178.10	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
36.00	592.0
37.00	3352.0
38.00	2928.0
39.00	1282.0
39.80	204.0
43.00	138.0
44.00	1139.0
45.00	641.0
46.10	125.0
47.00	682.0
48.00	463.0
49.00	3177.0
50.00	13680.0
51.00	4063.0
52.00	224.0
54.90	317.0
56.00	1020.0
57.00	2180.0
57.80	117.0
59.90	789.0
61.00	3434.0
62.00	3196.0
63.00	3189.0
64.00	435.0
65.10	597.0
66.00	113.0
66.90	212.0
68.00	6674.0
69.00	6818.0
70.10	582.0
72.00	457.0
73.00	3329.0
74.00	13019.0
75.00	36600.0
76.00	3236.0
76.80	363.0
77.20	323.0
77.90	337.0
78.90	2548.0
79.90	795.0
81.00	2814.0
81.90	678.0
83.10	108.0
86.90	2856.0
87.90	3144.0
90.90	348.0
92.00	2136.0
93.00	3641.0
94.00	8575.0
95.00	72664.0
96.00	4734.0
97.00	270.0
103.90	330.0
104.80	115.0
106.00	445.0
114.80	108.0
115.80	322.0
116.90	596.0
117.70	291.0
119.00	413.0
127.90	251.0
129.00	251.0
129.90	331.0
130.90	155.0
134.80	217.0
136.90	124.0
140.90	796.0
142.10	103.0
142.90	945.0
144.80	125.0
145.80	120.0
147.80	213.0
154.80	221.0
157.00	132.0
158.70	124.0
161.10	141.0
171.90	746.0
173.00	628.0
173.90	62216.0
174.90	4465.0
175.90	60184.0
176.90	3492.0
178.10	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88

m/z	Abundance
40.10	240.0
43.90	515.0

Instrument :
MSVOA_V
ClientSampleId :
BFB88