
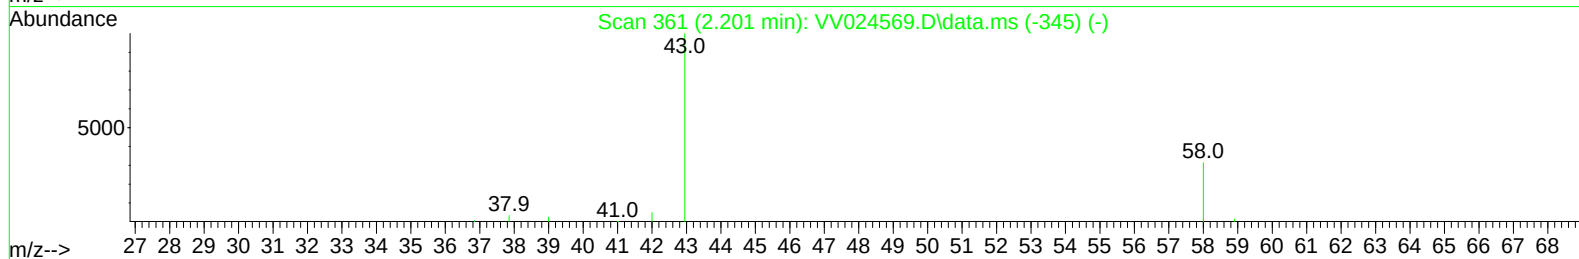
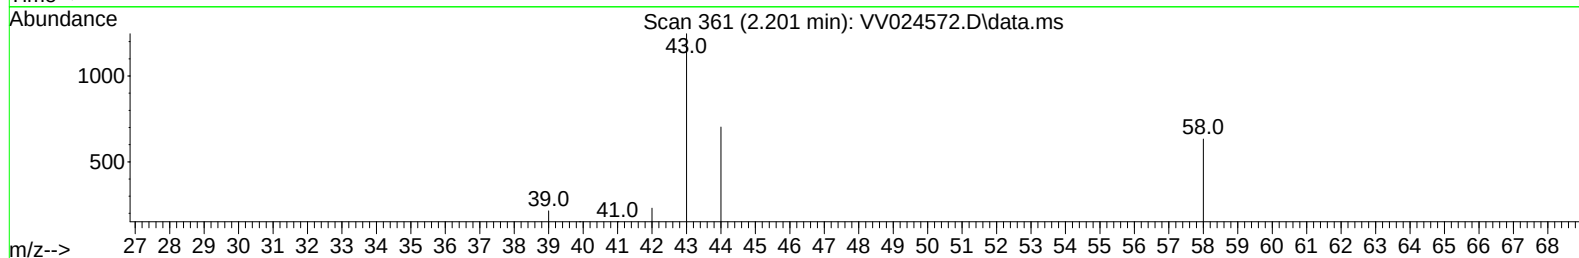


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024572.D
Acq On : 10 Feb 2022 16:52
Operator : SY/MD
Sample : N1476-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Feb 11 23:55:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration

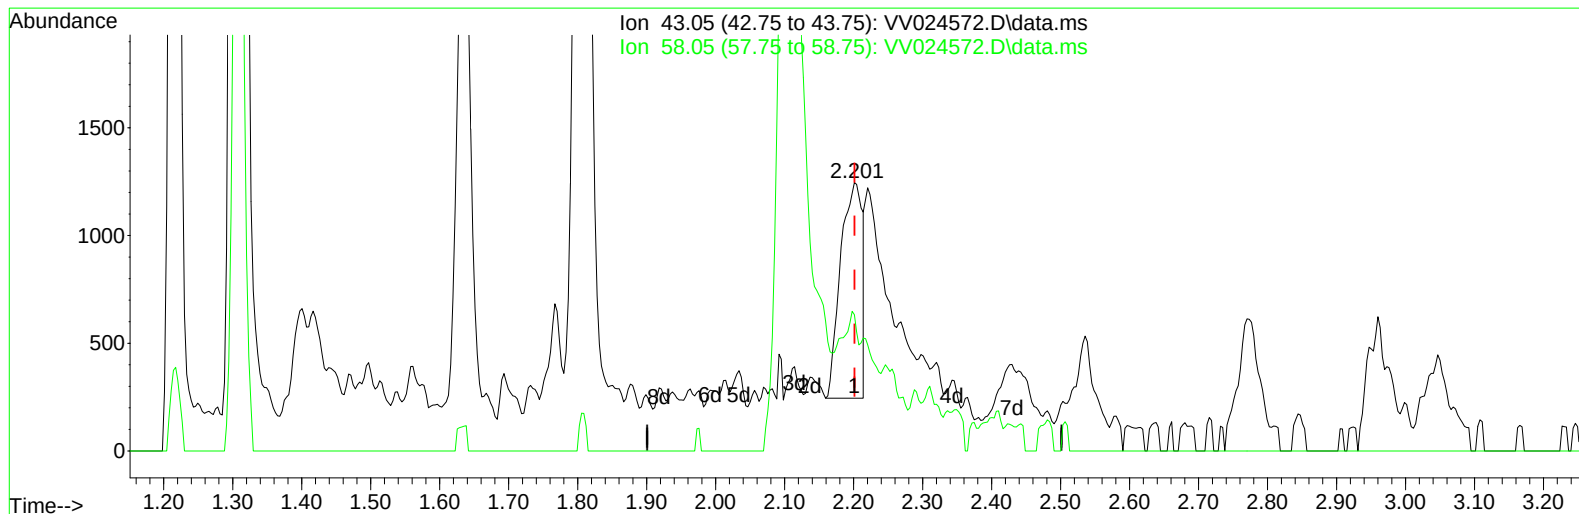

TIC: VV024572.D\data.ms

(13) Acetone (T)**2.201min (-0.000) 4603.97 ug/L****response 2174**

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	14.35
0.00	0.00	0.00
0.00	0.00	0.00