
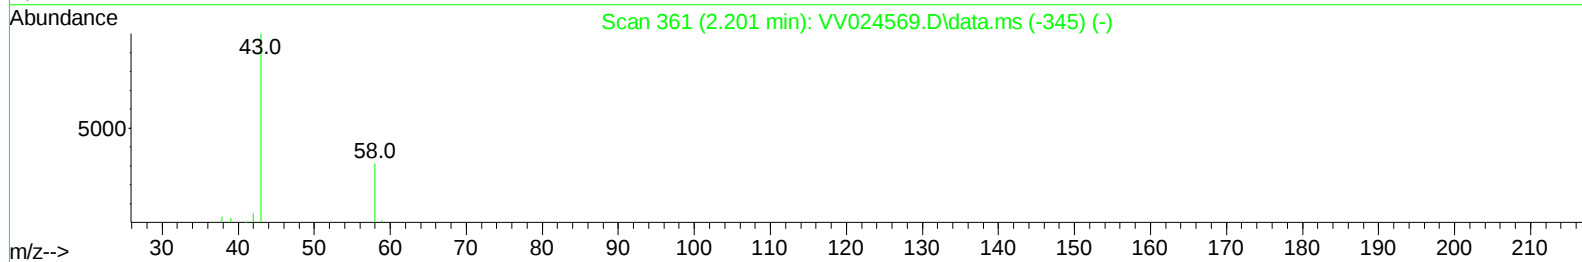
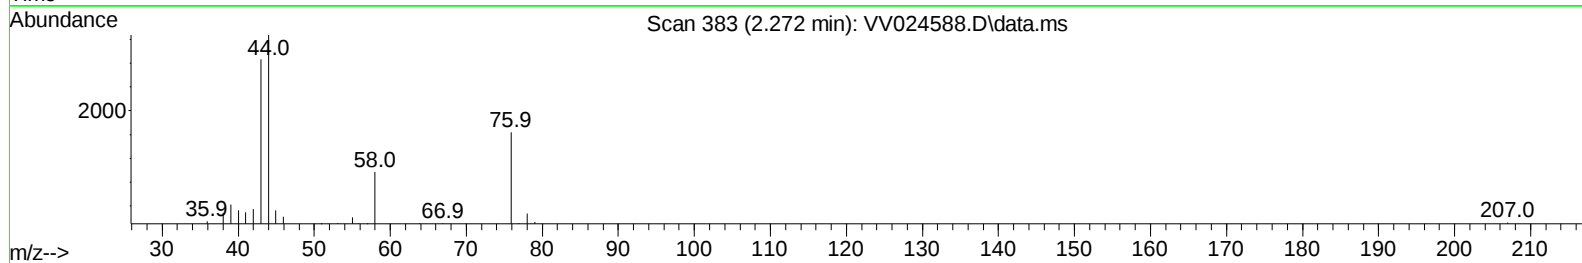


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024588.D
Acq On : 10 Feb 2022 23:06
Operator : SY/MD
Sample : N1475-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Feb 11 23:59:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration

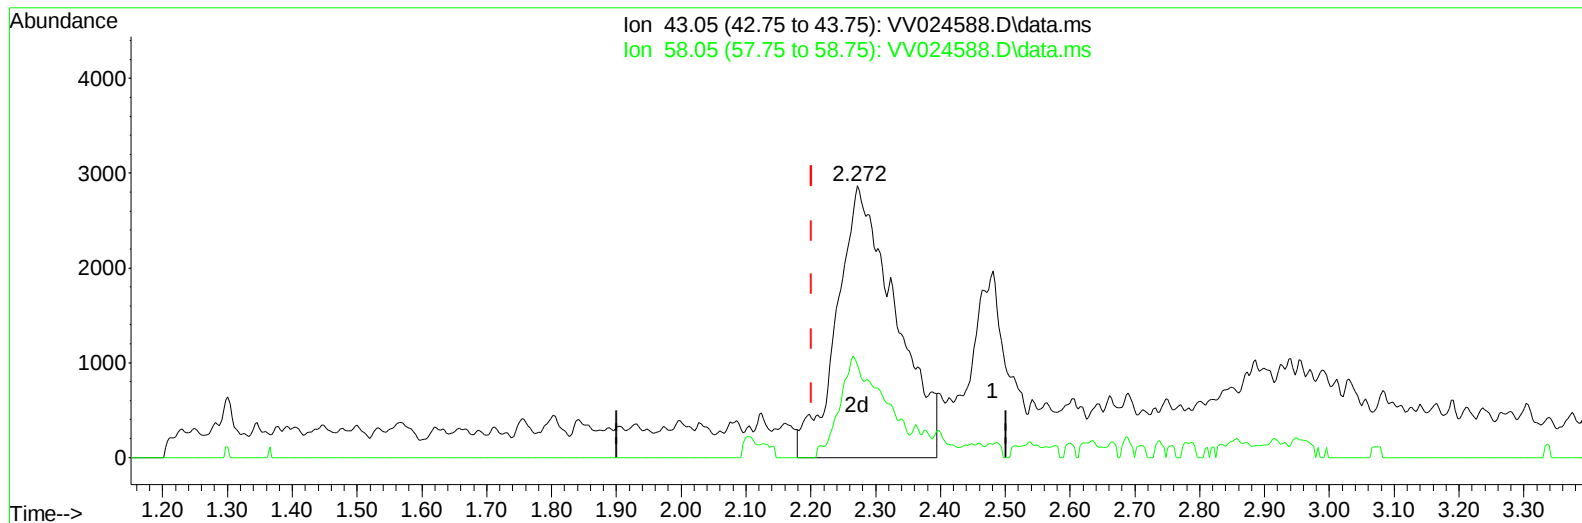

TIC: VV024588.D\data.ms

(13) Acetone (T)

2.272min (+ 0.071) 13.77 ug/L m

response 17887

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	1.05
0.00	0.00	0.00
0.00	0.00	0.00