

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW021022\
 Data File : VW024572.D
 Acq On : 10 Feb 2022 16:52
 Operator : SY/MD
 Sample : N1476-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Feb 11 23:55:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.654	114	43	5.000	ug/L	# 0.04
28) Chlorobenzene-d5	8.870	117	737	5.000	ug/L	# 0.02
58) 1,4-Dichlorobenzene-d4	11.255	152	843	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	69	19.143	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	382.800%#	
7) Chloroethane-d5	1.548	69	76	24.941	ug/L	-0.02
Spiked Amount	5.000	Range 65 - 130	Recovery	=	498.800%#	
11) 1,1-Dichloroethene-d2	2.111	63	437	55.428	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	1108.600%#	
20) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount	50.000	Range 40 - 130	Recovery	=	0.000%#	
24) Chloroform-d	4.371	84	42	6.621	ug/L	0.03
Spiked Amount	5.000	Range 70 - 125	Recovery	=	132.400%#	
26) 1,2-Dichloroethane-d4	0.000	65	0	0.000	ug/L	
Spiked Amount	5.000	Range 70 - 130	Recovery	=	0.000%#	
32) Benzene-d6	5.059	84	121	0.579	ug/L	0.01
Spiked Amount	5.000	Range 70 - 125	Recovery	=	11.600%#	
36) 1,2-Dichloropropane-d6	5.928	67	186	2.860	ug/L	-0.14
Spiked Amount	5.000	Range 60 - 140	Recovery	=	57.200%#	
41) Toluene-d8	7.336	98	360	1.846	ug/L	0.02
Spiked Amount	5.000	Range 70 - 130	Recovery	=	37.000%#	
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount	5.000	Range 55 - 130	Recovery	=	0.000%#	
46) 2-Hexanone-d5	8.236	63	228	24.640	ug/L	0.15
Spiked Amount	50.000	Range 45 - 130	Recovery	=	49.280%	
56) 1,1,2,2-Tetrachloroeth...	0.000	84	0	0.000	ug/L	
Spiked Amount	5.000	Range 65 - 120	Recovery	=	0.000%#	
66) 1,2-Dichlorobenzene-d4	11.635	152	604	4.445	ug/L	0.01
Spiked Amount	5.000	Range 80 - 120	Recovery	=	88.800%	
Target Compounds						
						Qvalue
3) Chloromethane	1.243	50	335	60.254	ug/L #	82
6) Bromomethane	1.532	94	380	103.096	ug/L	85
8) Chloroethane	1.577	64	20	5.454	ug/L #	44
12) 1,1-Dichloroethene	2.121	96	108	24.258	ug/L #	62
13) Acetone	2.201	43	2174	4603.973	ug/L	86
14) Carbon disulfide	2.298	76	594	41.978	ug/L #	54
15) Methyl Acetate	2.429	43	705	522.076	ug/L #	50
16) Methylene chloride	2.449	84	409	92.726	ug/L #	3
17) Methyl tert-butyl Ether	2.770	73	4308	469.561	ug/L #	87
19) 1,1-Dichloroethane	3.201	63	66	8.737	ug/L #	50
21) 2-Butanone	4.005	43	152	194.228	ug/L #	54
22) cis-1,2-Dichloroethene	3.947	96	41	9.298	ug/L	90
25) Chloroform	4.384	83	4549	575.353	ug/L	92
33) Benzene	5.114	78	4658	16.194	ug/L	100
34) Trichloroethene	5.924	95	652	8.232	ug/L #	58
40) 4-Methyl-2-pentanone	7.194	43	83	2.307	ug/L #	43
42) Toluene	7.394	91	11194	35.725	ug/L	92
45) 1,1,2-Trichloroethane	7.969	97	1764	39.043	ug/L #	5
47) Tetrachloroethene	7.976	164	162562	3093.706	ug/L	91

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024572.D
 Acq On : 10 Feb 2022 16:52
 Operator : SY/MD
 Sample : N1476-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Feb 11 23:55:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 23:54:44 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


48) 2-Hexanone	8.178	43	1000	40.604	ug/L #	74
49) Dibromochloromethane	7.973	129	165228	3028.449	ug/L #	11
52) Ethylbenzene	9.018	91	7031	20.167	ug/L	100
53) m,p-xylene	9.140	106	6147	46.547	ug/L	91
54) o-xylene	9.548	106	2795	21.949	ug/L	94
55) Styrene	9.574	104	731	3.497	ug/L	99
60) Isopropylbenzene	9.927	105	803	1.050	ug/L	94
61) 1,2,3-Trichloropropane	10.921	75	20	0.241	ug/L #	1
62) 1,3,5-Trimethylbenzene	10.542	105	2939	4.489	ug/L	91
63) 1,2,4-Trimethylbenzene	10.915	105	9030	13.873	ug/L	98
64) 1,3-Dichlorobenzene	11.185	146	230	0.739	ug/L #	31
65) 1,4-Dichlorobenzene	11.278	146	492	1.592	ug/L	95
67) 1,2-Dichlorobenzene	11.644	146	175	0.633	ug/L #	25
69) 1,3,5-Trichlorobenzene	12.644	180	181	0.817	ug/L #	67
70) 1,2,4-trichlorobenzene	13.262	180	290	1.622	ug/L #	78
71) Naphthalene	13.509	128	2054	6.342	ug/L #	88
72) 1,2,3-Trichlorobenzene	13.744	180	43	0.286	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024572.D
Acq On : 10 Feb 2022 16:52
Operator : SY/MD
Sample : N1476-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Feb 11 23:55:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 23:54:44 2022
Response via : Initial Calibration




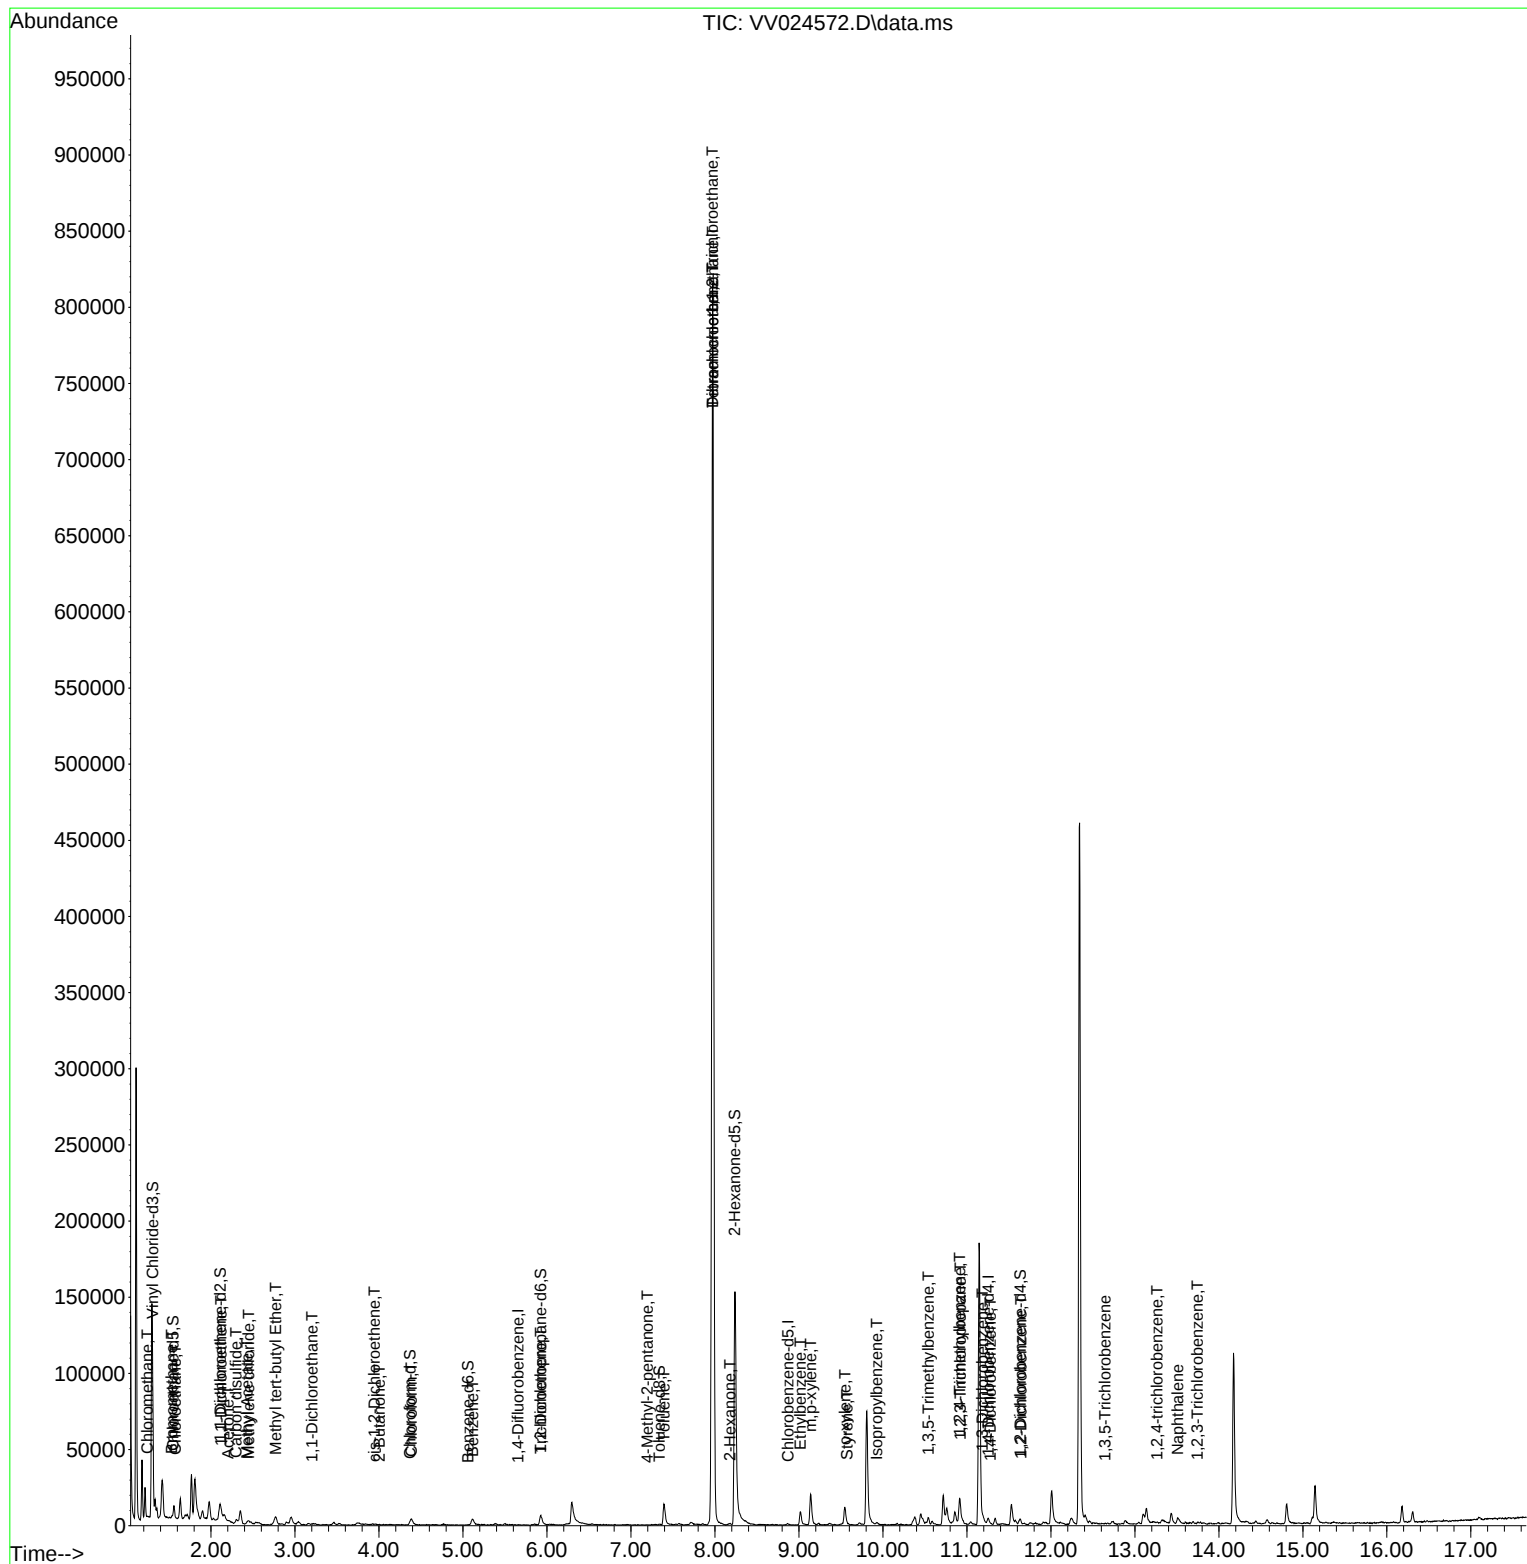


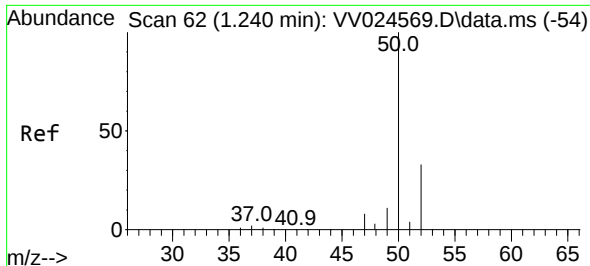

#3
Chloromethane
Concen: 60.254 ug/L
RT: 1.243 min Scan# 61
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 50 Resp: 335
Ion Ratio Lower Upper
50 100
52 41.4 22.0 41.0#

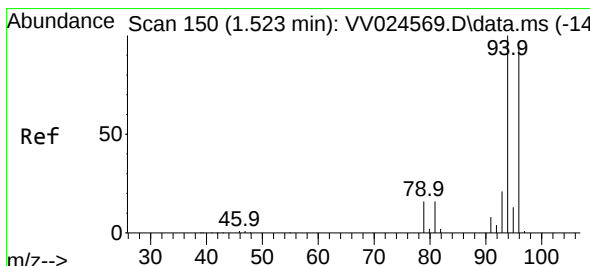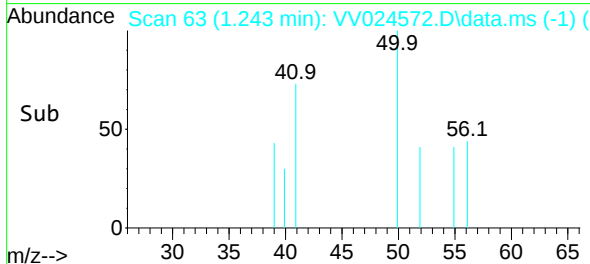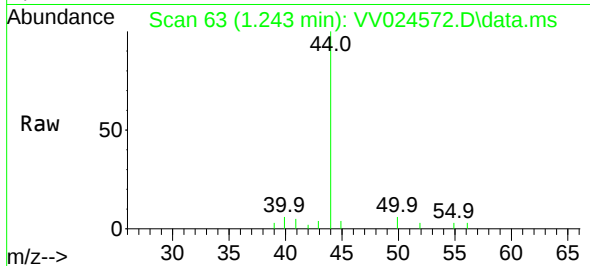

#6
Bromomethane
Concen: 103.096 ug/L
RT: 1.532 min Scan# 153
Delta R.T. 0.010 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52


Tgt Ion: 94 Resp: 380
Ion Ratio Lower Upper
94 100
96 80.0 66.2 123.0

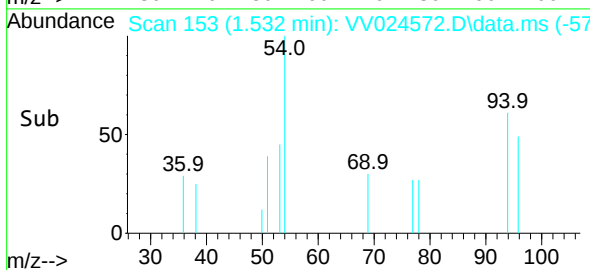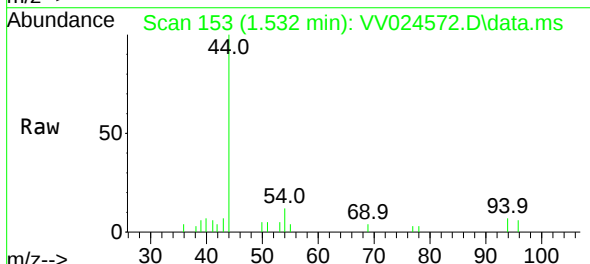






#8
Chloroethane
Concen: 5.454 ug/L
RT: 1.577 min Scan# 1
Delta R.T. -0.007 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Instrument :
MSVOA_V
ClientSampleId :







Tgt Ion: 64 Resp: 20
Ion Ratio Lower Upper
64 100
66 0.0 21.4 39.8#

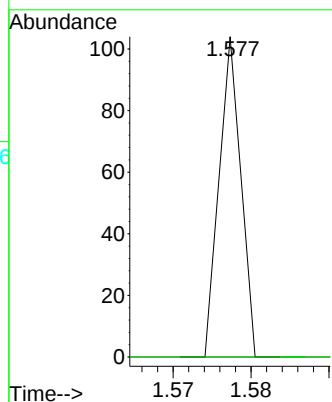

#12
1,1-Dichloroethene
Concen: 24.258 ug/L
RT: 2.121 min Scan# 336
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52


Tgt Ion: 96 Resp: 108
Ion Ratio Lower Upper
96 100
61 88.7 116.1 215.5#
63 101.8 79.4 147.4

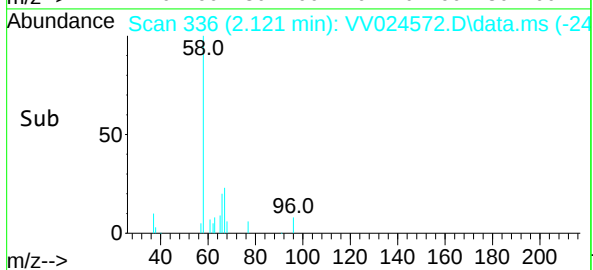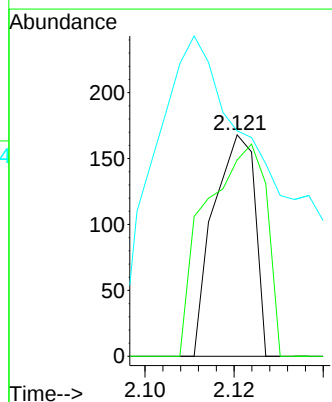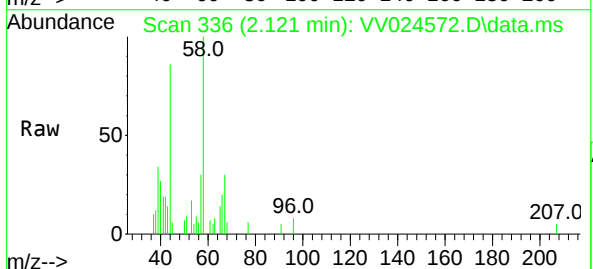






#13
Acetone
Concen: 4603.973 ug/L
RT: 2.201 min Scan# 361
Delta R.T. -0.000 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52


Instrument :
MSVOA_V
ClientSampleId :





Tgt Ion: 43 Resp: 2174
Ion Ratio Lower Upper
43 100
58 14.4 0.0 41.4

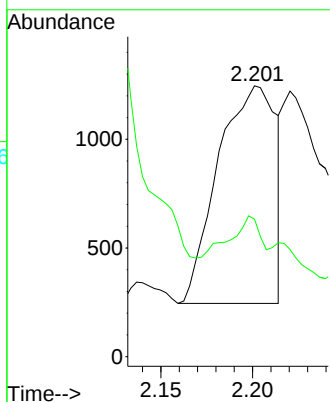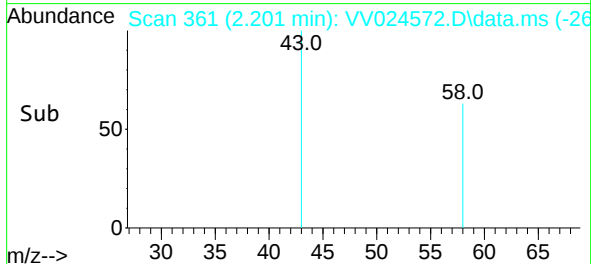


#14
Carbon disulfide
Concen: 41.978 ug/L
RT: 2.298 min Scan# 391
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52




Tgt Ion: 76 Resp: 594
Ion Ratio Lower Upper
76 100
78 26.2 7.5 11.3#

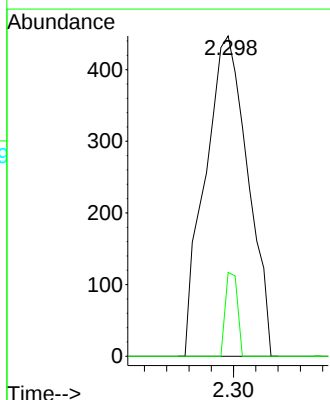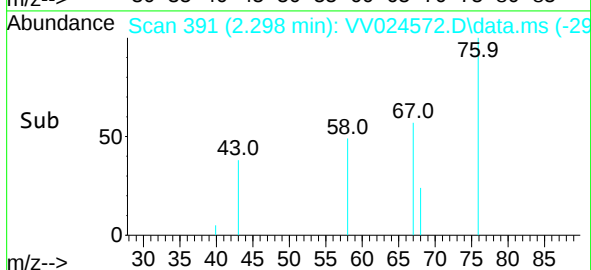






#15
Methyl Acetate
Concen: 522.076 ug/L
RT: 2.429 min Scan# 41
Delta R.T. -0.013 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Instrument :
MSVOA_V
ClientSampleId :







Tgt Ion: 43 Resp: 705
Ion Ratio Lower Upper
43 100
74 0.0 20.2 30.2#

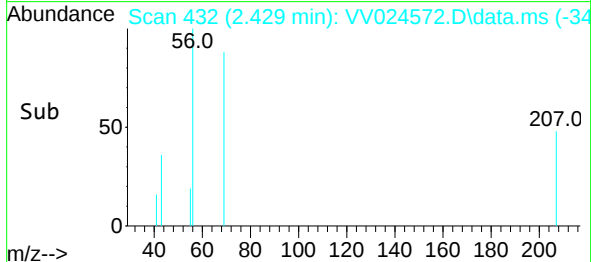

#16
Methylene chloride
Concen: 92.726 ug/L
RT: 2.449 min Scan# 438
Delta R.T. -0.058 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52


Tgt Ion: 84 Resp: 409
Ion Ratio Lower Upper
84 100
86 0.0 42.6 79.0#
49 0.0 79.7 147.9#

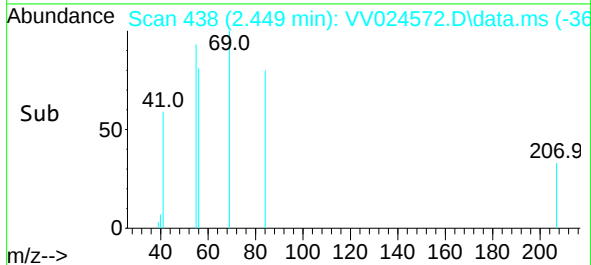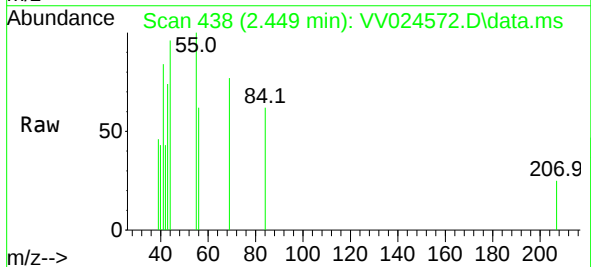






#17
Methyl tert-butyl Ether
Concen: 469.561 ug/L
RT: 2.770 min Scan# 51
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52


Instrument :
MSVOA_V
ClientSampleId :

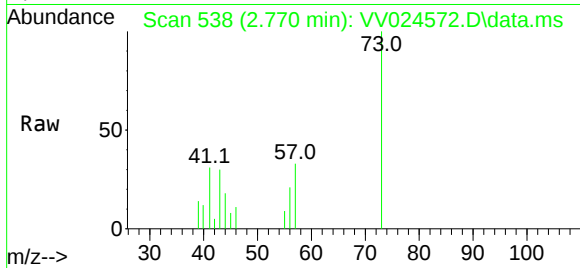



Tgt Ion: 73 Resp: 4308
Ion Ratio Lower Upper
73 100
43 31.8 15.5 23.3#
57 21.8 17.1 25.7

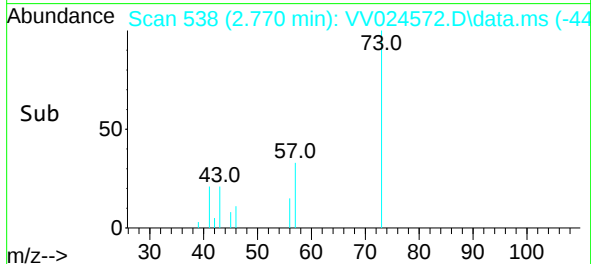


#19
1,1-Dichloroethane
Concen: 8.737 ug/L
RT: 3.201 min Scan# 672
Delta R.T. 0.013 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

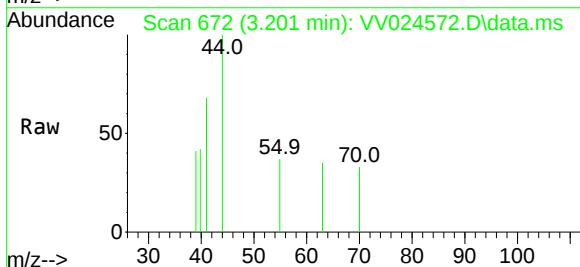


Tgt Ion: 63 Resp: 66
Ion Ratio Lower Upper
63 100
65 0.0 22.3 41.3#
83 0.0 10.7 19.9#

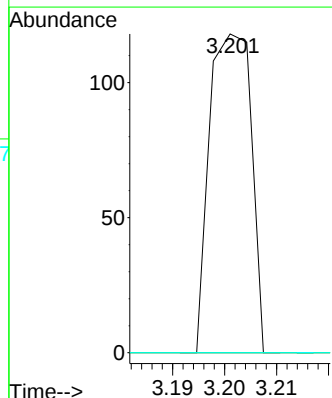






#21
2-Butanone
Concen: 194.228 ug/L
RT: 4.005 min Scan# 91
Delta R.T. 0.016 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Instrument :
MSVOA_V
ClientSampleId :







Tgt Ion: 43 Resp: 152
Ion Ratio Lower Upper
43 100
72 0.0 11.1 33.1#

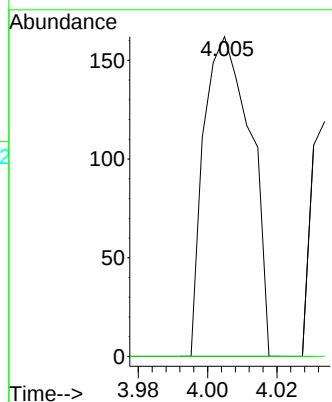

#22
cis-1,2-Dichloroethene
Concen: 9.298 ug/L
RT: 3.947 min Scan# 904
Delta R.T. 0.038 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Tgt Ion: 96 Resp: 41
Ion Ratio Lower Upper
96 100
61 108.5 83.4 154.8
68 0.0 0.0 0.0

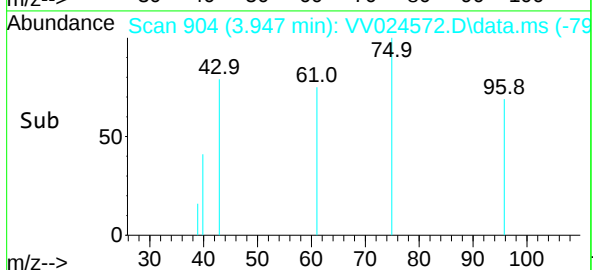



#25

Chloroform

Concen: 575.353 ug/L

RT: 4.384 min Scan# 1040

Delta R.T. 0.013 min

Lab File: VV024572.D

Acq: 10 Feb 2022 16:52

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 83 Resp: 4549

Ion Ratio Lower Upper

83 100

85 58.0 45.2 84.0

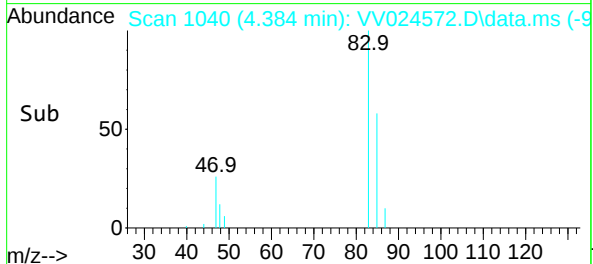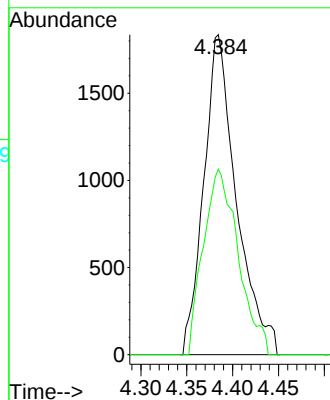

#33

Benzene

Concen: 16.194 ug/L




RT: 5.114 min Scan# 1267


Delta R.T. 0.019 min

Lab File: VV024572.D

Acq: 10 Feb 2022 16:52


Tgt Ion: 78 Resp: 4658

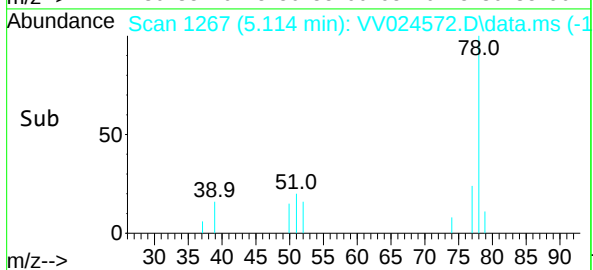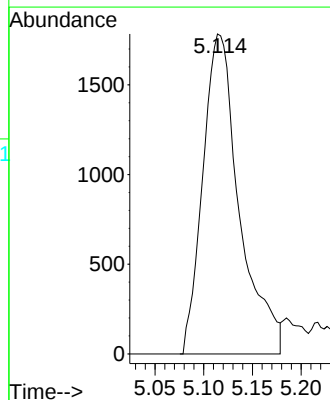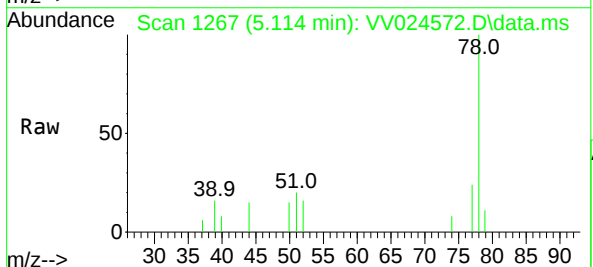






#34
Trichloroethene
Concen: 8.232 ug/L
RT: 5.924 min Scan# 11
Delta R.T. 0.013 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Instrument :
MSVOA_V
ClientSampleId :



Tgt Ion: 95 Resp: 652




Ion	Ratio	Lower	Upper
95	100		
97	56.4	45.2	84.0
132	54.7	76.1	141.3#
130	53.3	75.4	140.0#

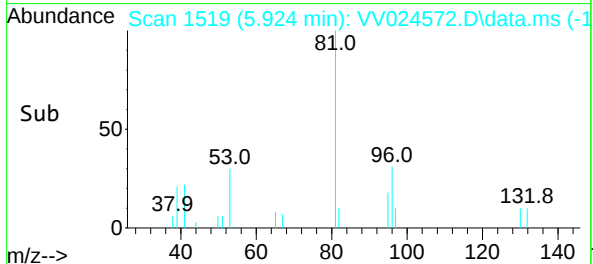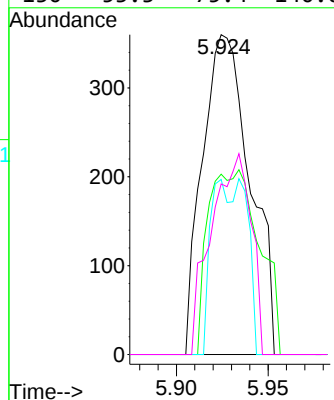


#40
4-Methyl-2-pentanone
Concen: 2.307 ug/L
RT: 7.194 min Scan# 1914
Delta R.T. -0.029 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Tgt Ion: 43 Resp: 83

Ion	Ratio	Lower	Upper
43	100		
58	0.0	32.3	48.5#
100	0.0	13.0	19.6#


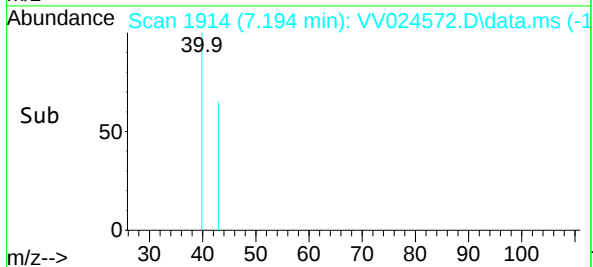
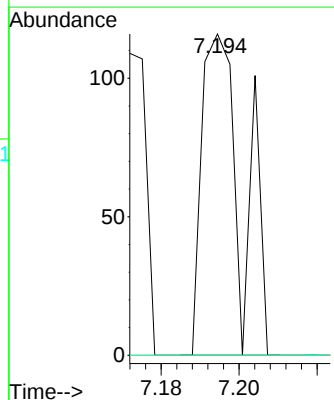
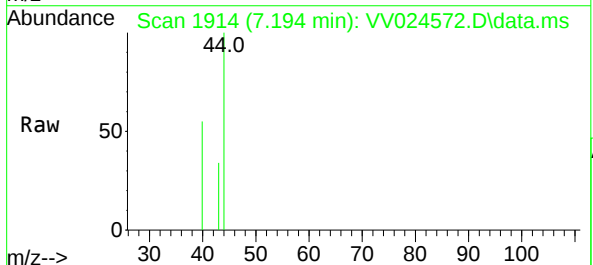




#42
Toluene
Concen: 35.725 ug/L
RT: 7.394 min Scan# 11
Delta R.T. 0.010 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion: 91 Resp: 11194
Ion Ratio Lower Upper
91 100
92 53.2 41.5 77.1

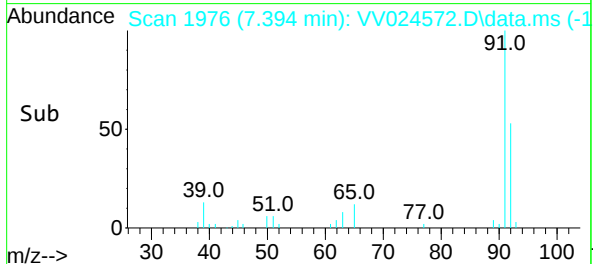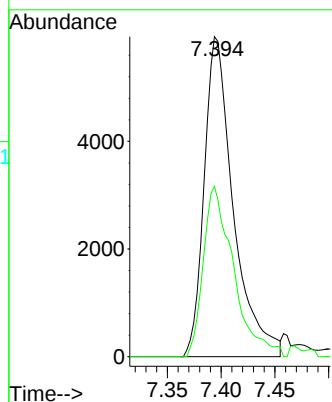

#45
1,1,2-Trichloroethane
Concen: 39.043 ug/L
RT: 7.969 min Scan# 2155
Delta R.T. 0.132 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52


Tgt Ion: 97 Resp: 1764
Ion Ratio Lower Upper
97 100
99 19.4 43.1 80.1#
83 232.7 57.9 107.5#
85 32.9 38.0 70.6#

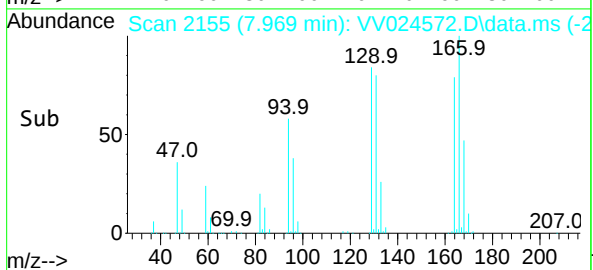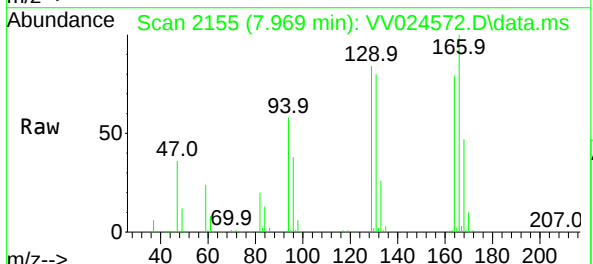






#47
Tetrachloroethene
Concen: 3093.706 ug/L
RT: 7.976 min Scan# 2156
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Instrument :
MSVOA_V
ClientSampleId :







Tgt Ion:164 Resp: 162562
Ion Ratio Lower Upper
164 100
129 102.6 62.6 116.2
131 100.7 61.0 113.4
166 125.9 87.3 162.1

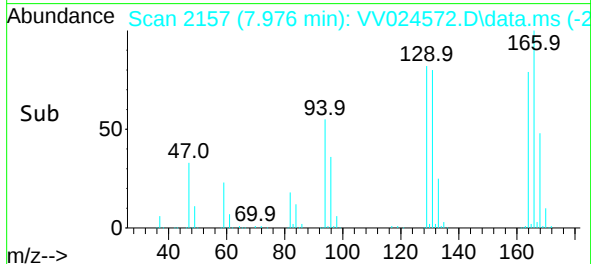

#48
2-Hexanone
Concen: 40.604 ug/L
RT: 8.178 min Scan# 2220
Delta R.T. 0.042 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Tgt Ion: 43 Resp: 1000
Ion Ratio Lower Upper
43 100
58 42.0 44.5 66.7#
57 0.0 15.1 22.7#
100 0.0 10.7 16.1#

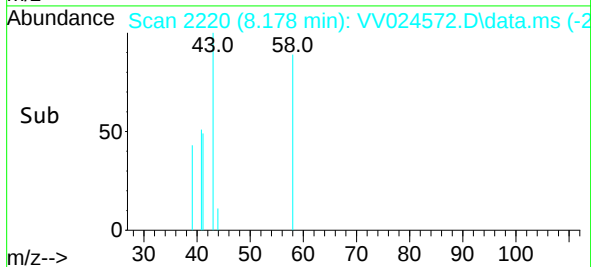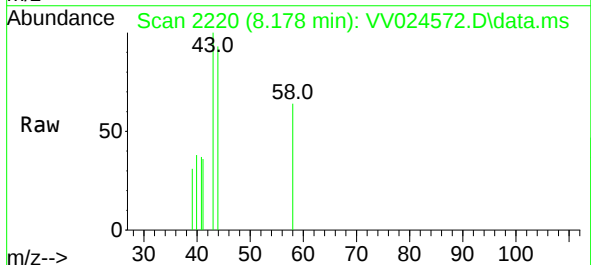



#49

Dibromochloromethane

Concen: 3028.449 ug/L

RT: 7.973 min Scan# 2156

Delta R.T. -0.270 min

Lab File: VV024572.D

Acq: 10 Feb 2022 16:52

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion:129 Resp: 165228

Ion Ratio Lower Upper

129 100

127 0.0 53.5 99.3#

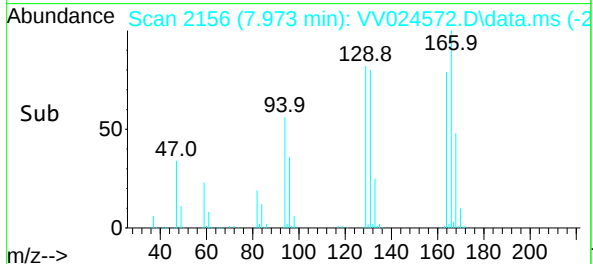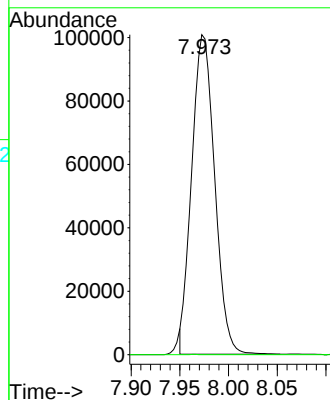

#52

Ethylbenzene

Concen: 20.167 ug/L

RT: 9.018 min Scan# 2481

Delta R.T. 0.010 min

Lab File: VV024572.D




Acq: 10 Feb 2022 16:52


Tgt Ion: 91 Resp: 7031

Ion Ratio Lower Upper

91 100

106 31.7 22.0 41.0


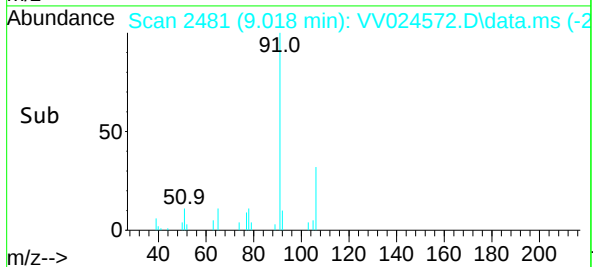
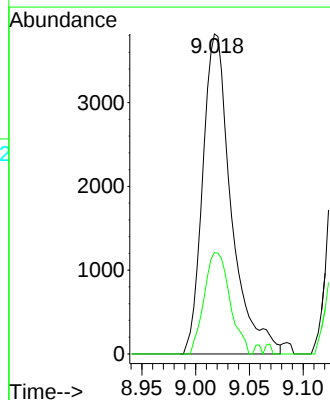
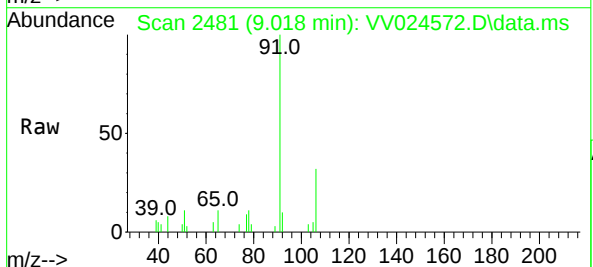




#53
m,p-xylene
Concen: 46.547 ug/L
RT: 9.140 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:106 Resp: 6147
Ion Ratio Lower Upper
106 100
91 185.4 139.5 259.1

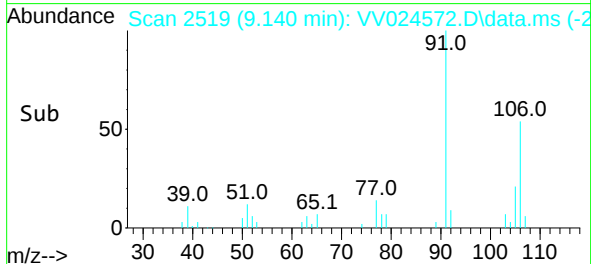

#54
o-xylene
Concen: 21.949 ug/L
RT: 9.548 min Scan# 2646
Delta R.T. 0.006 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Tgt Ion:106 Resp: 2795
Ion Ratio Lower Upper
106 100
91 220.2 147.9 274.7


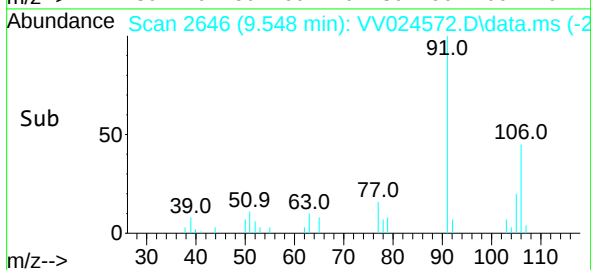

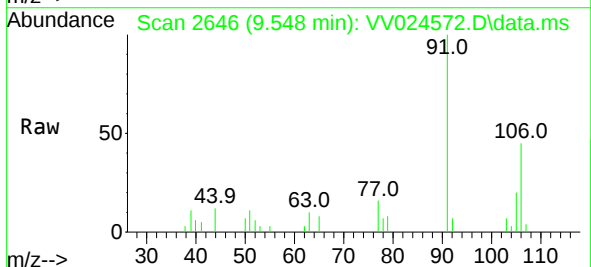




#55
Styrene
Concen: 3.497 ug/L
RT: 9.574 min Scan# 20
Delta R.T. 0.016 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:104 Resp: 731
Ion Ratio Lower Upper
104 100
78 43.5 31.0 57.6

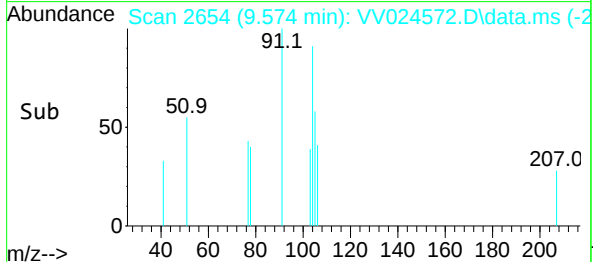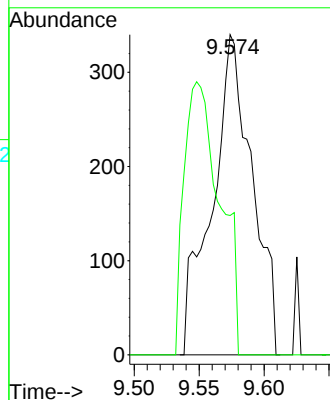

#60
Isopropylbenzene
Concen: 1.050 ug/L
RT: 9.927 min Scan# 2764
Delta R.T. -0.000 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Tgt Ion:105 Resp: 803
Ion Ratio Lower Upper
105 100
120 22.3 21.4 32.0
77 16.4 12.2 18.4

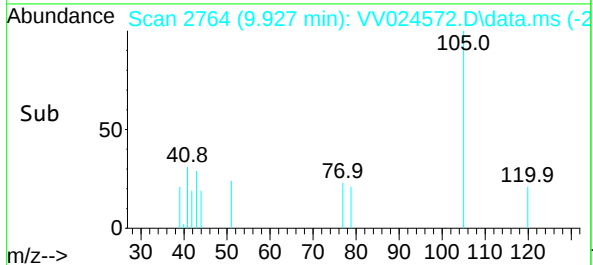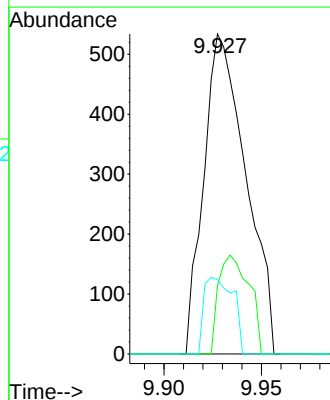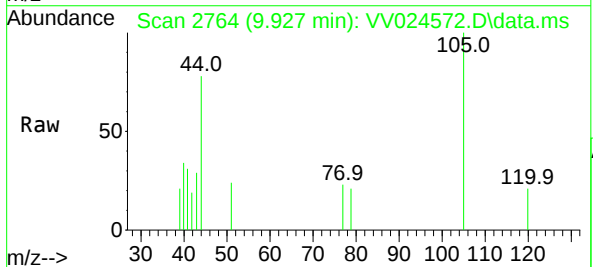



#61

1,2,3-Trichloropropane

Concen: 0.241 ug/L

RT: 10.921 min Scan# 30

Delta R.T. 0.649 min

Lab File: VV024572.D

Acq: 10 Feb 2022 16:52





Instrument :

MSVOA_V

ClientSampleId :

Tgt Ion: 75 Resp: 20

Ion	Ratio	Lower	Upper
75	100		
77	7195.0	26.4	39.6#
110	0.0	34.2	51.2#

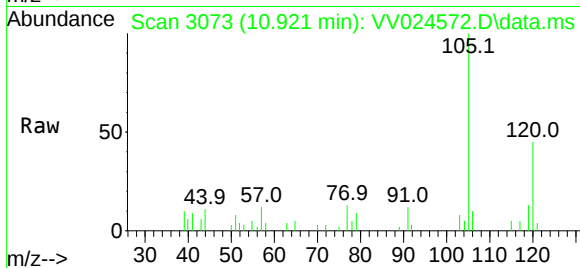

#62

1,3,5-Trimethylbenzene

Concen: 4.489 ug/L

RT: 10.542 min Scan# 2955




Delta R.T. 0.006 min


Lab File: VV024572.D

Acq: 10 Feb 2022 16:52

Tgt Ion: 105 Resp: 2939

Ion	Ratio	Lower	Upper
105	100		
120	44.2	40.1	60.1

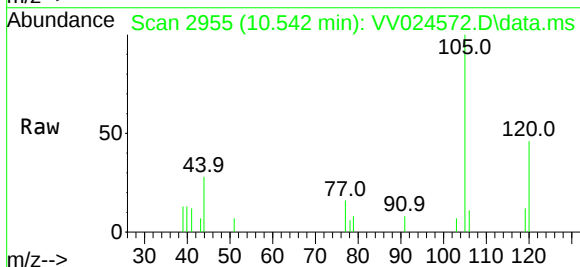



#63

1,2,4-Trimethylbenzene

Concen: 13.873 ug/L

RT: 10.915 min Scan# 3070

Delta R.T. 0.003 min

Lab File: VV024572.D

Acq: 10 Feb 2022 16:52

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion:105 Resp: 9030

Ion Ratio Lower Upper

105 100

120 44.5 36.7 55.1

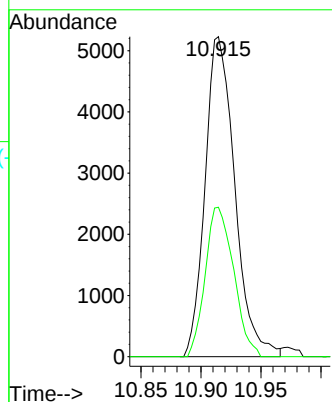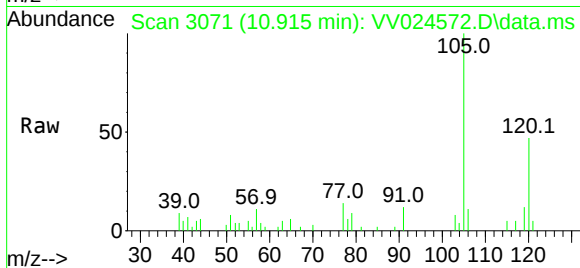

#64

1,3-Dichlorobenzene

Concen: 0.739 ug/L

RT: 11.185 min Scan# 3155

Delta R.T. 0.006 min

Lab File: VV024572.D

Acq: 10 Feb 2022 16:52




Tgt Ion:146 Resp: 230


Ion Ratio Lower Upper

146 100

111 66.0 26.3 48.9#

148 0.0 44.4 82.5#


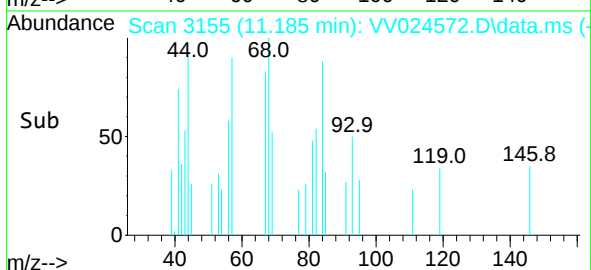

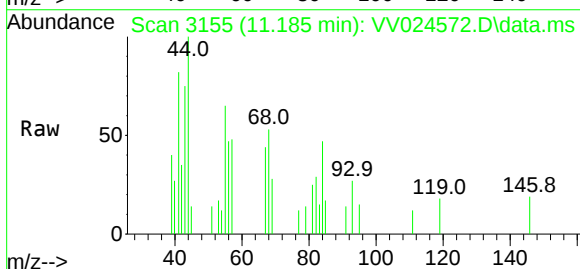




#65
1,4-Dichlorobenzene
Concen: 1.592 ug/L
RT: 11.278 min Scan# 3182
Delta R.T. 0.006 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52




Instrument :
MSVOA_V
ClientSampleId :


Tgt Ion:146 Resp: 492
Ion Ratio Lower Upper
146 100
111 35.7 25.6 47.6
148 69.2 44.8 83.2

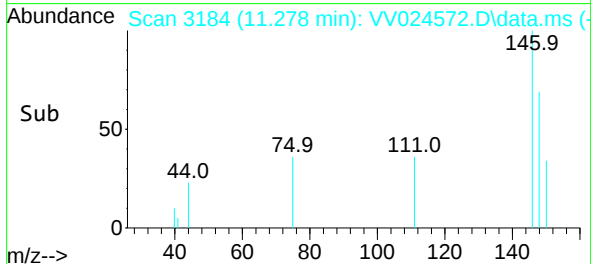

#67
1,2-Dichlorobenzene
Concen: 0.633 ug/L
RT: 11.644 min Scan# 3298
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Tgt Ion:146 Resp: 175
Ion Ratio Lower Upper
146 100
111 0.0 31.9 47.9#
148 0.0 50.5 75.7#

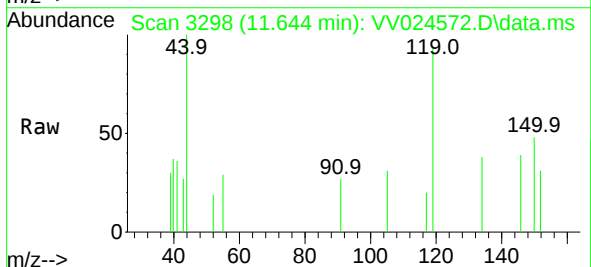



#69

1,3,5-Trichlorobenzene

Concen: 0.817 ug/L

RT: 12.644 min Scan# 3

Delta R.T. -0.000 min


Lab File: VV024572.D

Acq: 10 Feb 2022 16:52

Instrument :

MSVOA_V

ClientSampleId :

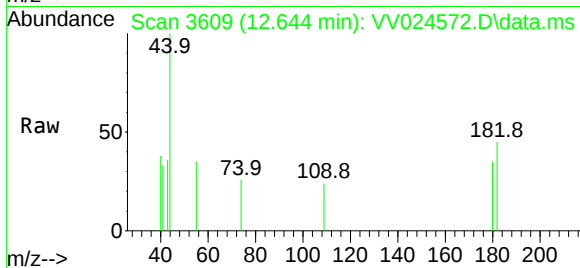

Tgt Ion:180 Resp: 181




Ion Ratio Lower Upper

180 100

182 114.9 76.4 114.6#

184 0.0 24.2 36.4#

145 0.0 23.2 34.8#

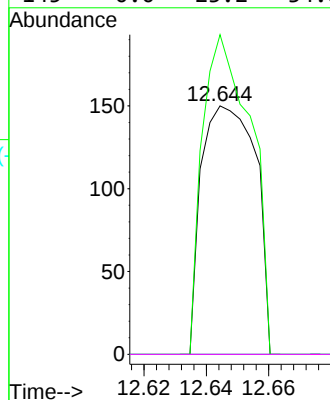

#70

1,2,4-trichlorobenzene

Concen: 1.622 ug/L

RT: 13.262 min Scan# 3801

Delta R.T. 0.003 min

Lab File: VV024572.D

Acq: 10 Feb 2022 16:52




Tgt Ion:180 Resp: 290


Ion Ratio Lower Upper

180 100

182 81.0 74.4 111.6


145 0.0 23.3 34.9#

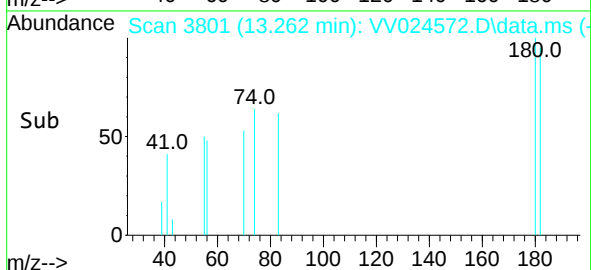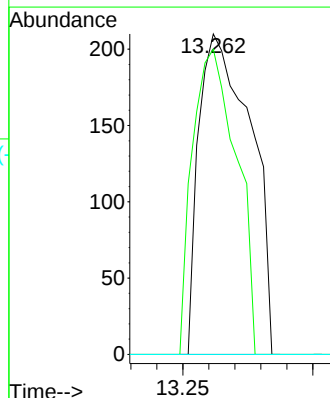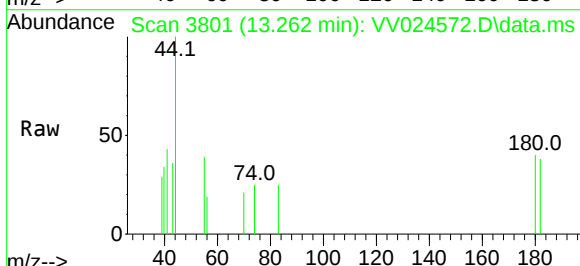






#71
Naphthalene
Concen: 6.342 ug/L
RT: 13.509 min Scan# 3875
Delta R.T. 0.010 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Instrument :
MSVOA_V
ClientSampleId :

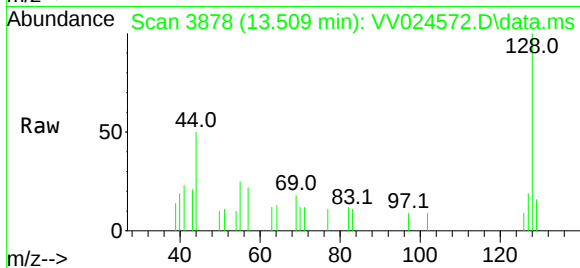

Tgt Ion:128 Resp: 2054
Ion Ratio Lower Upper
128 100
129 7.4 9.0 13.4#
127 7.5 10.2 15.4#

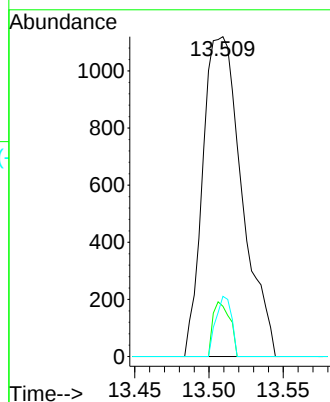

#72
1,2,3-Trichlorobenzene
Concen: 0.286 ug/L
RT: 13.744 min Scan# 3951
Delta R.T. 0.003 min
Lab File: VV024572.D
Acq: 10 Feb 2022 16:52

Tgt Ion:180 Resp: 43
Ion Ratio Lower Upper
180 100
182 95.3 76.8 115.2
145 0.0 25.8 38.6#

