




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024572.D
 Acq On : 10 Feb 2022 16:52
 Operator : SY/MD
 Sample : N1476-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXZ1

Manual IntegrationsAPPROVED

Quant Time: Feb 11 04:52:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 04:51:03 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
 Supervised By :Semsettin Yesilyurt 02/17/2022

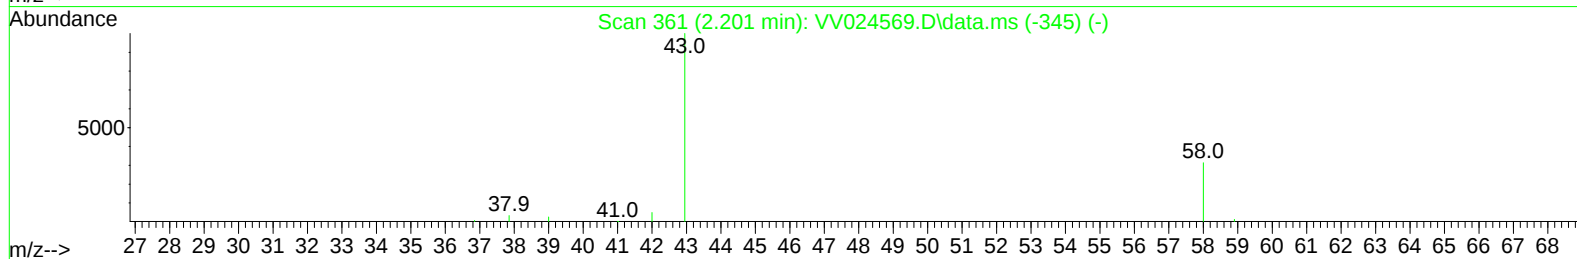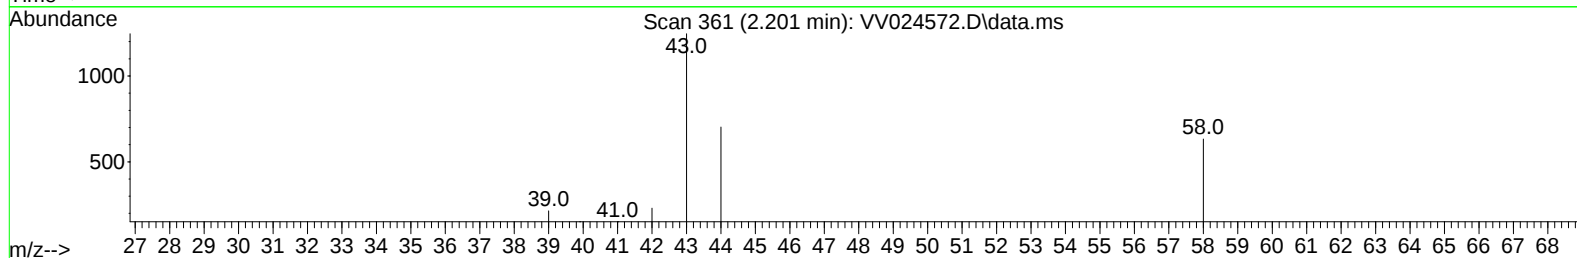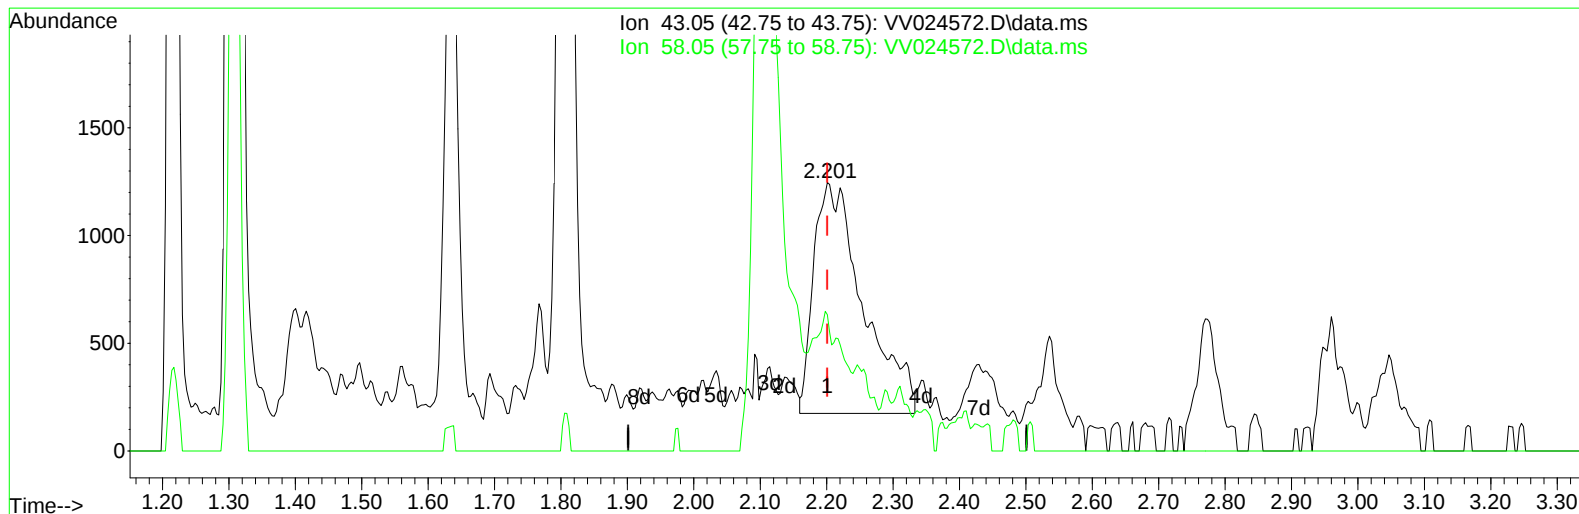

TIC: VV024572.D\data.ms

(13) Acetone (T)

2.201min (-0.000) 11745.00 ug/L m

response	5546	
Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	5.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024572.D
Acq On : 10 Feb 2022 16:52
Operator : SY/MD
Sample : N1476-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXZ1

Manual IntegrationsAPPROVED

Quant Time: Feb 11 04:52:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
Supervised By :Semsettin Yesilyurt 02/17/2022

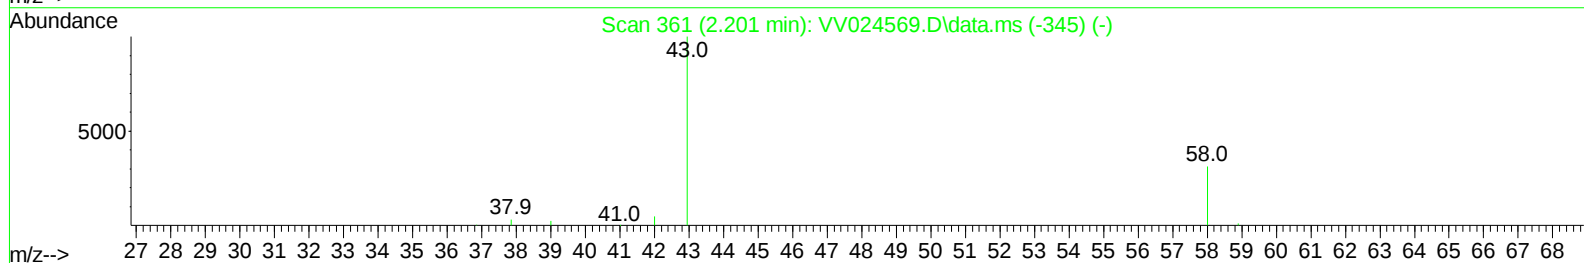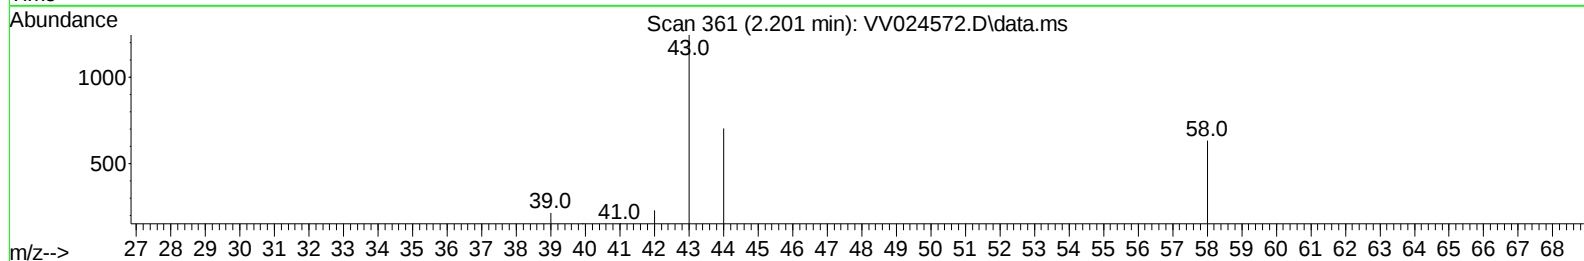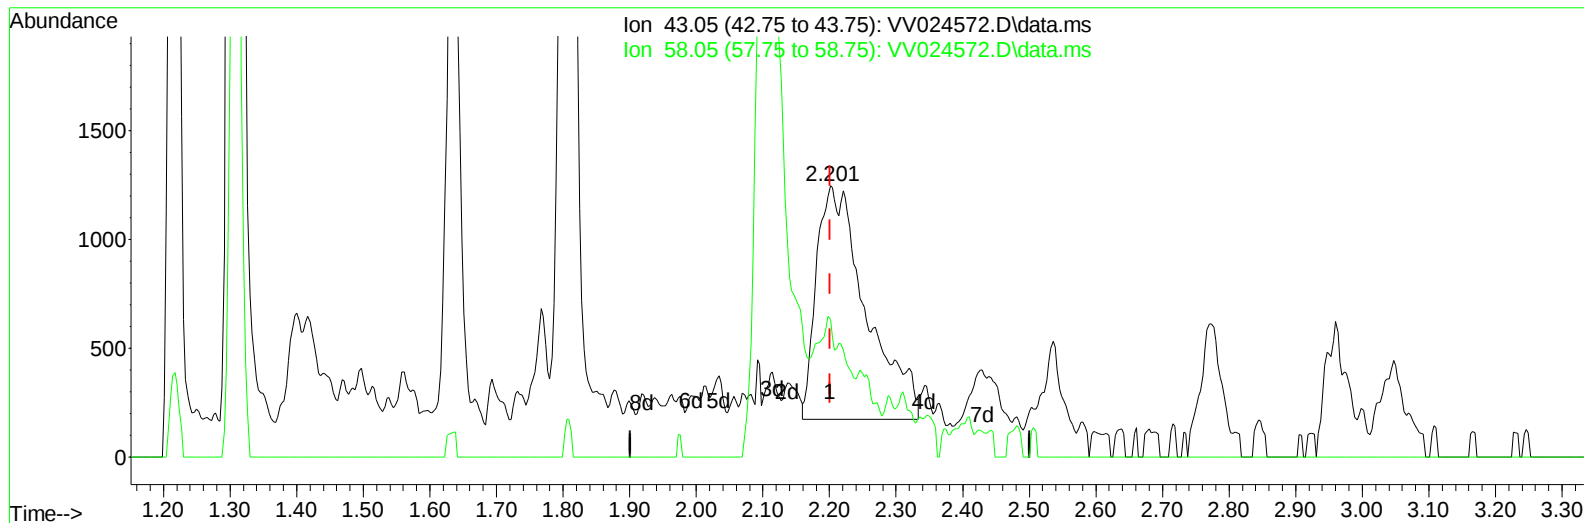

TIC: VV024572.D\data.ms

(13) Acetone (T)

2.201min (-0.000) 11745.00 ug/L m

response 5546

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.70	5.63
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
 Data File : VV024572.D
 Acq On : 10 Feb 2022 16:52
 Operator : SY/MD
 Sample : N1476-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXZ1

Manual IntegrationsAPPROVED

Quant Time: Feb 11 04:52:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Feb 11 04:51:03 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
 Supervised By :Semsettin Yesilyurt 02/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.654	114	43	5.000	ug/L	# 0.04
28) Chlorobenzene-d5	8.870	117	737	5.000	ug/L	# 0.02
58) 1,4-Dichlorobenzene-d4	11.255	152	843	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	69	19.143	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	= 382.800%	#	
7) Chloroethane-d5	1.548	69	76	24.941	ug/L	-0.02
Spiked Amount 5.000	Range 65	- 130	Recovery	= 498.800%	#	
11) 1,1-Dichloroethene-d2	2.111	63	437	55.428	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	= 1108.600%	#	
20) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount 50.000	Range 40	- 130	Recovery	= 0.000%	#	
24) Chloroform-d	4.371	84	42	6.621	ug/L	0.03
Spiked Amount 5.000	Range 70	- 125	Recovery	= 132.400%	#	
26) 1,2-Dichloroethane-d4	0.000	65	0	0.000	ug/L	
Spiked Amount 5.000	Range 70	- 130	Recovery	= 0.000%	#	
32) Benzene-d6	5.059	84	121	0.579	ug/L	0.01
Spiked Amount 5.000	Range 70	- 125	Recovery	= 11.600%	#	
36) 1,2-Dichloropropane-d6	5.928	67	186	2.860	ug/L	-0.14
41) Toluene-d8	7.336	98	360	1.846	ug/L	0.02
Spiked Amount 5.000	Range 70	- 130	Recovery	= 37.000%	#	
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount 5.000	Range 55	- 130	Recovery	= 0.000%	#	
46) 2-Hexanone-d5	8.236	63	228	24.640	ug/L	0.15
Spiked Amount 50.000	Range 45	- 130	Recovery	= 49.280%		
56) 1,1,2,2-Tetrachloroeth...	0.000	84	0	0.000	ug/L	
Spiked Amount 5.000	Range 65	- 120	Recovery	= 0.000%	#	
66) 1,2-Dichlorobenzene-d4	11.635	152	604	4.445	ug/L	0.01
Spiked Amount 5.000	Range 80	- 120	Recovery	= 88.800%		
Target Compounds						
					Qvalue	
13) Acetone	2.201	43	5167m	10942.377	ug/L	
14) Carbon disulfide	2.298	76	594	41.978	ug/L #	54
17) Methyl tert-butyl Ether	2.770	73	4308	469.561	ug/L #	87
25) Chloroform	4.384	83	4549	575.353	ug/L	92
33) Benzene	5.114	78	4658	16.194	ug/L	100
42) Toluene	7.394	91	11194	35.725	ug/L	92
47) Tetrachloroethene	7.976	164	162562	3093.706	ug/L	91
52) Ethylbenzene	9.018	91	7031	20.167	ug/L	100
53) m,p-xylene	9.140	106	6147	46.547	ug/L	91
54) o-xylene	9.548	106	2795	21.949	ug/L	94
62) 1,3,5-Trimethylbenzene	10.542	105	2939	4.489	ug/L	91
63) 1,2,4-Trimethylbenzene	10.915	105	9030	13.873	ug/L	98
65) 1,4-Dichlorobenzene	11.278	146	492	1.592	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV021022\
Data File : VV024572.D
Acq On : 10 Feb 2022 16:52
Operator : SY/MD
Sample : N1476-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXZ1

Manual IntegrationsAPPROVED

Quant Time: Feb 11 04:52:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR020922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Feb 11 04:51:03 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/15/2022
Supervised By :Semsettin Yesilyurt 02/17/2022

